

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045267.D
 Acq On : 16 Apr 2024 05:55
 Operator : MA/JU
 Sample : P2051-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	20	rVB	8677	10854	0.62%	0.077%
2	3.381	48	50	53	rBV3	2170	2393	0.14%	0.017%
3	3.593	82	86	97	rBV	21762	47479	2.72%	0.338%
4	3.863	130	132	136	rVB5	3471	3669	0.21%	0.026%
5	4.399	221	223	225	rBV3	1623	1843	0.11%	0.013%
6	4.646	263	265	270	rBV6	1338	1899	0.11%	0.014%
7	5.593	425	426	432	rBV5	1128	1865	0.11%	0.013%
8	6.440	568	570	574	rVB4	1386	2094	0.12%	0.015%
9	6.775	621	627	636	rBV2	27796	59444	3.40%	0.423%
10	6.869	640	643	646	rVB4	1850	2007	0.11%	0.014%
11	6.940	648	655	665	rBV	182334	303129	17.36%	2.156%
12	7.116	677	685	700	rBV	161393	281493	16.12%	2.002%
13	7.581	757	764	774	rBV	222264	363342	20.81%	2.584%
14	7.763	794	795	799	rBV3	1712	1902	0.11%	0.014%
15	7.993	830	834	836	rBV4	1846	1887	0.11%	0.013%
16	8.293	879	885	897	rBV	101895	183954	10.53%	1.308%
17	8.745	955	962	974	rBV	209465	364994	20.90%	2.596%
18	9.098	1019	1022	1024	rBV4	1553	1830	0.10%	0.013%
19	9.210	1038	1041	1044	rBV3	1037	1773	0.10%	0.013%
20	9.457	1074	1083	1093	rBV	161018	288759	16.54%	2.053%
21	9.987	1166	1173	1189	rBV	196389	392522	22.48%	2.791%
22	10.351	1228	1235	1244	rVB	291693	486586	27.86%	3.460%
23	10.516	1257	1263	1283	rBV	123607	306261	17.54%	2.178%
24	10.663	1286	1288	1293	rVB5	1211	1774	0.10%	0.013%
25	11.081	1353	1359	1363	rBV5	2733	5038	0.29%	0.036%
26	11.981	1508	1512	1519	rBV4	3198	6095	0.35%	0.043%
27	12.757	1637	1644	1650	rVB2	6345	11143	0.64%	0.079%
28	13.128	1704	1707	1711	rVB3	2709	3742	0.21%	0.027%
29	13.551	1774	1779	1782	rVB4	1070	1781	0.10%	0.013%
30	13.663	1788	1798	1809	rBV	484290	720707	41.27%	5.125%
31	13.922	1832	1842	1853	rBV	576709	855378	48.98%	6.083%
32	14.233	1888	1895	1903	rBV	429073	636574	36.45%	4.527%
33	14.539	1937	1947	1948	rBV7	7284	17595	1.01%	0.125%
34	14.580	1952	1954	1957	rVB4	1926	2214	0.13%	0.016%
35	14.686	1970	1972	1976	rVB4	2447	2404	0.14%	0.017%
36	15.010	2024	2027	2030	rVB3	2513	2750	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045267.D
 Acq On : 16 Apr 2024 05:55
 Operator : MA/JU
 Sample : P2051-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.233	2059	2065	2080	rVB	759166	1100266	63.01%	7.824%
38	15.380	2083	2090	2100	rBV	189270	301834	17.28%	2.146%
39	15.480	2104	2107	2111	rVB5	3467	4893	0.28%	0.035%
40	15.886	2172	2176	2181	rVB4	5467	8251	0.47%	0.059%
41	16.027	2197	2200	2204	rVB5	2430	2931	0.17%	0.021%
42	16.421	2265	2267	2270	rVB3	2177	1909	0.11%	0.014%
43	16.621	2299	2301	2307	rVB	1516	2231	0.13%	0.016%
44	16.933	2347	2354	2356	rVV4	4323	5413	0.31%	0.038%
45	16.992	2358	2364	2372	rVV	541562	726935	41.63%	5.169%
46	17.092	2375	2381	2396	rVV2	845937	1264431	72.41%	8.991%
47	17.192	2396	2398	2401	rVV3	2573	2814	0.16%	0.020%
48	17.392	2429	2432	2433	rBV2	2322	2274	0.13%	0.016%
49	17.774	2494	2497	2501	rBV4	2292	3146	0.18%	0.022%
50	17.904	2514	2519	2529	rBV3	38096	60423	3.46%	0.430%
51	17.968	2529	2530	2534	rVV4	1988	2766	0.16%	0.020%
52	18.339	2588	2593	2597	rBV7	3146	4660	0.27%	0.033%
53	18.774	2664	2667	2671	rBV6	5191	8275	0.47%	0.059%
54	18.962	2695	2699	2705	rVB3	8053	10226	0.59%	0.073%
55	19.039	2708	2712	2715	rBV3	7061	9965	0.57%	0.071%
56	19.074	2715	2718	2721	rVB5	2419	3831	0.22%	0.027%
57	19.198	2735	2739	2744	rBV3	18761	26443	1.51%	0.188%
58	19.321	2758	2760	2762	rBV3	2123	1981	0.11%	0.014%
59	19.398	2767	2773	2782	rBV	1031638	1423810	81.54%	10.125%
60	19.609	2806	2809	2810	rBV3	2756	2826	0.16%	0.020%
61	19.757	2831	2834	2835	rBV3	2750	2781	0.16%	0.020%
62	20.933	3030	3034	3041	rBV7	26198	50203	2.87%	0.357%
63	21.203	3075	3080	3093	rBV	568748	829102	47.48%	5.896%
64	22.380	3277	3280	3286	rVB	62767	86777	4.97%	0.617%
65	23.268	3424	3431	3437	rBV	963921	1746244	100.00%	12.418%
66	23.403	3448	3454	3468	rVB	520850	985752	56.45%	7.010%




Sum of corrected areas: 14062567

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045267.D
Acq On : 16 Apr 2024 05:55
Operator : MA/JU
Sample : P2051-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

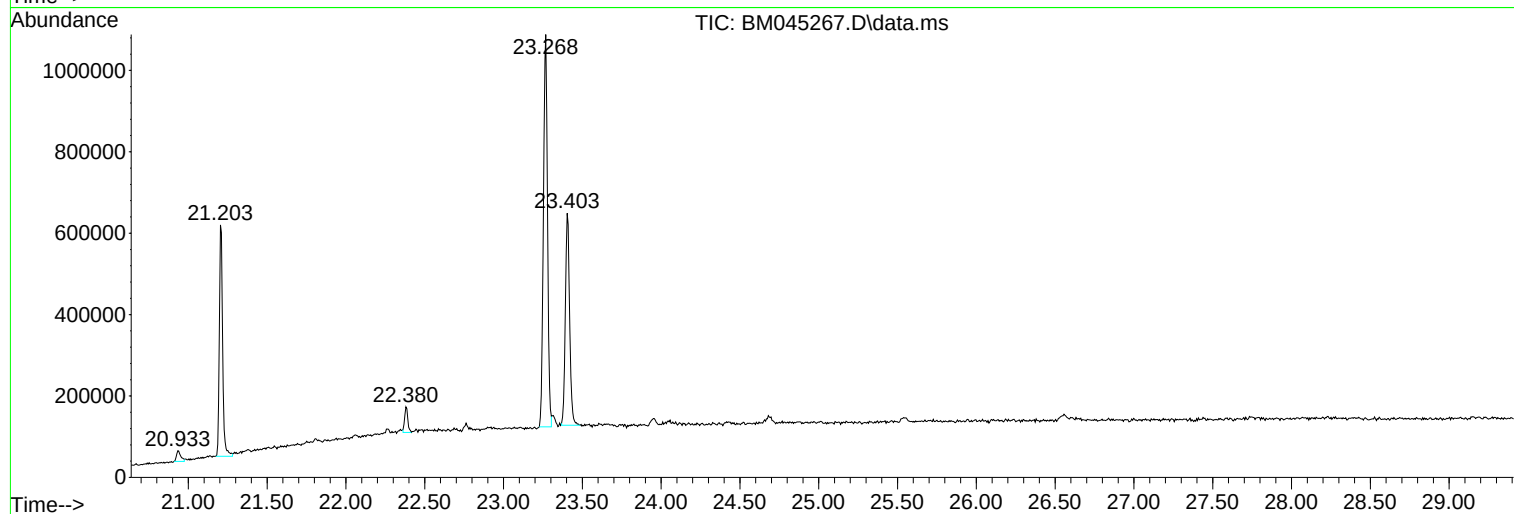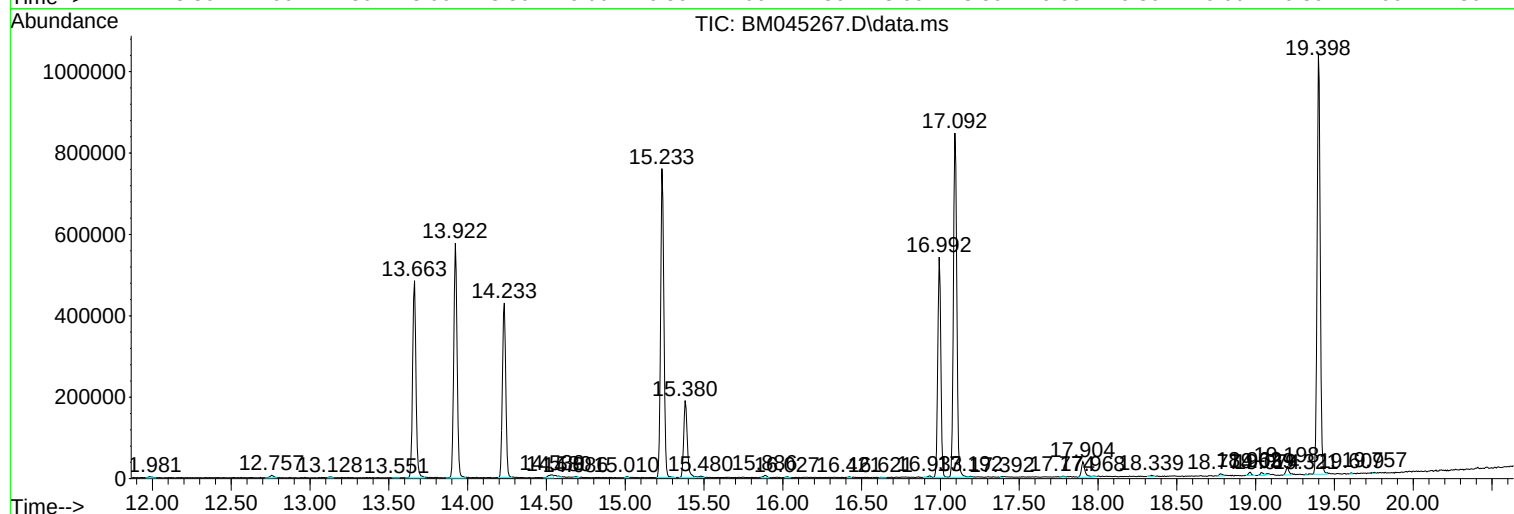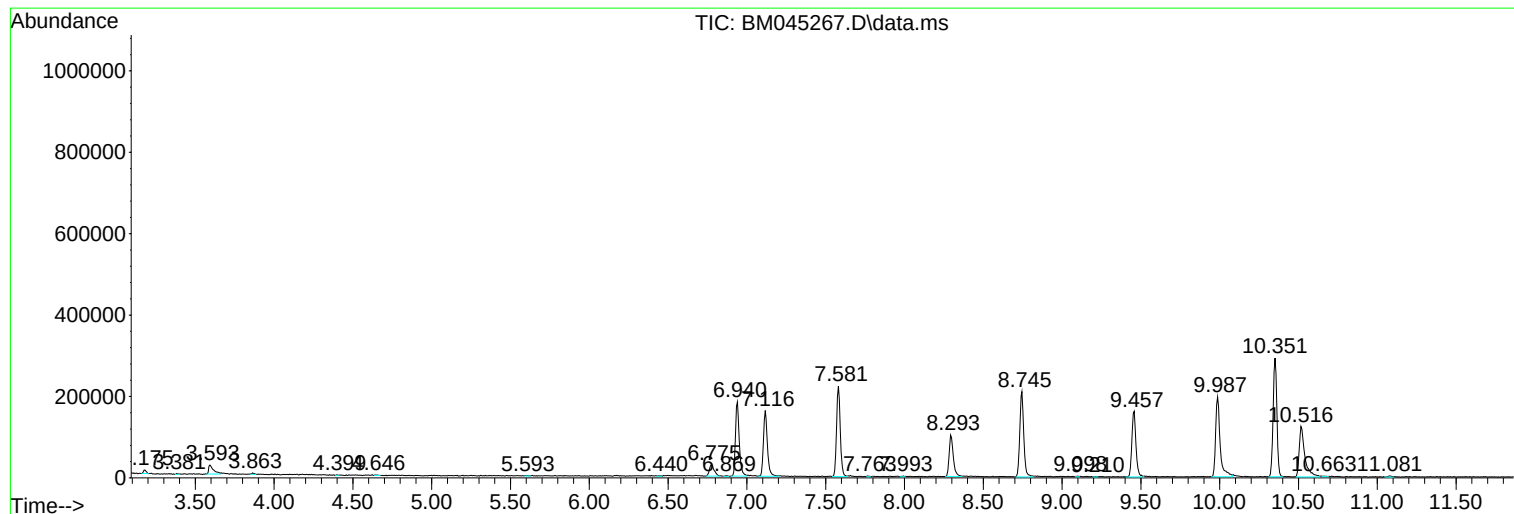

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045267.D
Acq On : 16 Apr 2024 05:55
Operator : MA/JU
Sample : P2051-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045267.D
Acq On : 16 Apr 2024 05:55
Operator : MA/JU
Sample : P2051-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc