

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045268.D
 Acq On : 16 Apr 2024 06:31
 Operator : MA/JU
 Sample : P2051-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rBV	8735	11714	0.66%	0.081%
2	3.593	81	86	94	rBV	16304	35811	2.02%	0.247%
3	3.675	98	100	103	rVB3	2495	1877	0.11%	0.013%
4	3.751	111	113	117	rBV5	1541	2070	0.12%	0.014%
5	3.816	123	124	128	rBV3	2317	2687	0.15%	0.019%
6	3.869	130	133	137	rVB4	4694	6260	0.35%	0.043%
7	4.916	307	311	312	rBV4	1742	2069	0.12%	0.014%
8	5.922	478	482	484	rVB4	1483	1980	0.11%	0.014%
9	5.987	491	493	498	rVB5	1469	2146	0.12%	0.015%
10	6.569	590	592	595	rBV4	1569	2226	0.13%	0.015%
11	6.775	618	627	636	rBV	34714	70344	3.96%	0.485%
12	6.939	646	655	667	rBV	195502	323705	18.23%	2.231%
13	7.116	676	685	694	rBV	176359	304007	17.12%	2.096%
14	7.269	708	711	714	rBV4	1510	2509	0.14%	0.017%
15	7.581	757	764	772	rBV	237487	379555	21.38%	2.616%
16	8.292	880	885	897	rBV	115718	206730	11.64%	1.425%
17	8.745	955	962	973	rBV	217752	375742	21.16%	2.590%
18	8.822	973	975	978	rVB4	1514	1848	0.10%	0.013%
19	9.451	1075	1082	1094	rBV	176147	312779	17.62%	2.156%
20	9.528	1094	1095	1105	rVB4	1494	2964	0.17%	0.020%
21	9.986	1167	1173	1191	rBV	205617	418351	23.56%	2.884%
22	10.351	1228	1235	1244	rBV	309979	510570	28.76%	3.519%
23	10.516	1256	1263	1283	rBV	100421	258265	14.55%	1.780%
24	10.686	1288	1292	1295	rVV3	1433	2297	0.13%	0.016%
25	10.951	1334	1337	1341	rBV4	1560	2266	0.13%	0.016%
26	11.080	1353	1359	1364	rVB4	5231	9734	0.55%	0.067%
27	11.980	1507	1512	1522	rVB7	3339	7674	0.43%	0.053%
28	12.751	1637	1643	1651	rVB2	12796	22689	1.28%	0.156%
29	13.086	1696	1700	1703	rBV5	1934	2893	0.16%	0.020%
30	13.663	1792	1798	1807	rBV	501343	728117	41.01%	5.019%
31	13.921	1836	1842	1851	rBV2	583771	855423	48.18%	5.896%
32	13.986	1851	1853	1857	rVV5	2258	2460	0.14%	0.017%
33	14.233	1888	1895	1905	rVV	460761	671709	37.84%	4.630%
34	14.521	1938	1944	1947	rBV5	7316	15860	0.89%	0.109%
35	15.074	2035	2038	2042	rBV3	1467	2676	0.15%	0.018%
36	15.233	2057	2065	2074	rBV	762783	1111628	62.61%	7.662%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045268.D
 Acq On : 16 Apr 2024 06:31
 Operator : MA/JU
 Sample : P2051-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.380	2084	2090	2102	rBV	217179	332972	18.76%	2.295%
38	15.492	2106	2109	2110	rVB2	2700	2710	0.15%	0.019%
39	15.886	2172	2176	2184	rVB	10573	16809	0.95%	0.116%
40	16.027	2195	2200	2206	rBV4	2417	3963	0.22%	0.027%
41	16.421	2265	2267	2271	rBV3	1960	1916	0.11%	0.013%
42	16.762	2320	2325	2326	rBV4	1571	2199	0.12%	0.015%
43	16.933	2350	2354	2357	rBV5	5382	6966	0.39%	0.048%
44	16.992	2358	2364	2374	rVV	588204	778330	43.84%	5.365%
45	17.092	2374	2381	2396	rVV2	867228	1288326	72.57%	8.880%
46	17.186	2396	2397	2403	rVB5	2296	2617	0.15%	0.018%
47	17.398	2430	2433	2438	rVB6	2043	3069	0.17%	0.021%
48	17.903	2513	2519	2531	rBV2	29643	49397	2.78%	0.340%
49	18.345	2588	2594	2596	rBV5	3598	5162	0.29%	0.036%
50	18.668	2645	2649	2650	rBV4	1930	1891	0.11%	0.013%
51	18.780	2664	2668	2672	rBV5	5386	11559	0.65%	0.080%
52	18.962	2696	2699	2705	rVB5	8368	11938	0.67%	0.082%
53	19.039	2708	2712	2715	rBV2	7134	10363	0.58%	0.071%
54	19.198	2735	2739	2745	rBV5	15330	24163	1.36%	0.167%
55	19.398	2767	2773	2785	rBV	1049024	1476265	83.15%	10.176%
56	19.962	2868	2869	2872	rBV3	2769	3268	0.18%	0.023%
57	20.409	2943	2945	2947	rBV3	5129	5414	0.30%	0.037%
58	20.933	3030	3034	3039	rBV8	20420	34095	1.92%	0.235%
59	21.203	3075	3080	3088	rBV	625091	862459	48.58%	5.945%
60	22.386	3277	3281	3289	rVB2	56355	81945	4.62%	0.565%
61	23.268	3424	3431	3437	rBV	991685	1775340	100.00%	12.237%
62	23.403	3448	3454	3466	rVB	548315	1042622	58.73%	7.187%




Sum of corrected areas: 14507393

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045268.D
Acq On : 16 Apr 2024 06:31
Operator : MA/JU
Sample : P2051-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

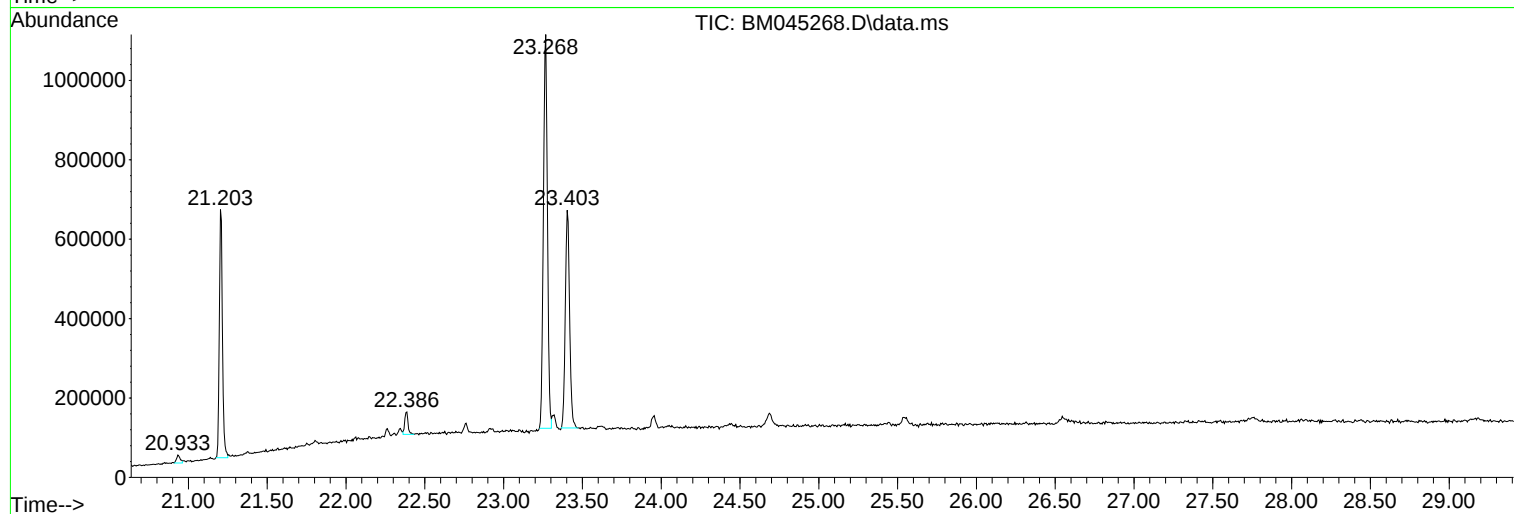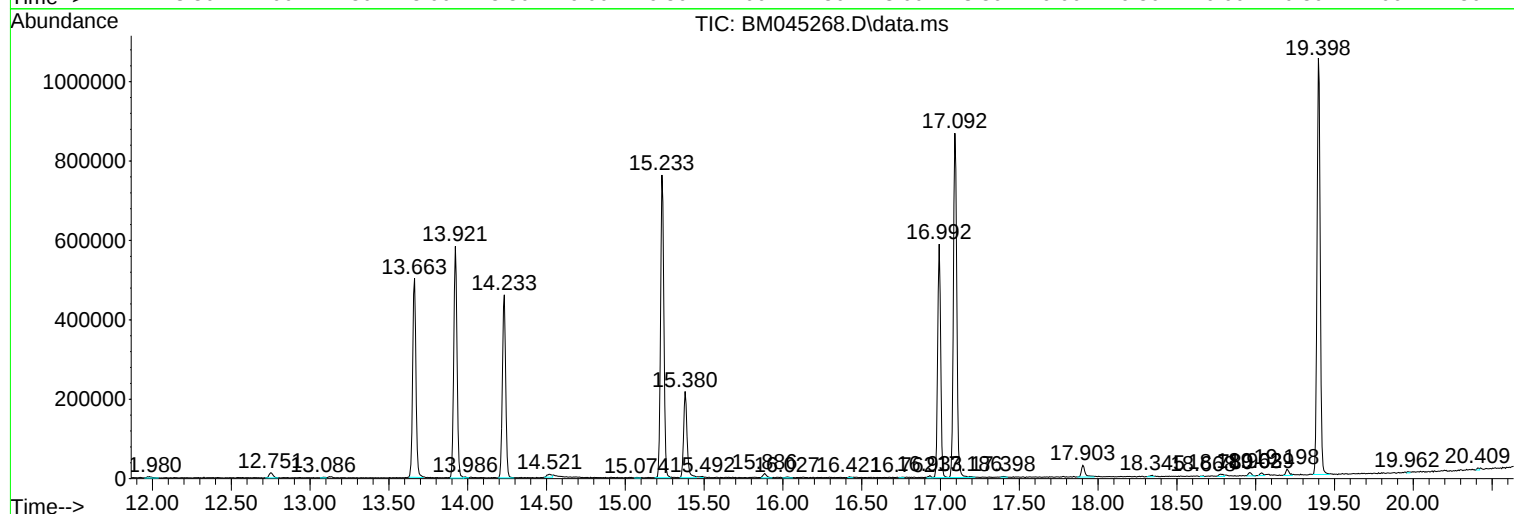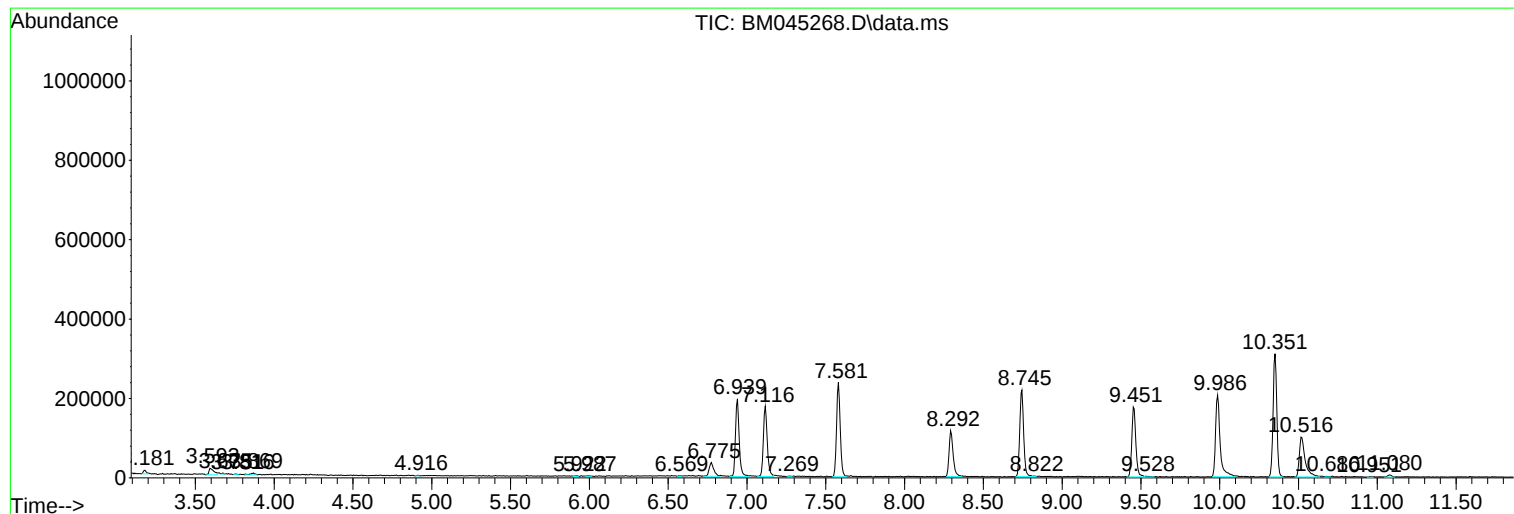

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045268.D
Acq On : 16 Apr 2024 06:31
Operator : MA/JU
Sample : P2051-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045268.D
Acq On : 16 Apr 2024 06:31
Operator : MA/JU
Sample : P2051-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc