

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045278.D
 Acq On : 16 Apr 2024 13:13
 Operator : MA/JU
 Sample : PB160223BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	22	rVB	15937	22232	1.58%	0.152%
2	3.234	22	25	26	rBV3	2033	2080	0.15%	0.014%
3	3.446	59	61	64	rVB4	1924	1700	0.12%	0.012%
4	3.575	80	83	107	rBV	160070	299722	21.30%	2.054%
5	3.863	130	132	138	rVB3	4776	7721	0.55%	0.053%
6	3.975	149	151	154	rBV3	1672	2329	0.17%	0.016%
7	4.016	157	158	161	rBV3	1568	1676	0.12%	0.011%
8	4.140	177	179	181	rBV3	2322	1857	0.13%	0.013%
9	4.640	261	264	267	rVB5	1634	2075	0.15%	0.014%
10	4.693	272	273	277	rBV4	1690	2092	0.15%	0.014%
11	4.904	307	309	312	rVB3	1735	1595	0.11%	0.011%
12	4.957	312	318	319	rBV5	1168	1890	0.13%	0.013%
13	5.057	333	335	337	rBV2	1659	1474	0.10%	0.010%
14	5.681	436	441	445	rBV6	1560	2616	0.19%	0.018%
15	5.769	454	456	457	rBV2	1676	1528	0.11%	0.010%
16	5.857	469	471	474	rVB3	1643	1651	0.12%	0.011%
17	5.892	474	477	479	rBV3	1356	1457	0.10%	0.010%
18	6.404	561	564	566	rVB3	1572	1843	0.13%	0.013%
19	6.422	566	567	569	rBV2	1678	1431	0.10%	0.010%
20	6.763	619	625	638	rBV	213812	377635	26.84%	2.588%
21	6.939	648	655	666	rBV	187271	310187	22.05%	2.126%
22	7.116	678	685	695	rBV	241010	399420	28.39%	2.738%
23	7.186	695	697	702	rVB4	2225	2885	0.21%	0.020%
24	7.334	717	722	724	rBV5	1587	1719	0.12%	0.012%
25	7.581	757	764	772	rVV	245834	395877	28.14%	2.713%
26	8.069	843	847	848	rBV3	1853	2241	0.16%	0.015%
27	8.292	878	885	899	rBV	257028	459265	32.64%	3.148%
28	8.433	907	909	913	rBV4	1287	1813	0.13%	0.012%
29	8.604	934	938	941	rBV4	1426	2364	0.17%	0.016%
30	8.745	955	962	975	rBV	214965	376006	26.72%	2.577%
31	8.933	991	994	996	rVB4	1277	1484	0.11%	0.010%
32	8.963	996	999	1001	rBV2	1471	1429	0.10%	0.010%
33	9.451	1073	1082	1093	rBV	182161	325037	23.10%	2.228%
34	9.527	1093	1095	1098	rVV3	2257	2222	0.16%	0.015%
35	9.669	1116	1119	1124	rVB4	1083	2191	0.16%	0.015%
36	9.986	1166	1173	1192	rBV	234841	460469	32.73%	3.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045278.D
 Acq On : 16 Apr 2024 13:13
 Operator : MA/JU
 Sample : PB160223BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.351	1227	1235	1244	rVV	312058	534335	37.98%	3.663%
38	10.516	1256	1263	1281	rBV	194740	466366	33.15%	3.197%
39	11.674	1457	1460	1464	rVB4	1664	1941	0.14%	0.013%
40	11.716	1464	1467	1470	rBV4	1312	1439	0.10%	0.010%
41	11.986	1509	1513	1519	rVB6	2607	5592	0.40%	0.038%
42	13.133	1703	1708	1714	rVB6	2564	4523	0.32%	0.031%
43	13.663	1791	1798	1810	rVV	449296	697681	49.59%	4.782%
44	13.921	1833	1842	1854	rBV	548372	838737	59.61%	5.749%
45	14.015	1857	1858	1863	rVB3	1809	1615	0.11%	0.011%
46	14.233	1888	1895	1903	rBV	452546	684119	48.62%	4.689%
47	14.374	1915	1919	1925	rBV5	1711	2770	0.20%	0.019%
48	14.474	1928	1936	1959	rBV2	96726	275505	19.58%	1.888%
49	14.780	1985	1988	1991	rVB3	1296	1550	0.11%	0.011%
50	14.921	2007	2012	2013	rBV3	1194	1488	0.11%	0.010%
51	15.233	2059	2065	2076	rVV	670275	1012525	71.96%	6.940%
52	15.380	2085	2090	2100	rBV	166754	268919	19.11%	1.843%
53	15.480	2104	2107	2110	rVB4	2724	3078	0.22%	0.021%
54	15.557	2117	2120	2123	rVB5	1462	1898	0.13%	0.013%
55	15.792	2156	2160	2161	rBV2	1360	1683	0.12%	0.012%
56	15.833	2165	2167	2171	rVV3	1244	1604	0.11%	0.011%
57	16.027	2196	2200	2203	rVB4	2035	2140	0.15%	0.015%
58	16.351	2252	2255	2257	rBV2	1143	1465	0.10%	0.010%
59	16.409	2263	2265	2270	rVB2	1181	1566	0.11%	0.011%
60	16.451	2270	2272	2276	rBV3	1295	1806	0.13%	0.012%
61	16.768	2321	2326	2327	rBV3	1186	1560	0.11%	0.011%
62	16.992	2358	2364	2372	rBV	559077	768111	54.59%	5.265%
63	17.092	2375	2381	2395	rVV2	686643	1061589	75.45%	7.276%
64	17.527	2451	2455	2457	rVV5	1572	1830	0.13%	0.013%
65	17.603	2464	2468	2471	rVB3	1373	1840	0.13%	0.013%
66	17.627	2471	2472	2476	rBV4	1017	1421	0.10%	0.010%
67	17.945	2524	2526	2528	rBV3	2049	1824	0.13%	0.013%
68	18.021	2537	2539	2542	rBV3	1707	1919	0.14%	0.013%
69	18.362	2595	2597	2598	rBV2	1736	1420	0.10%	0.010%
70	18.668	2648	2649	2653	rBV2	1578	2407	0.17%	0.016%
71	18.833	2673	2677	2681	rVB7	1791	2887	0.21%	0.020%
72	18.880	2681	2685	2686	rBV4	1335	2009	0.14%	0.014%
73	18.962	2696	2699	2705	rVV6	8091	11114	0.79%	0.076%
74	19.039	2709	2712	2716	rVV2	5078	5703	0.41%	0.039%
75	19.186	2736	2737	2740	rBV3	1736	1829	0.13%	0.013%
76	19.297	2753	2756	2757	rBV3	1564	1961	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045278.D
Acq On : 16 Apr 2024 13:13
Operator : MA/JU
Sample : PB160223BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	19.403	2767	2774	2786	rBV	819786	1191902	84.71%	8.170%
78	19.539	2795	2797	2801	rBV5	2109	2525	0.18%	0.017%
79	19.709	2824	2826	2828	rBV2	2817	2463	0.18%	0.017%
80	19.944	2864	2866	2868	rBV3	2907	2731	0.19%	0.019%
81	20.592	2974	2976	2977	rBV2	3830	2427	0.17%	0.017%
82	21.209	3075	3081	3092	rBV	571674	836173	59.43%	5.731%
83	23.268	3424	3431	3437	rBV2	766045	1407013	100.00%	9.644%
84	23.403	3448	3454	3468	rVB	506762	979114	69.59%	6.711%




Sum of corrected areas: 14589330

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045278.D
Acq On : 16 Apr 2024 13:13
Operator : MA/JU
Sample : PB160223BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

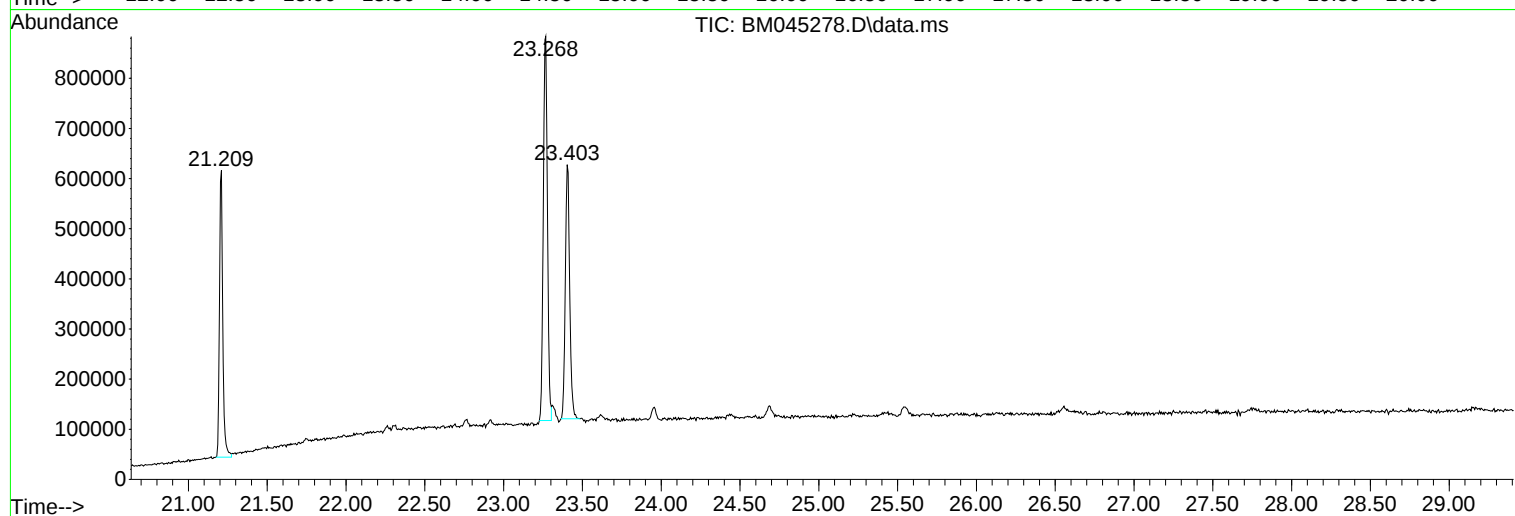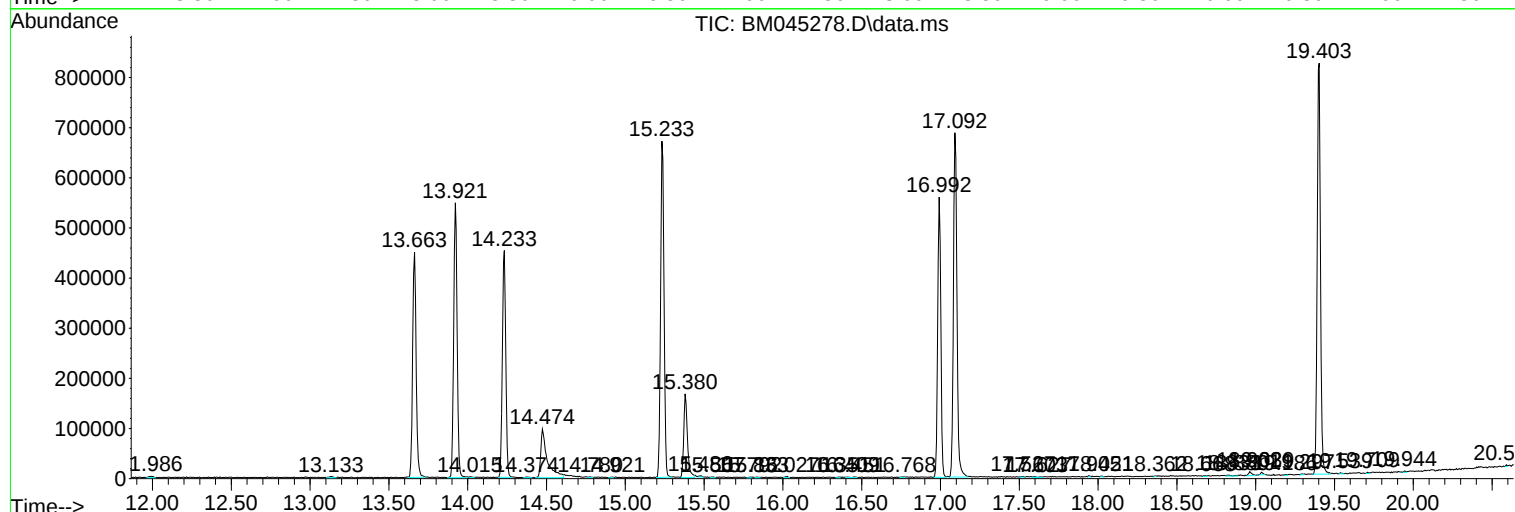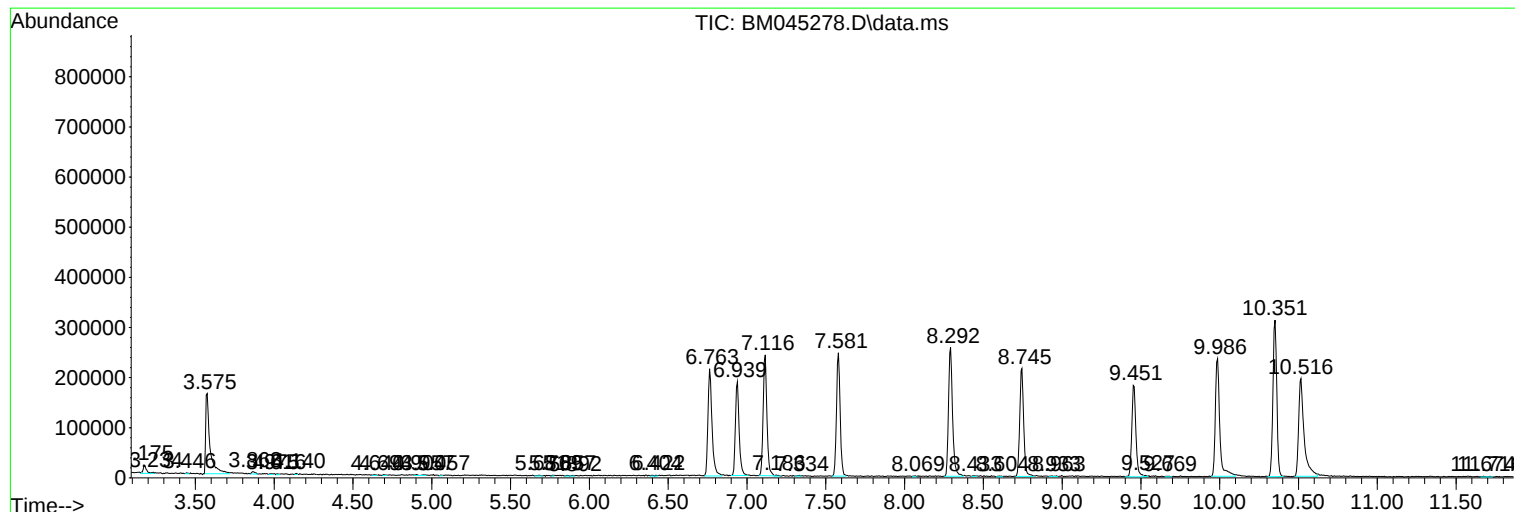

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045278.D
Acq On : 16 Apr 2024 13:13
Operator : MA/JU
Sample : PB160223BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045278.D
Acq On : 16 Apr 2024 13:13
Operator : MA/JU
Sample : PB160223BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------