

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045279.D
 Acq On : 16 Apr 2024 13:50
 Operator : MA/JU
 Sample : PB160225BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	21	rVB	13386	17291	1.18%	0.117%
2	3.287	32	34	37	rVB3	2220	2180	0.15%	0.015%
3	3.328	40	41	44	rBV3	1829	1575	0.11%	0.011%
4	3.357	44	46	50	rVB5	2146	2768	0.19%	0.019%
5	3.393	50	52	54	rBV3	1986	1849	0.13%	0.013%
6	3.534	75	76	80	rBV3	2428	2776	0.19%	0.019%
7	3.575	80	83	99	rBV	155786	285304	19.50%	1.931%
8	3.869	129	133	135	rVB5	4134	4658	0.32%	0.032%
9	4.163	181	183	187	rVB4	2130	2161	0.15%	0.015%
10	4.281	202	203	206	rBV3	1532	1699	0.12%	0.012%
11	5.351	383	385	388	rVB4	1709	1774	0.12%	0.012%
12	5.710	443	446	449	rVB3	1390	1671	0.11%	0.011%
13	6.228	530	534	538	rVB5	1590	2753	0.19%	0.019%
14	6.634	601	603	608	rVB5	1583	2275	0.16%	0.015%
15	6.763	619	625	637	rBV	214699	381469	26.07%	2.582%
16	6.939	649	655	666	rBV	188402	317632	21.71%	2.150%
17	7.045	671	673	677	rVB4	1811	1719	0.12%	0.012%
18	7.116	677	685	698	rBV	240663	404737	27.66%	2.740%
19	7.581	757	764	775	rBV	248323	398598	27.24%	2.698%
20	7.710	781	786	788	rBV3	1614	2216	0.15%	0.015%
21	7.992	828	834	835	rBV2	1206	1504	0.10%	0.010%
22	8.163	859	863	865	rBV5	1235	1487	0.10%	0.010%
23	8.292	878	885	897	rVV	261656	466761	31.90%	3.159%
24	8.398	901	903	906	rVV4	1895	2313	0.16%	0.016%
25	8.745	954	962	977	rBV	213529	379885	25.96%	2.571%
26	8.910	986	990	991	rBV3	1425	1718	0.12%	0.012%
27	9.457	1074	1083	1097	rBV	181752	326597	22.32%	2.211%
28	9.775	1133	1137	1139	rVB4	1275	1636	0.11%	0.011%
29	9.810	1139	1143	1144	rBV3	1095	1465	0.10%	0.010%
30	9.986	1166	1173	1202	rBV	240881	487929	33.35%	3.303%
31	10.351	1227	1235	1243	rBV	319500	533450	36.46%	3.611%
32	10.516	1256	1263	1281	rBV2	192094	475271	32.48%	3.217%
33	10.857	1319	1321	1324	rBV4	1883	1979	0.14%	0.013%
34	11.998	1509	1515	1516	rBV4	2326	3667	0.25%	0.025%
35	12.027	1516	1520	1523	rVB5	1345	1945	0.13%	0.013%
36	12.580	1609	1614	1618	rVB4	1305	2469	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045279.D
 Acq On : 16 Apr 2024 13:50
 Operator : MA/JU
 Sample : PB160225BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	12.621	1618	1621	1622	rBV2	1478	1739	0.12%	0.012%
38	13.086	1697	1700	1703	rBV2	1141	1646	0.11%	0.011%
39	13.127	1703	1707	1712	rVB5	3464	6472	0.44%	0.044%
40	13.263	1724	1730	1732	rBV4	1077	1947	0.13%	0.013%
41	13.663	1791	1798	1812	rBV	458220	704196	48.13%	4.767%
42	13.815	1820	1824	1826	rBV2	1641	2175	0.15%	0.015%
43	13.921	1834	1842	1852	rBV	569943	842729	57.60%	5.704%
44	13.986	1852	1853	1860	rVB4	1986	1887	0.13%	0.013%
45	14.233	1888	1895	1903	rBV	455432	679082	46.41%	4.597%
46	14.315	1906	1909	1913	rVB2	1330	1475	0.10%	0.010%
47	14.474	1929	1936	1953	rBV	100388	262986	17.97%	1.780%
48	14.751	1979	1983	1984	rBV2	1426	1648	0.11%	0.011%
49	14.774	1984	1987	1988	rVB2	1624	1579	0.11%	0.011%
50	14.792	1988	1990	1992	rBV2	1446	1607	0.11%	0.011%
51	14.862	1999	2002	2007	rVB4	898	1492	0.10%	0.010%
52	15.233	2058	2065	2074	rBV	679117	1029944	70.39%	6.972%
53	15.380	2085	2090	2103	rBV	176538	278487	19.03%	1.885%
54	15.480	2106	2107	2111	rVV3	2848	3287	0.22%	0.022%
55	15.815	2160	2164	2166	rVB4	1381	1575	0.11%	0.011%
56	16.021	2197	2199	2202	rVB4	1743	1698	0.12%	0.011%
57	16.715	2313	2317	2318	rBV2	1197	1466	0.10%	0.010%
58	16.780	2325	2328	2329	rBV3	1771	1546	0.11%	0.010%
59	16.992	2358	2364	2375	rBV	574437	767033	52.42%	5.192%
60	17.092	2375	2381	2396	rVV	725739	1081359	73.91%	7.320%
61	17.539	2452	2457	2459	rBV4	1218	1615	0.11%	0.011%
62	17.698	2482	2484	2489	rVB3	1242	1891	0.13%	0.013%
63	17.927	2519	2523	2526	rBV2	1712	2463	0.17%	0.017%
64	17.992	2531	2534	2536	rVB3	1633	1543	0.11%	0.010%
65	18.068	2545	2547	2549	rBV3	1480	1585	0.11%	0.011%
66	18.692	2650	2653	2654	rBV3	1774	1642	0.11%	0.011%
67	18.968	2696	2700	2703	rBV5	6449	9000	0.62%	0.061%
68	19.039	2708	2712	2718	rBV3	6073	8756	0.60%	0.059%
69	19.286	2753	2754	2757	rVB2	2044	1552	0.11%	0.011%
70	19.397	2767	2773	2785	rBV	844216	1212389	82.86%	8.206%
71	19.639	2813	2814	2818	rBV5	2073	1879	0.13%	0.013%
72	19.909	2859	2860	2863	rBV3	2667	2824	0.19%	0.019%
73	21.209	3075	3081	3093	rBV	563525	838788	57.33%	5.678%
74	23.268	3424	3431	3438	rBV2	808198	1463164	100.00%	9.904%
75	23.403	3448	3454	3470	rVB	498343	1018244	69.59%	6.892%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045279.D
Acq On : 16 Apr 2024 13:50
Operator : MA/JU
Sample : PB160225BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK225

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 14773571

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045279.D
Acq On : 16 Apr 2024 13:50
Operator : MA/JU
Sample : PB160225BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

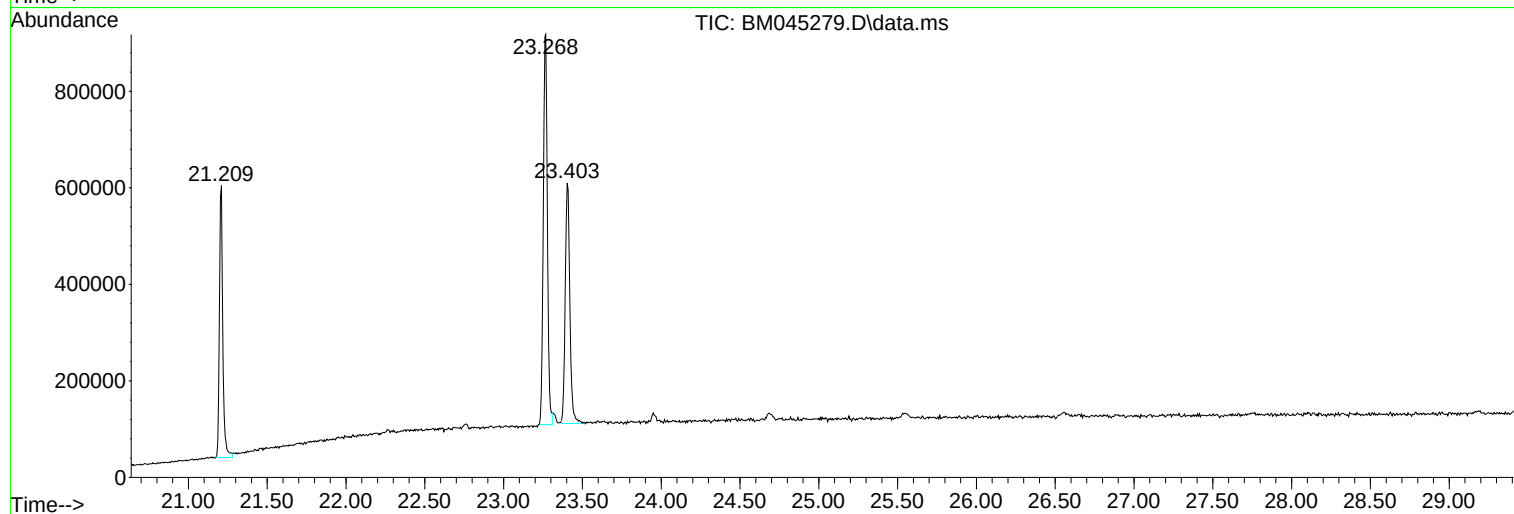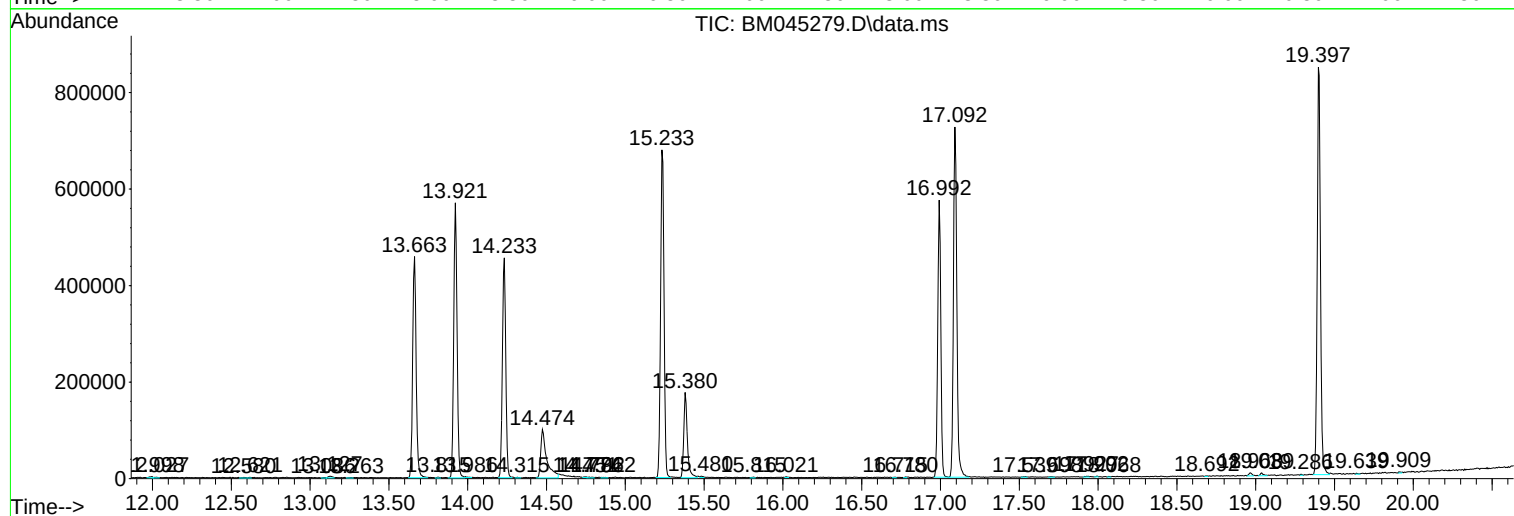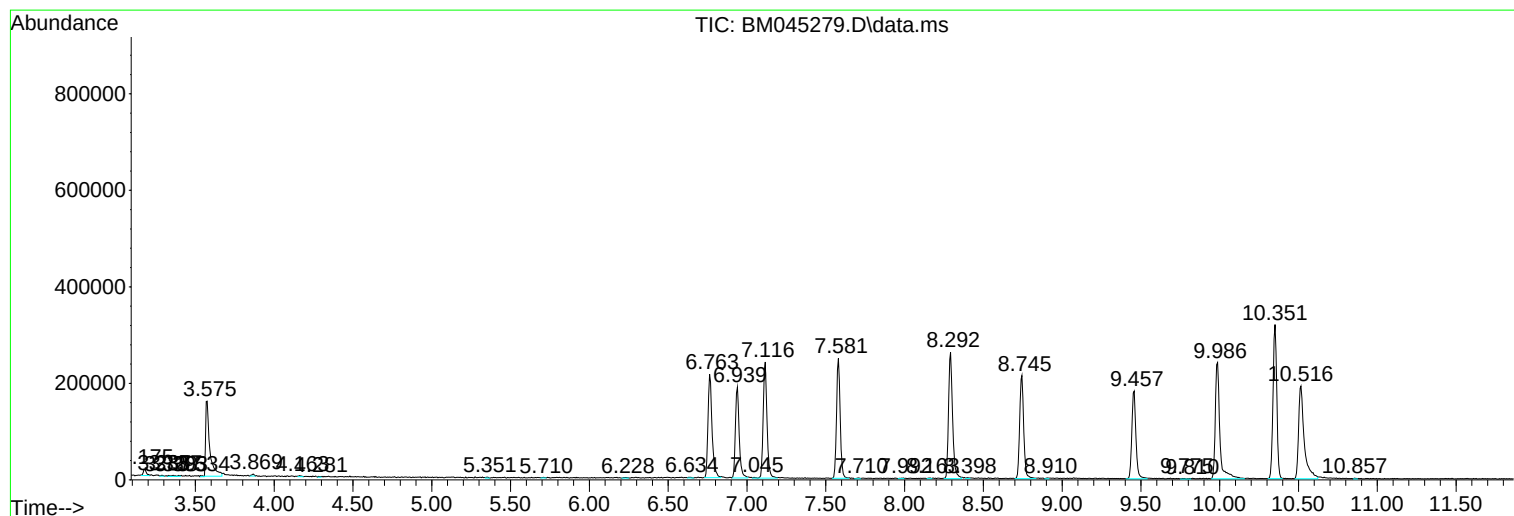

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045279.D
Acq On : 16 Apr 2024 13:50
Operator : MA/JU
Sample : PB160225BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045279.D
Acq On : 16 Apr 2024 13:50
Operator : MA/JU
Sample : PB160225BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------