

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045286.D
 Acq On : 16 Apr 2024 18:11
 Operator : MA/JU
 Sample : P2032-14
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	13	15	24	rVV2	9738	14829	0.83%	0.108%
2	3.487	65	68	70	rBV3	2025	2285	0.13%	0.017%
3	3.593	82	86	96	rBV	25938	55528	3.12%	0.403%
4	3.716	105	107	110	rVB3	3442	3528	0.20%	0.026%
5	3.758	112	114	118	rVV4	1614	2015	0.11%	0.015%
6	3.858	129	131	136	rVB4	2992	4236	0.24%	0.031%
7	4.087	168	170	171	rBV2	2715	1784	0.10%	0.013%
8	4.263	199	200	205	rVB5	2564	2570	0.14%	0.019%
9	4.952	313	317	323	rVB5	4762	7951	0.45%	0.058%
10	5.493	406	409	412	rBV4	1679	2122	0.12%	0.015%
11	6.451	571	572	576	rBV3	1906	1870	0.11%	0.014%
12	6.687	610	612	619	rVB7	2943	4895	0.27%	0.035%
13	6.769	619	626	640	rBV	37384	79189	4.45%	0.574%
14	6.940	649	655	667	rBV	180893	308764	17.35%	2.238%
15	7.116	678	685	696	rBV	176760	307298	17.26%	2.228%
16	7.581	756	764	774	rBV	206957	345353	19.40%	2.504%
17	8.216	869	872	876	rVB4	1499	2607	0.15%	0.019%
18	8.293	876	885	897	rBV2	123838	230013	12.92%	1.668%
19	8.481	915	917	922	rVB4	1487	2463	0.14%	0.018%
20	8.740	954	961	974	rBV	210083	380208	21.36%	2.756%
21	9.092	1018	1021	1027	rBV5	3234	3923	0.22%	0.028%
22	9.451	1076	1082	1094	rBV	171108	300338	16.87%	2.177%
23	9.981	1166	1172	1194	rBV	217210	443014	24.89%	3.212%
24	10.122	1194	1196	1201	rVV5	2507	3942	0.22%	0.029%
25	10.351	1228	1235	1243	rVB	266684	449483	25.25%	3.259%
26	10.516	1254	1263	1277	rBV	145378	350461	19.69%	2.541%
27	10.698	1291	1294	1299	rBV5	1122	1877	0.11%	0.014%
28	11.981	1508	1512	1519	rBV4	3610	5641	0.32%	0.041%
29	13.133	1703	1708	1709	rBV3	1963	2666	0.15%	0.019%
30	13.663	1791	1798	1809	rVB	488098	708758	39.82%	5.138%
31	13.827	1823	1826	1829	rBV3	1240	1943	0.11%	0.014%
32	13.922	1836	1842	1853	rBV	598377	858709	48.24%	6.225%
33	13.992	1853	1854	1858	rVV3	1819	1827	0.10%	0.013%
34	14.233	1886	1895	1904	rBV	390512	573731	32.23%	4.159%
35	14.316	1904	1909	1919	rBV5	7627	20653	1.16%	0.150%
36	14.533	1935	1946	1949	rBV8	10144	27731	1.56%	0.201%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045286.D
 Acq On : 16 Apr 2024 18:11
 Operator : MA/JU
 Sample : P2032-14
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.233	2059	2065	2074	rVB	719958	1085476	60.98%	7.869%
38	15.380	2084	2090	2104	rBV	212792	323024	18.15%	2.342%
39	15.474	2104	2106	2110	rVB3	2405	3132	0.18%	0.023%
40	15.639	2130	2134	2138	rBV3	2491	3957	0.22%	0.029%
41	16.027	2195	2200	2202	rBV3	1605	2150	0.12%	0.016%
42	16.445	2269	2271	2276	rVB3	2007	2860	0.16%	0.021%
43	16.557	2288	2290	2295	rVB4	1499	2146	0.12%	0.016%
44	16.598	2295	2297	2303	rBV4	1042	1926	0.11%	0.014%
45	16.721	2314	2318	2321	rVB5	1487	2474	0.14%	0.018%
46	16.786	2328	2329	2334	rVB4	1449	1962	0.11%	0.014%
47	16.845	2336	2339	2340	rBV3	3486	3732	0.21%	0.027%
48	16.992	2358	2364	2372	rBV	467459	647284	36.36%	4.693%
49	17.092	2375	2381	2395	rVV	835430	1212337	68.11%	8.789%
50	17.521	2450	2454	2458	rVB5	1768	2734	0.15%	0.020%
51	17.904	2515	2519	2527	rBV6	15712	28316	1.59%	0.205%
52	17.980	2530	2532	2536	rVB4	2732	3552	0.20%	0.026%
53	18.021	2536	2539	2541	rBV3	2176	2562	0.14%	0.019%
54	18.192	2565	2568	2572	rBV5	2099	3547	0.20%	0.026%
55	18.486	2616	2618	2621	rVV4	1970	2367	0.13%	0.017%
56	18.721	2654	2658	2660	rBV5	1282	1834	0.10%	0.013%
57	18.786	2665	2669	2670	rBV3	2916	3125	0.18%	0.023%
58	18.962	2696	2699	2703	rBV5	10106	12052	0.68%	0.087%
59	19.039	2706	2712	2714	rBV3	7258	10192	0.57%	0.074%
60	19.198	2736	2739	2747	rVB7	10630	16775	0.94%	0.122%
61	19.398	2767	2773	2782	rBV	1031073	1433142	80.51%	10.390%
62	19.598	2805	2807	2810	rBV4	1939	2466	0.14%	0.018%
63	19.751	2831	2833	2835	rBV3	2463	1921	0.11%	0.014%
64	21.209	3075	3081	3088	rBV	552614	739900	41.57%	5.364%
65	22.056	3222	3225	3231	rVB4	34532	45060	2.53%	0.327%
66	23.268	3424	3431	3445	rVB2	989440	1780050	100.00%	12.905%
67	23.409	3448	3455	3467	rVB	453633	897547	50.42%	6.507%




Sum of corrected areas: 13793807

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045286.D
Acq On : 16 Apr 2024 18:11
Operator : MA/JU
Sample : P2032-14
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

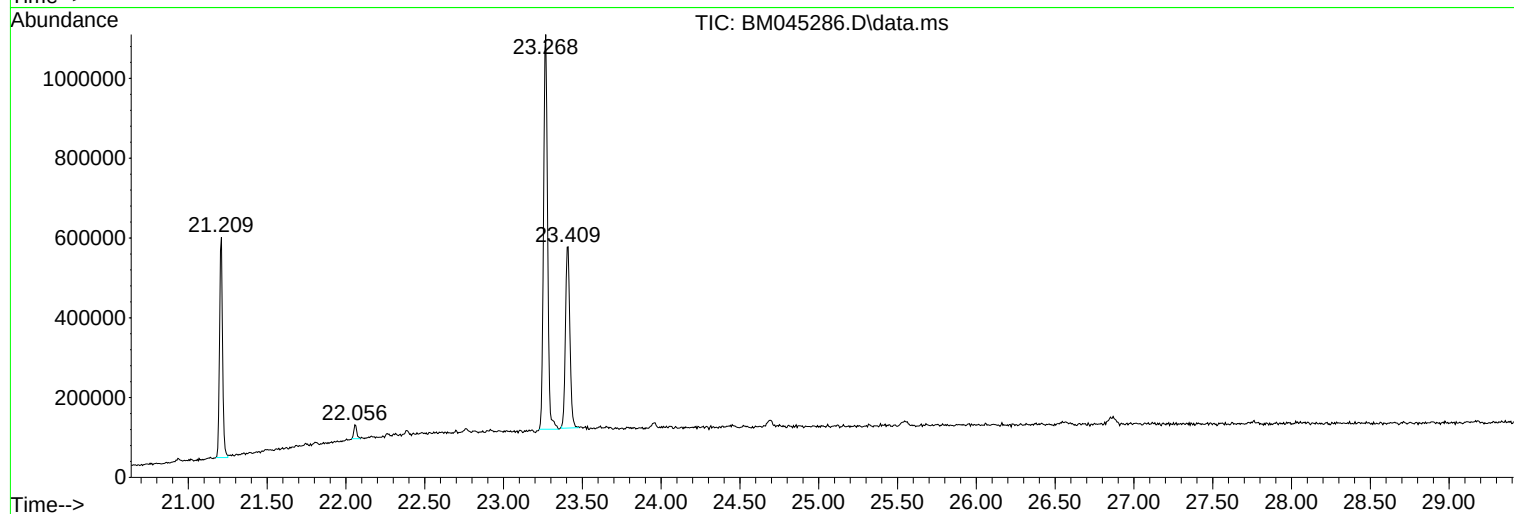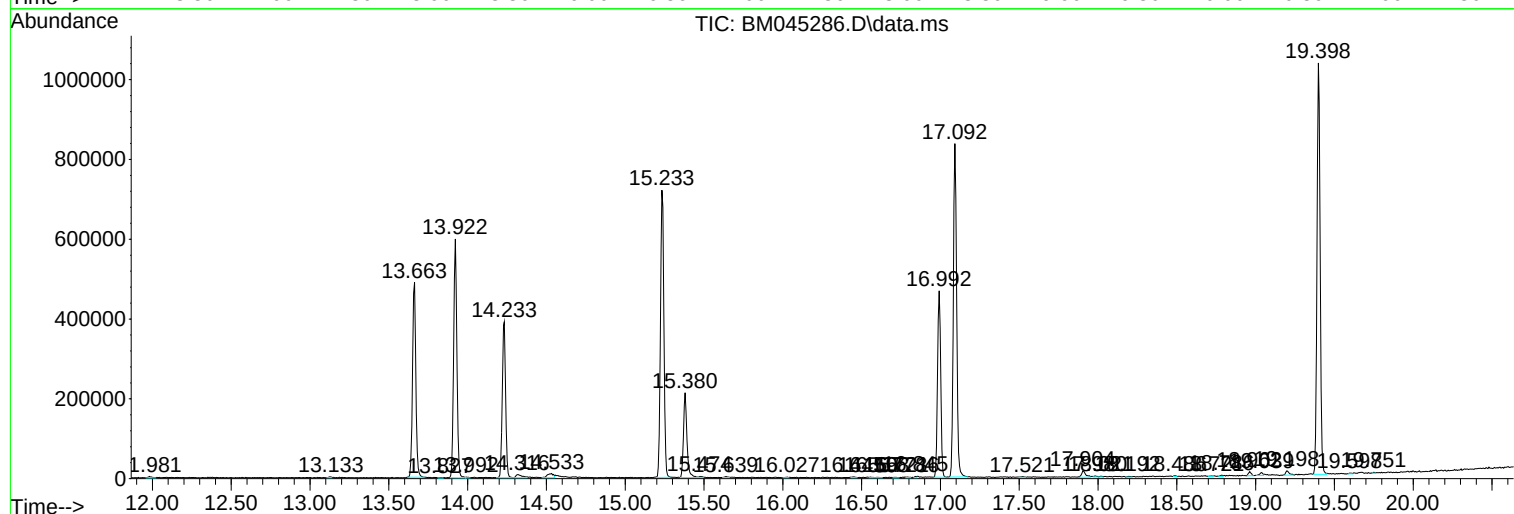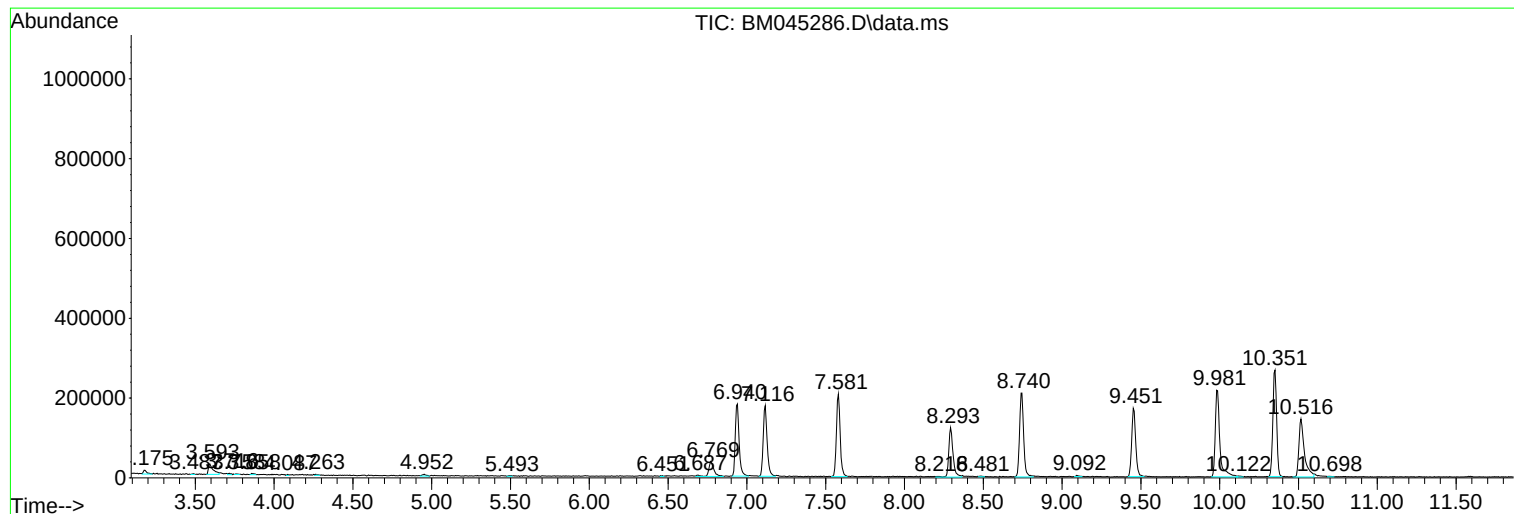

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045286.D
Acq On : 16 Apr 2024 18:11
Operator : MA/JU
Sample : P2032-14
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045286.D
Acq On : 16 Apr 2024 18:11
Operator : MA/JU
Sample : P2032-14
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc