

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045288.D
 Acq On : 16 Apr 2024 19:26
 Operator : MA/JU
 Sample : P2036-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	5	9	13	rBV	35925	45790	3.13%	0.357%
2	3.175	13	15	25	rVB	19029	28963	1.98%	0.226%
3	3.258	27	29	32	rVB4	2011	1685	0.12%	0.013%
4	3.305	35	37	40	rBV3	2283	2054	0.14%	0.016%
5	3.581	81	84	97	rBV	44682	91493	6.25%	0.712%
6	3.828	124	126	128	rBV3	3401	3221	0.22%	0.025%
7	3.857	129	131	137	rVB4	3539	5022	0.34%	0.039%
8	4.357	212	216	222	rVB2	15991	23005	1.57%	0.179%
9	4.428	226	228	232	rVV3	1984	1660	0.11%	0.013%
10	4.469	232	235	238	rVV5	1423	2068	0.14%	0.016%
11	4.546	246	248	251	rVV3	1385	1637	0.11%	0.013%
12	4.581	252	254	257	rVV4	1561	1514	0.10%	0.012%
13	4.952	312	317	323	rBV2	10565	18362	1.25%	0.143%
14	5.051	330	334	336	rBV4	1822	2134	0.15%	0.017%
15	5.351	382	385	387	rVB4	1385	1482	0.10%	0.012%
16	5.393	391	392	396	rBV3	1830	1945	0.13%	0.015%
17	5.593	421	426	430	rBV6	1220	2712	0.19%	0.021%
18	5.681	436	441	448	rVB2	13972	24562	1.68%	0.191%
19	6.193	525	528	530	rBV3	1643	1603	0.11%	0.012%
20	6.610	596	599	602	rBV4	958	1530	0.10%	0.012%
21	6.775	621	627	637	rBV2	30614	65325	4.46%	0.509%
22	6.940	649	655	668	rBV	178373	303380	20.72%	2.362%
23	7.040	671	672	678	rVV4	1696	3116	0.21%	0.024%
24	7.116	678	685	695	rVV	170245	298678	20.39%	2.325%
25	7.216	699	702	706	rVV4	1493	2240	0.15%	0.017%
26	7.581	757	764	778	rVB	216880	376520	25.71%	2.932%
27	7.928	819	823	828	rBV4	3637	6487	0.44%	0.051%
28	7.998	833	835	840	rBV6	1094	1643	0.11%	0.013%
29	8.292	877	885	898	rBV	110403	202000	13.79%	1.573%
30	8.739	954	961	972	rBV	199491	355526	24.28%	2.768%
31	8.816	972	974	976	rVB3	1803	1516	0.10%	0.012%
32	9.451	1076	1082	1096	rBV	161121	288107	19.67%	2.243%
33	9.981	1167	1172	1192	rBV	193198	395872	27.03%	3.082%
34	10.192	1205	1208	1210	rBV3	1853	1783	0.12%	0.014%
35	10.351	1224	1235	1243	rBV	282619	473069	32.30%	3.683%
36	10.516	1256	1263	1280	rBV	164082	386228	26.37%	3.007%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045288.D
 Acq On : 16 Apr 2024 19:26
 Operator : MA/JU
 Sample : P2036-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	11.916	1495	1501	1507	rBV3	10495	20700	1.41%	0.161%
38	11.969	1507	1510	1512	rVV4	1219	1465	0.10%	0.011%
39	12.563	1609	1611	1615	rBV4	1617	1969	0.13%	0.015%
40	12.639	1622	1624	1627	rBV4	1503	1779	0.12%	0.014%
41	13.127	1701	1707	1711	rBV6	3174	4296	0.29%	0.033%
42	13.663	1791	1798	1808	rVV	406495	628627	42.92%	4.894%
43	13.922	1836	1842	1855	rVV	530611	768114	52.45%	5.981%
44	14.033	1855	1861	1864	rVB5	1517	2662	0.18%	0.021%
45	14.227	1888	1894	1903	rBV	399576	582820	39.80%	4.538%
46	14.469	1931	1935	1940	rVB3	2131	3776	0.26%	0.029%
47	14.539	1940	1947	1948	rBV4	5297	8914	0.61%	0.069%
48	14.557	1948	1950	1955	rVB6	2341	3284	0.22%	0.026%
49	14.633	1960	1963	1967	rVV4	1864	3100	0.21%	0.024%
50	14.692	1969	1973	1976	rVB4	2243	2983	0.20%	0.023%
51	15.233	2058	2065	2075	rBV	665073	968584	66.14%	7.541%
52	15.380	2084	2090	2101	rBV	159621	258301	17.64%	2.011%
53	15.451	2101	2102	2105	rVV3	3893	3229	0.22%	0.025%
54	15.474	2105	2106	2111	rVV3	2308	3076	0.21%	0.024%
55	15.539	2114	2117	2120	rBV4	1378	1745	0.12%	0.014%
56	15.710	2144	2146	2149	rVB3	1842	1630	0.11%	0.013%
57	16.033	2198	2201	2205	rVB4	1964	2565	0.18%	0.020%
58	16.127	2214	2217	2218	rVB	1797	1641	0.11%	0.013%
59	16.421	2265	2267	2272	rBV3	1897	2428	0.17%	0.019%
60	16.598	2294	2297	2300	rBV4	1152	1791	0.12%	0.014%
61	16.786	2327	2329	2335	rVB4	1094	1854	0.13%	0.014%
62	16.927	2350	2353	2358	rBV5	4278	4196	0.29%	0.033%
63	16.992	2358	2364	2371	rVV	484252	647505	44.21%	5.041%
64	17.092	2373	2381	2393	rVV2	704077	1054078	71.98%	8.207%
65	17.192	2397	2398	2403	rVV5	2150	2798	0.19%	0.022%
66	17.410	2429	2435	2438	rBV6	2064	3214	0.22%	0.025%
67	17.480	2443	2447	2449	rBV4	4409	5124	0.35%	0.040%
68	17.686	2479	2482	2484	rBV3	2101	1968	0.13%	0.015%
69	17.904	2514	2519	2527	rBV2	26701	42380	2.89%	0.330%
70	18.021	2537	2539	2544	rVV5	1689	2340	0.16%	0.018%
71	18.139	2556	2559	2561	rBV4	2195	2207	0.15%	0.017%
72	18.198	2567	2569	2572	rVB3	1664	1777	0.12%	0.014%
73	18.333	2589	2592	2594	rBV4	2357	2342	0.16%	0.018%
74	18.562	2628	2631	2633	rBV2	1638	1662	0.11%	0.013%
75	18.780	2665	2668	2674	rVV8	4350	7676	0.52%	0.060%
76	18.845	2676	2679	2680	rVV2	1563	1659	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045288.D
 Acq On : 16 Apr 2024 19:26
 Operator : MA/JU
 Sample : P2036-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	18.962	2696	2699	2703	rBV5	7113	8451	0.58%	0.066%
78	19.039	2708	2712	2718	rBV3	6263	10804	0.74%	0.084%
79	19.104	2722	2723	2726	rVB3	2340	2051	0.14%	0.016%
80	19.204	2735	2740	2747	rVV6	14686	22565	1.54%	0.176%
81	19.345	2761	2764	2767	rBV4	2267	4086	0.28%	0.032%
82	19.398	2767	2773	2783	rVV	867590	1202419	82.10%	9.362%
83	19.462	2783	2784	2790	rVB6	2942	4836	0.33%	0.038%
84	19.662	2816	2818	2820	rBV3	2044	1823	0.12%	0.014%
85	19.786	2838	2839	2841	rBV2	2946	2077	0.14%	0.016%
86	19.815	2841	2844	2846	rBV3	2734	3796	0.26%	0.030%
87	19.868	2851	2853	2856	rVV4	3010	2387	0.16%	0.019%
88	20.245	2915	2917	2919	rBV3	3190	3911	0.27%	0.030%
89	20.939	3031	3035	3043	rBV9	16321	32593	2.23%	0.254%
90	21.209	3075	3081	3089	rBV	495819	719904	49.16%	5.605%
91	23.268	3424	3431	3437	rBV	807742	1464491	100.00%	11.402%
92	23.403	3448	3454	3464	rVB	456099	871228	59.49%	6.783%


Sum of corrected areas: 12843613

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045288.D
Acq On : 16 Apr 2024 19:26
Operator : MA/JU
Sample : P2036-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

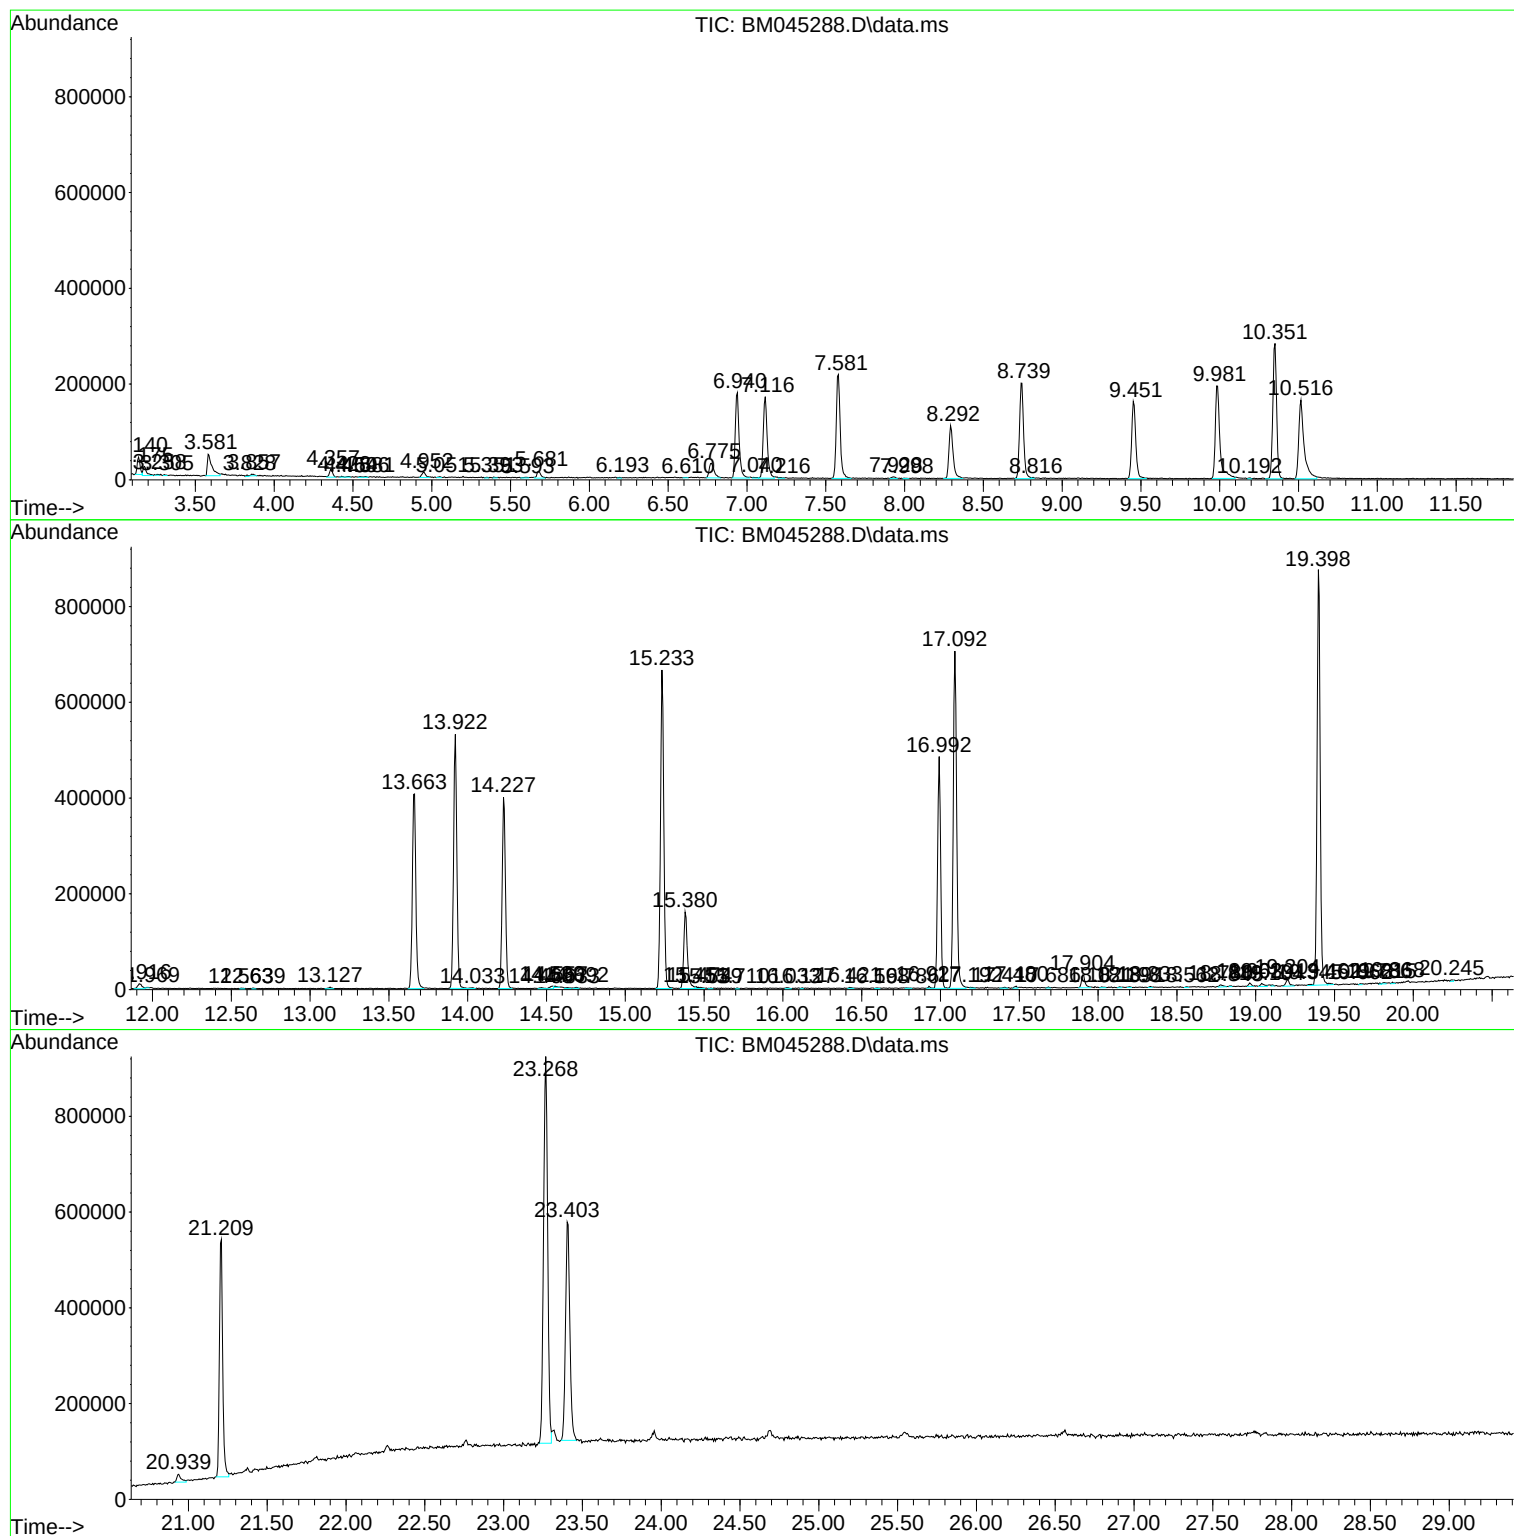

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045288.D
Acq On : 16 Apr 2024 19:26
Operator : MA/JU
Sample : P2036-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045288.D
Acq On : 16 Apr 2024 19:26
Operator : MA/JU
Sample : P2036-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc