

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045289.D
 Acq On : 16 Apr 2024 20:03
 Operator : MA/JU
 Sample : P2036-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	5	9	13	rBV	95774	122867	9.64%	0.982%
2	3.175	13	15	19	rVB2	9769	12499	0.98%	0.100%
3	3.369	46	48	50	rVB3	1807	1504	0.12%	0.012%
4	3.399	50	53	54	rBV2	2400	2291	0.18%	0.018%
5	3.457	61	63	66	rBV3	1499	1529	0.12%	0.012%
6	3.593	83	86	93	rBV2	18594	37582	2.95%	0.300%
7	3.869	128	133	137	rVB4	3557	6463	0.51%	0.052%
8	4.357	211	216	227	rVB	264999	375069	29.41%	2.996%
9	4.546	246	248	251	rVB3	2399	2334	0.18%	0.019%
10	4.887	304	306	308	rBV3	1593	1785	0.14%	0.014%
11	4.922	308	312	322	rVB2	19697	33732	2.65%	0.269%
12	5.104	340	343	345	rBV4	1320	1639	0.13%	0.013%
13	5.234	361	365	368	rVB4	1797	2858	0.22%	0.023%
14	5.657	434	437	438	rBV2	1578	1573	0.12%	0.013%
15	5.940	482	485	488	rBV4	1628	1702	0.13%	0.014%
16	6.769	622	626	637	rBV	27700	58705	4.60%	0.469%
17	6.940	647	655	666	rBV	169375	289556	22.71%	2.313%
18	7.116	679	685	697	rBV	155941	278974	21.88%	2.229%
19	7.193	697	698	700	rVV2	1975	1502	0.12%	0.012%
20	7.463	740	744	749	rBV5	3066	4933	0.39%	0.039%
21	7.581	757	764	776	rBV	223087	382745	30.02%	3.058%
22	7.745	787	792	793	rBV3	1439	2201	0.17%	0.018%
23	7.928	817	823	829	rBV4	7409	13262	1.04%	0.106%
24	8.175	862	865	868	rVB3	1487	1654	0.13%	0.013%
25	8.210	868	871	872	rBV3	1406	1484	0.12%	0.012%
26	8.298	880	886	894	rBV	48654	92012	7.22%	0.735%
27	8.745	955	962	972	rBV	191998	334553	26.24%	2.673%
28	9.451	1075	1082	1091	rBV	159637	279190	21.89%	2.230%
29	9.986	1166	1173	1193	rBV	185888	384765	30.17%	3.074%
30	10.128	1195	1197	1200	rVB2	1488	1470	0.12%	0.012%
31	10.216	1205	1212	1217	rBV5	6342	11236	0.88%	0.090%
32	10.351	1227	1235	1245	rBV	277513	468700	36.76%	3.744%
33	10.522	1259	1264	1278	rVB2	44359	116701	9.15%	0.932%
34	10.739	1299	1301	1304	rVB4	1562	1583	0.12%	0.013%
35	11.198	1372	1379	1389	rBV5	18097	49122	3.85%	0.392%
36	11.969	1506	1510	1515	rBV4	2792	4167	0.33%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045289.D
 Acq On : 16 Apr 2024 20:03
 Operator : MA/JU
 Sample : P2036-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.127	1702	1707	1711	rVB4	3224	5527	0.43%	0.044%
38	13.663	1786	1798	1813	rBV	407414	634508	49.76%	5.069%
39	13.922	1835	1842	1853	rBV	479393	703607	55.18%	5.621%
40	14.074	1867	1868	1873	rVB4	1038	1476	0.12%	0.012%
41	14.122	1873	1876	1878	rBV4	1230	1589	0.12%	0.013%
42	14.227	1888	1894	1904	rVV	408814	584031	45.80%	4.666%
43	14.527	1939	1945	1952	rBV6	6700	17596	1.38%	0.141%
44	14.580	1952	1954	1957	rVV3	4710	5901	0.46%	0.047%
45	14.616	1957	1960	1963	rVV4	2836	4370	0.34%	0.035%
46	14.674	1967	1970	1977	rVV8	2548	5149	0.40%	0.041%
47	14.757	1981	1984	1987	rBV3	1787	2008	0.16%	0.016%
48	15.098	2038	2042	2043	rBV3	1104	1482	0.12%	0.012%
49	15.233	2058	2065	2074	rBV	679717	972991	76.30%	7.773%
50	15.380	2084	2090	2099	rBV	162054	258191	20.25%	2.063%
51	15.480	2104	2107	2109	rVV4	4008	4658	0.37%	0.037%
52	15.504	2109	2111	2115	rVV5	2761	3051	0.24%	0.024%
53	15.610	2127	2129	2132	rVB3	1898	2443	0.19%	0.020%
54	15.639	2132	2134	2136	rBV3	1768	1633	0.13%	0.013%
55	15.657	2136	2137	2140	rBV3	1928	1521	0.12%	0.012%
56	15.710	2143	2146	2149	rBV4	1080	1654	0.13%	0.013%
57	15.916	2177	2181	2184	rBV3	1354	2060	0.16%	0.016%
58	15.974	2189	2191	2192	rVV2	2849	2233	0.18%	0.018%
59	16.027	2197	2200	2204	rVB6	3032	4228	0.33%	0.034%
60	16.074	2204	2208	2211	rBV4	1957	3040	0.24%	0.024%
61	16.292	2241	2245	2247	rBV3	2188	2119	0.17%	0.017%
62	16.321	2247	2250	2253	rVB3	1970	2732	0.21%	0.022%
63	16.363	2253	2257	2259	rBV4	1704	1935	0.15%	0.015%
64	16.427	2265	2268	2269	rBV	1894	1506	0.12%	0.012%
65	16.474	2274	2276	2278	rBV2	2336	2027	0.16%	0.016%
66	16.692	2310	2313	2317	rBV5	1632	2795	0.22%	0.022%
67	16.768	2325	2326	2329	rBV2	2032	1583	0.12%	0.013%
68	16.792	2329	2330	2335	rVB4	1739	2018	0.16%	0.016%
69	16.886	2341	2346	2347	rVB3	2856	2586	0.20%	0.021%
70	16.927	2347	2353	2354	rBV5	3321	2751	0.22%	0.022%
71	16.992	2357	2364	2372	rBV	491972	670525	52.58%	5.357%
72	17.092	2374	2381	2394	rVB	659792	958744	75.19%	7.659%
73	17.268	2408	2411	2413	rBV3	2284	1709	0.13%	0.014%
74	17.415	2433	2436	2439	rVB4	2292	2997	0.24%	0.024%
75	17.592	2463	2466	2468	rBV4	1516	1637	0.13%	0.013%
76	17.639	2472	2474	2477	rVV4	2195	2423	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045289.D
 Acq On : 16 Apr 2024 20:03
 Operator : MA/JU
 Sample : P2036-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.780	2496	2498	2501	rBV3	2158	2609	0.20%	0.021%
78	17.815	2503	2504	2507	rBV3	2634	1654	0.13%	0.013%
79	17.904	2515	2519	2525	rBV3	19414	29213	2.29%	0.233%
80	18.115	2553	2555	2558	rVB4	2107	1742	0.14%	0.014%
81	18.151	2558	2561	2563	rBV4	2599	3417	0.27%	0.027%
82	18.333	2590	2592	2598	rVB5	2707	3714	0.29%	0.030%
83	18.392	2598	2602	2603	rBV4	2603	3189	0.25%	0.025%
84	18.468	2614	2615	2619	rBV4	1974	2303	0.18%	0.018%
85	18.780	2665	2668	2669	rBV3	3245	2661	0.21%	0.021%
86	18.839	2676	2678	2681	rBV4	2904	3406	0.27%	0.027%
87	18.862	2681	2682	2684	rVV2	1878	1661	0.13%	0.013%
88	18.904	2688	2689	2693	rVV4	2033	1703	0.13%	0.014%
89	18.962	2695	2699	2704	rVB5	8964	11326	0.89%	0.090%
90	19.039	2708	2712	2715	rVV3	5721	8404	0.66%	0.067%
91	19.198	2736	2739	2745	rVB6	11495	17610	1.38%	0.141%
92	19.245	2745	2747	2749	rVB3	2961	1624	0.13%	0.013%
93	19.280	2749	2753	2754	rBV4	2394	3171	0.25%	0.025%
94	19.398	2767	2773	2784	rBV2	867398	1200249	94.13%	9.589%
95	19.603	2806	2808	2809	rBV2	2841	2034	0.16%	0.016%
96	19.821	2843	2845	2848	rVV4	2488	2170	0.17%	0.017%
97	19.874	2852	2854	2858	rBV5	2194	2284	0.18%	0.018%
98	21.203	3075	3080	3093	rBV	559090	774463	60.73%	6.187%
99	23.268	3424	3431	3437	rBV	713997	1275162	100.00%	10.187%
100	23.403	3448	3454	3465	rBV	467460	892695	70.01%	7.132%




Sum of corrected areas: 12517440

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045289.D
Acq On : 16 Apr 2024 20:03
Operator : MA/JU
Sample : P2036-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

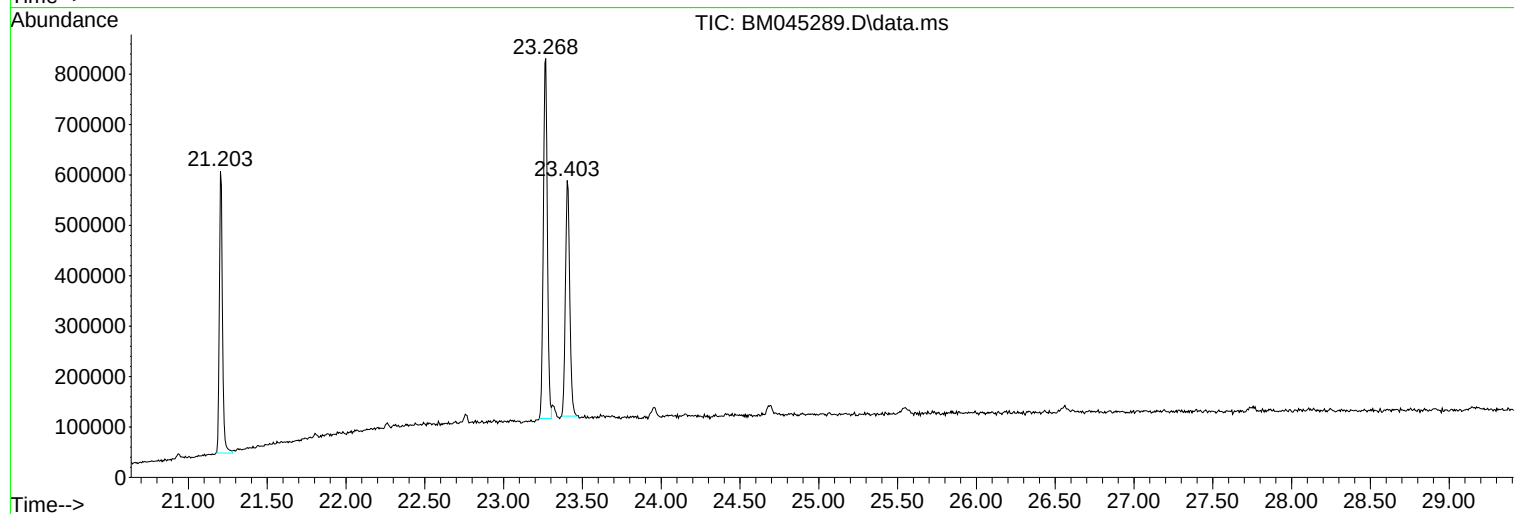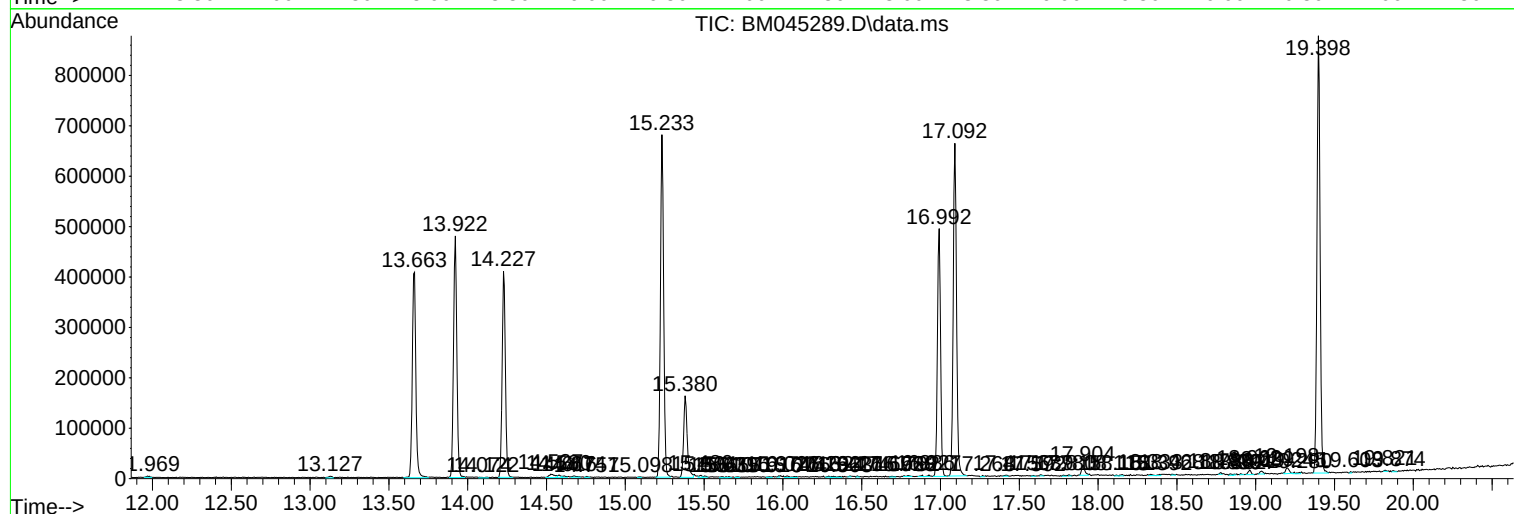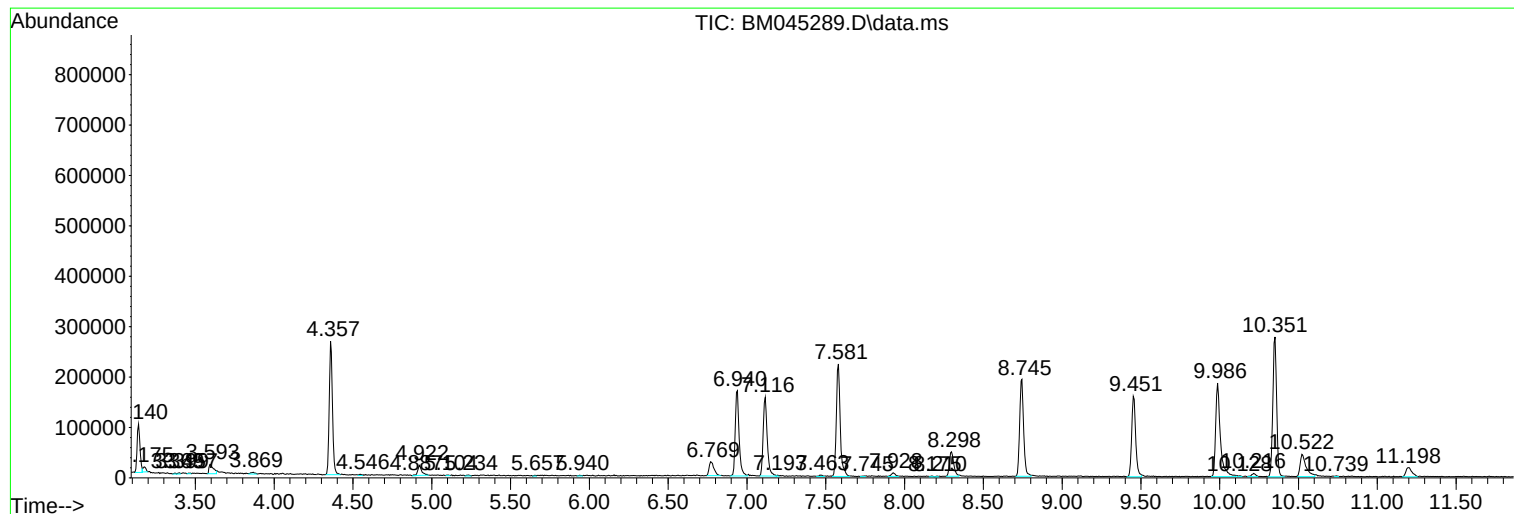

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045289.D
Acq On : 16 Apr 2024 20:03
Operator : MA/JU
Sample : P2036-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.198	2.10 ng/ul	49122	Naphthalene-d8	10.351

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Naphthalenol, 1-amino-		159	C10H9NO	002834-92-6	38	
2	2,5-Difluorobenzoic acid, decyl ...		298	C17H24F2O2	1000338-80-9	38	
3	4(1H)-Quinolinone, 1-methyl-		159	C10H9NO	000083-54-5	35	
4	Nonanoic acid, dodecyl ester		326	C21H42O2	1000340-27-9	32	
5	2,4-Difluorobenzoic acid, undecy...		312	C18H26F2O2	1000338-78-9	32	

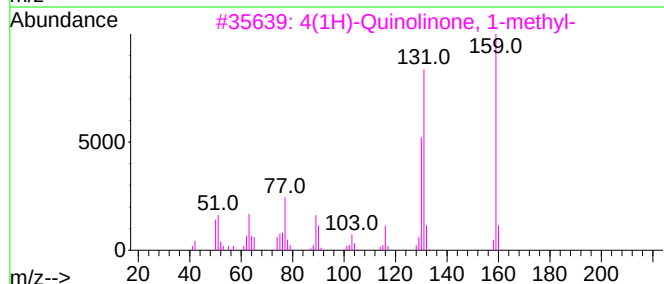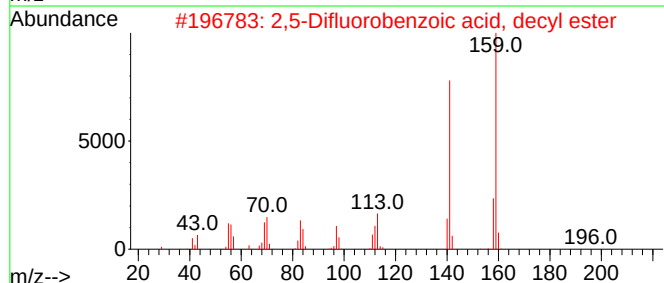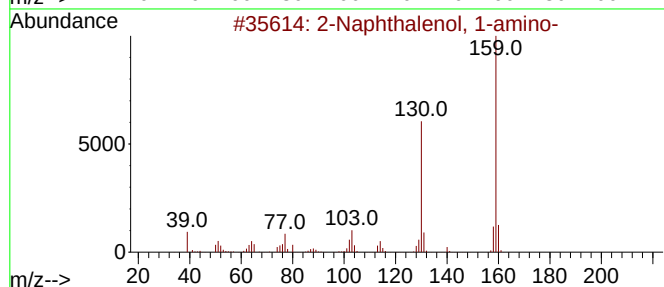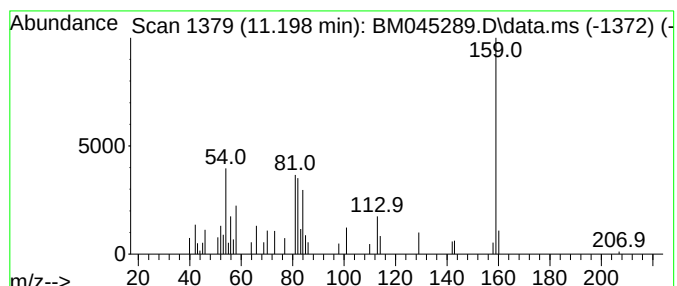

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045289.D
Acq On : 16 Apr 2024 20:03
Operator : MA/JU
Sample : P2036-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	11.198	2.1	ng/u1	49122	2	10.351	468700	20.0