

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045290.D
 Acq On : 16 Apr 2024 20:41
 Operator : MA/JU
 Sample : P2051-16
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB3	10397	12283	0.69%	0.087%
2	3.593	83	86	97	rBV	21615	46796	2.63%	0.332%
3	3.875	128	134	136	rVV5	3685	7091	0.40%	0.050%
4	3.922	140	142	147	rVB5	2177	2435	0.14%	0.017%
5	4.187	184	187	190	rVB5	2414	2935	0.17%	0.021%
6	4.669	266	269	270	rBV3	2116	1960	0.11%	0.014%
7	5.593	425	426	429	rBV4	1772	2049	0.12%	0.015%
8	6.698	612	614	618	rVB5	1696	1785	0.10%	0.013%
9	6.769	621	626	640	rVB	35245	68888	3.88%	0.489%
10	6.934	648	654	664	rBV	194348	324666	18.27%	2.306%
11	7.116	678	685	700	rBV	180714	316358	17.80%	2.247%
12	7.581	757	764	774	rBV	231245	370898	20.87%	2.635%
13	8.292	879	885	895	rBV2	114281	204099	11.48%	1.450%
14	8.616	935	940	942	rBV3	1034	1888	0.11%	0.013%
15	8.739	952	961	974	rBV	221729	392557	22.09%	2.788%
16	9.016	1007	1008	1013	rVB4	1454	1799	0.10%	0.013%
17	9.451	1075	1082	1091	rBV	178071	315735	17.76%	2.243%
18	9.981	1165	1172	1189	rVV	213838	417909	23.51%	2.968%
19	10.222	1210	1213	1218	rVB4	1000	1897	0.11%	0.013%
20	10.351	1228	1235	1245	rBV	294398	494488	27.82%	3.512%
21	10.510	1256	1262	1282	rBV	158981	389938	21.94%	2.770%
22	11.975	1507	1511	1513	rBV3	2581	3020	0.17%	0.021%
23	11.992	1513	1514	1518	rVV3	2508	2156	0.12%	0.015%
24	13.127	1702	1707	1714	rVB5	2506	4457	0.25%	0.032%
25	13.657	1791	1797	1810	rBV	456229	689415	38.79%	4.897%
26	13.921	1835	1842	1851	rBV	584038	863038	48.56%	6.130%
27	14.045	1860	1863	1867	rBV5	1805	2765	0.16%	0.020%
28	14.227	1888	1894	1904	rBV	440532	646709	36.39%	4.594%
29	14.527	1940	1945	1946	rBV4	4574	5677	0.32%	0.040%
30	15.233	2059	2065	2077	rVB	731651	1061352	59.72%	7.539%
31	15.380	2083	2090	2103	rBV	185267	290747	16.36%	2.065%
32	15.480	2106	2107	2111	rVB2	2791	2320	0.13%	0.016%
33	16.021	2197	2199	2203	rVB4	1977	2395	0.13%	0.017%
34	16.939	2350	2355	2357	rVB6	2015	3259	0.18%	0.023%
35	16.992	2357	2364	2371	rBV	544988	748487	42.11%	5.317%
36	17.092	2374	2381	2397	rVB	791353	1176410	66.19%	8.356%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045290.D
Acq On : 16 Apr 2024 20:41
Operator : MA/JU
Sample : P2051-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CORJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.227	2402	2404	2409	rVB5	1327	1810	0.10%	0.013%
38	17.404	2428	2434	2437	rBV3	1160	2130	0.12%	0.015%
39	17.639	2472	2474	2476	rBV3	2007	2180	0.12%	0.015%
40	17.904	2515	2519	2527	rBV5	18580	32336	1.82%	0.230%
41	18.333	2590	2592	2595	rBV4	1944	2274	0.13%	0.016%
42	18.780	2667	2668	2672	rVB2	2095	1999	0.11%	0.014%
43	18.856	2679	2681	2686	rVB5	1114	1787	0.10%	0.013%
44	18.962	2696	2699	2704	rBV4	7795	11098	0.62%	0.079%
45	19.039	2707	2712	2716	rBV2	6417	10148	0.57%	0.072%
46	19.203	2734	2740	2745	rBV7	11823	19540	1.10%	0.139%
47	19.280	2751	2753	2757	rBV5	1879	1908	0.11%	0.014%
48	19.351	2763	2765	2767	rBV2	2848	2880	0.16%	0.020%
49	19.398	2767	2773	2785	rVV	978159	1346871	75.78%	9.567%
50	19.603	2806	2808	2811	rBV4	2114	2714	0.15%	0.019%
51	19.933	2862	2864	2865	rBV2	2239	1885	0.11%	0.013%
52	20.339	2931	2933	2934	rBV2	2754	1911	0.11%	0.014%
53	21.203	3075	3080	3090	rBV	633255	881672	49.61%	6.263%
54	23.268	3423	3431	3438	rBV2	962887	1777295	100.00%	12.624%
55	23.403	3448	3454	3466	rVB	562333	1095054	61.61%	7.778%




Sum of corrected areas: 14078153

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045290.D
Acq On : 16 Apr 2024 20:41
Operator : MA/JU
Sample : P2051-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

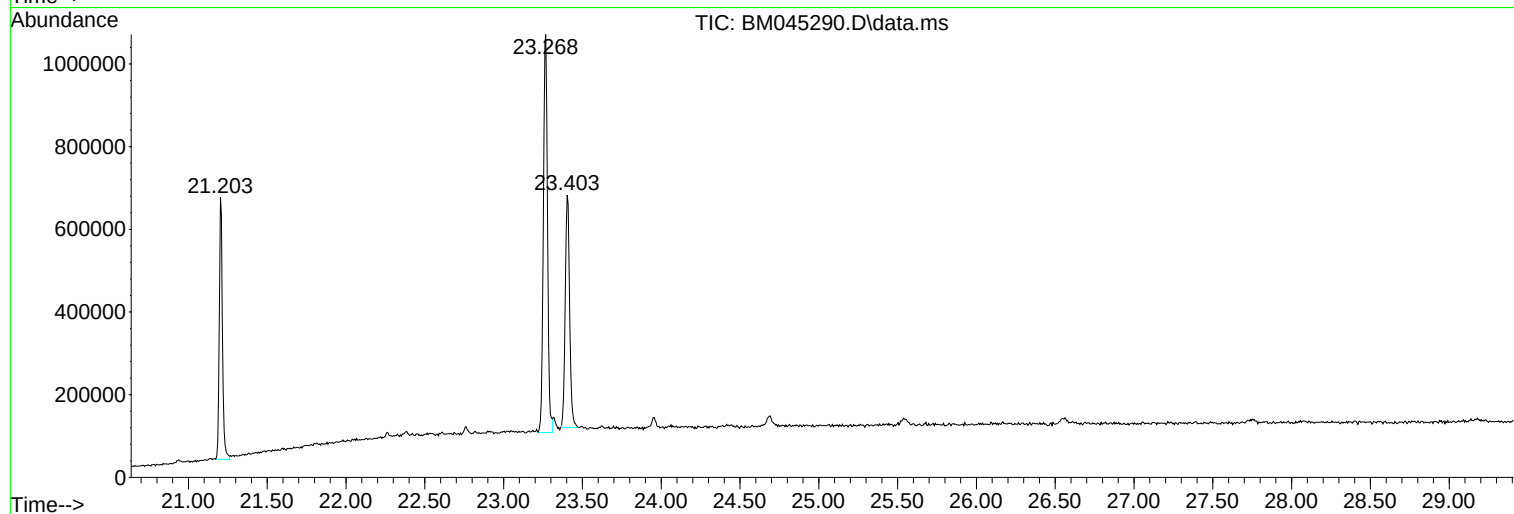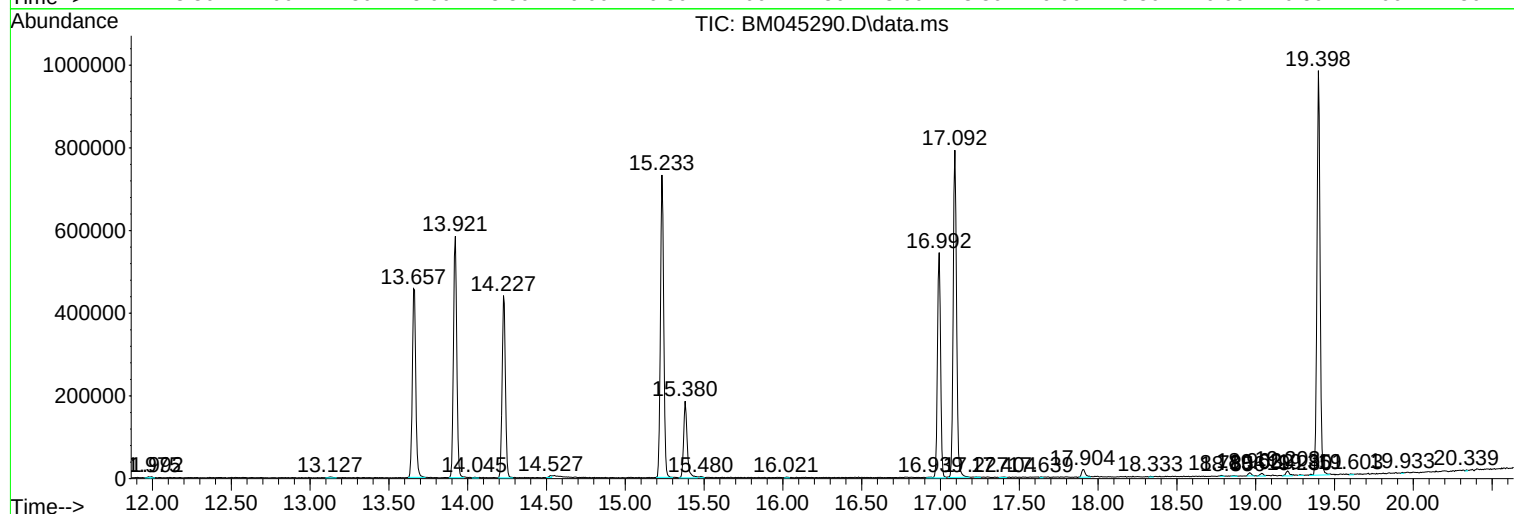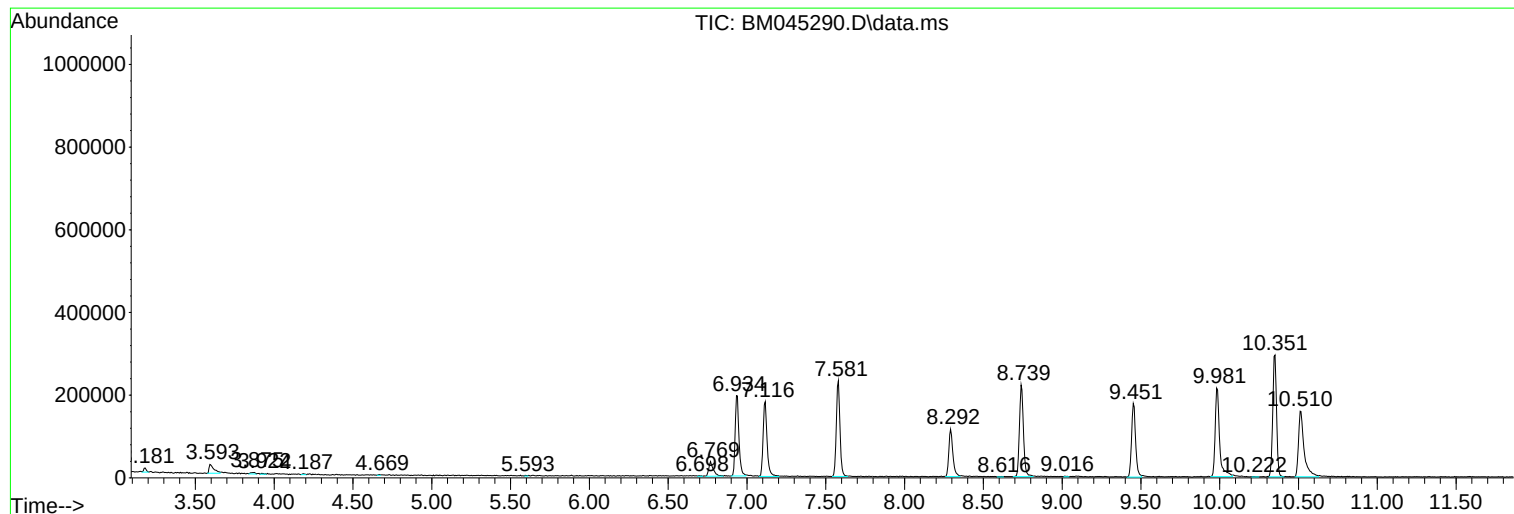

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045290.D
Acq On : 16 Apr 2024 20:41
Operator : MA/JU
Sample : P2051-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045290.D
Acq On : 16 Apr 2024 20:41
Operator : MA/JU
Sample : P2051-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------