

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045291.D
 Acq On : 16 Apr 2024 21:18
 Operator : MA/JU
 Sample : P2098-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	22	rBV2	9491	12800	0.81%	0.094%
2	3.322	37	40	43	rBV5	1463	1642	0.10%	0.012%
3	3.493	67	69	72	rVB4	2626	2253	0.14%	0.016%
4	3.593	83	86	98	rBV	22758	52900	3.37%	0.387%
5	3.863	129	132	136	rBV5	4319	5799	0.37%	0.042%
6	4.199	187	189	191	rBV3	2078	1584	0.10%	0.012%
7	4.305	204	207	209	rVB3	2279	2602	0.17%	0.019%
8	5.504	406	411	413	rBV3	1411	2047	0.13%	0.015%
9	5.599	426	427	431	rBV3	1814	2391	0.15%	0.017%
10	6.369	555	558	564	rBV6	1112	1679	0.11%	0.012%
11	6.499	577	580	583	rBV5	1611	1708	0.11%	0.012%
12	6.769	620	626	638	rBV	28921	62671	3.99%	0.458%
13	6.940	649	655	668	rBV	173852	294054	18.72%	2.149%
14	7.116	678	685	696	rBV	160836	283248	18.03%	2.070%
15	7.581	757	764	772	rBV	240043	399468	25.43%	2.920%
16	7.651	775	776	779	rVV3	1962	1724	0.11%	0.013%
17	7.704	783	785	790	rVV2	1062	1582	0.10%	0.012%
18	8.293	878	885	898	rBV	109008	193465	12.32%	1.414%
19	8.740	954	961	976	rBV	196612	349401	22.25%	2.554%
20	9.451	1075	1082	1092	rBV	160610	274651	17.49%	2.007%
21	9.981	1166	1172	1191	rBV	185388	380787	24.24%	2.783%
22	10.351	1227	1235	1248	rBV	309904	523963	33.36%	3.830%
23	10.516	1253	1263	1284	rBV	140557	349282	22.24%	2.553%
24	10.798	1308	1311	1315	rVB3	1567	2575	0.16%	0.019%
25	10.845	1315	1319	1321	rBV3	1346	1881	0.12%	0.014%
26	11.981	1509	1512	1521	rVB6	2616	4771	0.30%	0.035%
27	12.133	1536	1538	1541	rBV3	1199	1600	0.10%	0.012%
28	13.128	1704	1707	1710	rVV4	2500	3294	0.21%	0.024%
29	13.663	1791	1798	1811	rBV	386856	595692	37.93%	4.354%
30	13.922	1835	1842	1855	rBV	507217	740616	47.16%	5.413%
31	14.227	1888	1894	1903	rBV	447190	645717	41.11%	4.720%
32	14.463	1924	1934	1942	rBV	245921	528458	33.65%	3.862%
33	14.533	1942	1946	1949	rVV5	5186	9954	0.63%	0.073%
34	14.574	1951	1953	1957	rVB5	2519	3281	0.21%	0.024%
35	14.680	1968	1971	1976	rBV5	1441	2612	0.17%	0.019%
36	15.010	2024	2027	2034	rVB7	2567	5311	0.34%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045291.D
 Acq On : 16 Apr 2024 21:18
 Operator : MA/JU
 Sample : P2098-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.086	2037	2040	2043	rBV3	1355	1662	0.11%	0.012%
38	15.233	2059	2065	2076	rVB	646648	939291	59.80%	6.865%
39	15.380	2084	2090	2098	rBV	173273	264561	16.84%	1.934%
40	15.480	2104	2107	2111	rVB4	1883	2745	0.17%	0.020%
41	15.921	2178	2182	2184	rBV2	1300	1630	0.10%	0.012%
42	16.027	2196	2200	2204	rBV4	1666	1802	0.11%	0.013%
43	16.427	2265	2268	2271	rBV3	2162	2257	0.14%	0.016%
44	16.780	2326	2328	2330	rBV2	1537	1593	0.10%	0.012%
45	16.804	2330	2332	2337	rVV5	1828	1842	0.12%	0.013%
46	16.992	2358	2364	2372	rBV	552356	734577	46.77%	5.369%
47	17.092	2375	2381	2398	rBV	761689	1108805	70.60%	8.104%
48	17.415	2432	2436	2439	rBV3	1275	2421	0.15%	0.018%
49	17.686	2478	2482	2486	rBV5	3158	4536	0.29%	0.033%
50	17.780	2493	2498	2502	rBV5	1224	2135	0.14%	0.016%
51	17.857	2508	2511	2515	rBV4	1028	1863	0.12%	0.014%
52	17.904	2515	2519	2527	rVV5	22412	36324	2.31%	0.265%
53	18.051	2540	2544	2546	rBV3	1463	1668	0.11%	0.012%
54	18.451	2608	2612	2613	rBV4	1684	1889	0.12%	0.014%
55	18.468	2613	2615	2618	rVV3	1985	2482	0.16%	0.018%
56	18.521	2622	2624	2626	rVV3	2031	1699	0.11%	0.012%
57	18.780	2664	2668	2669	rBV4	2192	2310	0.15%	0.017%
58	18.839	2675	2678	2679	rBV3	1997	2066	0.13%	0.015%
59	18.868	2679	2683	2686	rVB3	11327	12107	0.77%	0.088%
60	18.962	2696	2699	2703	rVB5	6909	9014	0.57%	0.066%
61	19.009	2703	2707	2708	rBV4	3915	4112	0.26%	0.030%
62	19.039	2708	2712	2715	rBV2	6215	8649	0.55%	0.063%
63	19.198	2732	2739	2743	rBV6	21165	32795	2.09%	0.240%
64	19.398	2767	2773	2784	rBV	943385	1270151	80.87%	9.284%
65	19.527	2793	2795	2797	rBV3	1995	1805	0.11%	0.013%
66	21.203	3075	3080	3091	rBV	602408	856286	54.52%	6.259%
67	23.262	3424	3430	3438	rBV	880995	1570591	100.00%	11.479%
68	23.403	3448	3454	3470	rVB	537731	1048641	66.77%	7.665%


Sum of corrected areas: 13681772

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045291.D
Acq On : 16 Apr 2024 21:18
Operator : MA/JU
Sample : P2098-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CORA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

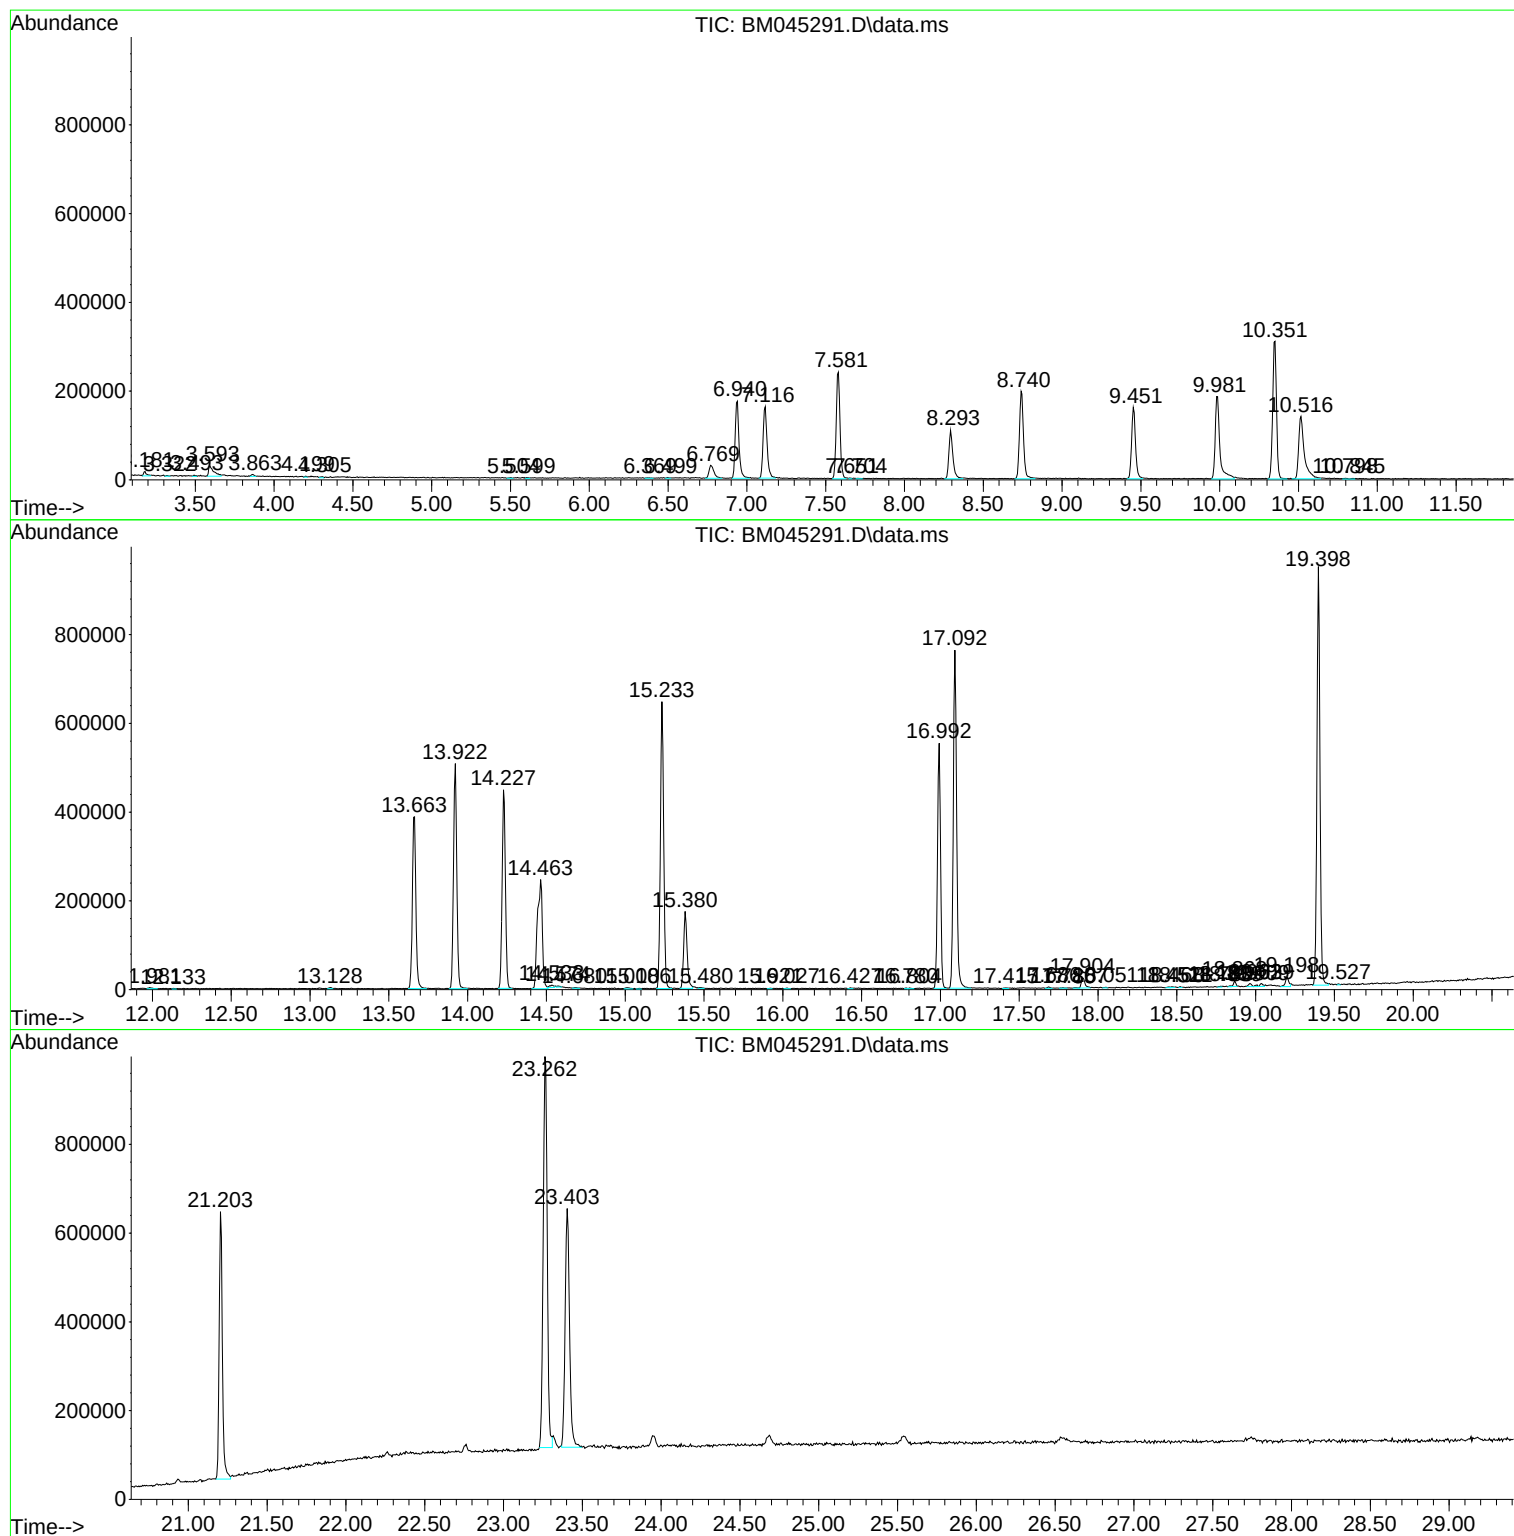

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045291.D
Acq On : 16 Apr 2024 21:18
Operator : MA/JU
Sample : P2098-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CORA1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.463	16.37 ng/ul	528458	Acenaphthene-d10	14.227

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Tetradecanol acetate	256	C16H32O2	051354-23-5	37
2			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	32
3			4-Dodecanol, acetate	228	C14H28O2	060826-25-7	17
4			2-Pentanol, 2-methyl-, acetate	144	C8H16O2	034859-98-8	12
5			1,3-Dioxolane-4-carboxaldehyde, ...	130	C6H10O3	015186-48-8	12

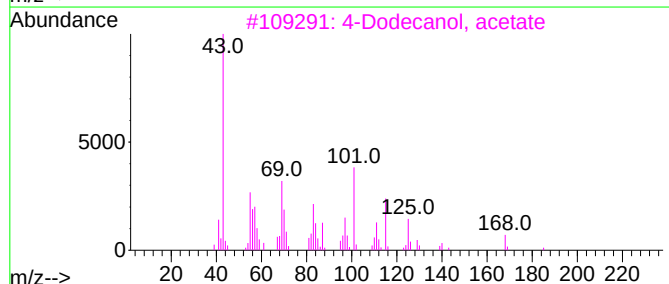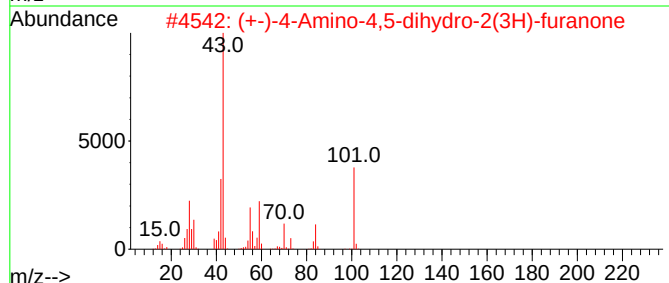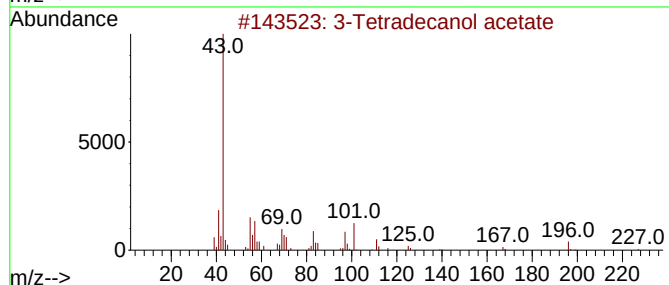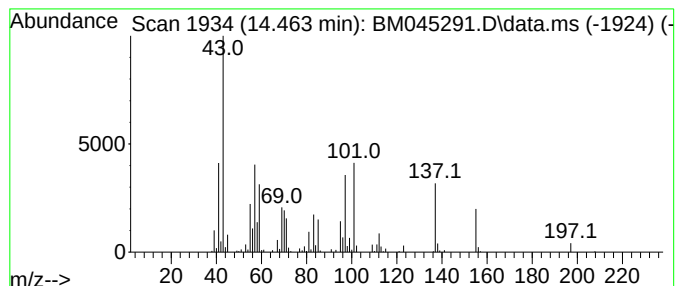

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045291.D
Acq On : 16 Apr 2024 21:18
Operator : MA/JU
Sample : P2098-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	14.463	16.4	ng/u1	528458	3	14.227	645717	20.0