

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045295.D
 Acq On : 17 Apr 2024 00:22
 Operator : MA/JU
 Sample : PB160240BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	5	6	9	rVB2	2270	1283	0.11%	0.010%
2	3.175	12	15	21	rBV	13336	20034	1.66%	0.161%
3	3.575	80	83	102	rBV	148340	267512	22.20%	2.150%
4	3.863	130	132	139	rVB6	4135	6589	0.55%	0.053%
5	3.940	143	145	147	rVB2	1756	1240	0.10%	0.010%
6	4.346	212	214	216	rBV2	1880	1743	0.14%	0.014%
7	4.369	216	218	221	rVV3	1715	1724	0.14%	0.014%
8	4.575	252	253	260	rBV4	1404	2285	0.19%	0.018%
9	4.846	294	299	300	rVV5	1525	1494	0.12%	0.012%
10	5.040	329	332	333	rBV3	1611	1481	0.12%	0.012%
11	5.140	345	349	352	rVB4	1533	2239	0.19%	0.018%
12	5.210	358	361	362	rVB2	1988	1644	0.14%	0.013%
13	5.275	368	372	373	rVB3	1426	1244	0.10%	0.010%
14	5.322	378	380	383	rVV3	1226	1293	0.11%	0.010%
15	5.393	389	392	395	rVB5	1082	1270	0.11%	0.010%
16	5.487	405	408	411	rBV4	1362	1492	0.12%	0.012%
17	5.657	436	437	441	rVB2	2020	1345	0.11%	0.011%
18	5.704	443	445	448	rVB3	1461	1421	0.12%	0.011%
19	5.769	454	456	458	rBV	1231	1251	0.10%	0.010%
20	5.799	460	461	464	rBV2	1677	1885	0.16%	0.015%
21	6.075	505	508	510	rVB4	1437	1371	0.11%	0.011%
22	6.210	528	531	533	rBV3	1374	1352	0.11%	0.011%
23	6.328	548	551	553	rBV3	1221	1339	0.11%	0.011%
24	6.763	619	625	636	rVV	190225	342758	28.45%	2.754%
25	6.840	636	638	639	rVB2	1809	1289	0.11%	0.010%
26	6.934	648	654	666	rBV	171195	286090	23.75%	2.299%
27	7.034	668	671	673	rVB4	1676	1917	0.16%	0.015%
28	7.110	678	684	697	rVB	216192	370006	30.71%	2.973%
29	7.334	721	722	726	rVB3	1439	1380	0.11%	0.011%
30	7.393	730	732	734	rBV2	1787	1411	0.12%	0.011%
31	7.575	756	763	774	rBV	217547	367862	30.53%	2.956%
32	8.110	852	854	857	rVB4	1101	1299	0.11%	0.010%
33	8.287	877	884	902	rBV	230726	420849	34.93%	3.382%
34	8.404	902	904	906	rVV3	1852	1627	0.14%	0.013%
35	8.428	906	908	910	rVV3	1451	1262	0.10%	0.010%
36	8.481	914	917	920	rBV4	1137	1321	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045295.D
 Acq On : 17 Apr 2024 00:22
 Operator : MA/JU
 Sample : PB160240BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	8.740	955	961	973	rBV	193179	338872	28.13%	2.723%
38	9.281	1049	1053	1055	rVV3	1083	1314	0.11%	0.011%
39	9.316	1055	1059	1061	rVB2	1325	1660	0.14%	0.013%
40	9.451	1076	1082	1094	rBV	162058	283447	23.53%	2.278%
41	9.534	1094	1096	1099	rVV4	1949	2499	0.21%	0.020%
42	9.563	1099	1101	1104	rVB3	1345	1321	0.11%	0.011%
43	9.716	1122	1127	1128	rBV3	1116	1416	0.12%	0.011%
44	9.981	1166	1172	1191	rBV	206209	407343	33.81%	3.273%
45	10.345	1227	1234	1243	rBV	280993	479174	39.77%	3.851%
46	10.404	1243	1244	1248	rVB4	1349	1272	0.11%	0.010%
47	10.510	1255	1262	1283	rBV	166502	418439	34.73%	3.362%
48	10.763	1303	1305	1309	rVB3	1041	1282	0.11%	0.010%
49	11.433	1415	1419	1421	rVV4	1388	1473	0.12%	0.012%
50	11.910	1498	1500	1503	rVB2	1589	1655	0.14%	0.013%
51	11.975	1509	1511	1512	rBV	2734	1996	0.17%	0.016%
52	11.992	1512	1514	1518	rVB3	2351	2827	0.23%	0.023%
53	12.128	1533	1537	1540	rBV3	905	1406	0.12%	0.011%
54	12.992	1680	1684	1687	rVB3	1112	1839	0.15%	0.015%
55	13.045	1687	1693	1694	rBV3	1049	1397	0.12%	0.011%
56	13.069	1694	1697	1700	rVV4	958	1401	0.12%	0.011%
57	13.127	1705	1707	1712	rBV4	1871	2824	0.23%	0.023%
58	13.463	1760	1764	1768	rBV3	941	1526	0.13%	0.012%
59	13.522	1772	1774	1777	rVB2	1200	1450	0.12%	0.012%
60	13.557	1777	1780	1782	rBV2	1171	1247	0.10%	0.010%
61	13.657	1791	1797	1811	rVV	358415	563012	46.73%	4.524%
62	13.922	1834	1842	1850	rBV	469061	702285	58.29%	5.643%
63	14.227	1888	1894	1902	rVV	396389	590526	49.02%	4.745%
64	14.480	1931	1937	1961	rVV	62585	202444	16.80%	1.627%
65	14.651	1965	1966	1970	rVB4	3174	2692	0.22%	0.022%
66	15.151	2046	2051	2053	rBV4	896	1302	0.11%	0.010%
67	15.233	2058	2065	2076	rVV	583749	853645	70.86%	6.860%
68	15.380	2084	2090	2100	rBV	128354	203336	16.88%	1.634%
69	15.480	2105	2107	2109	rVB3	1862	1730	0.14%	0.014%
70	15.580	2122	2124	2128	rBV3	1027	1533	0.13%	0.012%
71	16.021	2198	2199	2203	rVB3	2080	1329	0.11%	0.011%
72	16.557	2288	2290	2292	rVV2	1633	1471	0.12%	0.012%
73	16.792	2328	2330	2335	rVB4	1115	1384	0.11%	0.011%
74	16.992	2356	2364	2372	rBV	461313	640833	53.19%	5.150%
75	17.092	2374	2381	2394	rVB	581481	866601	71.93%	6.964%
76	17.210	2399	2401	2405	rVB3	1079	1410	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045295.D
 Acq On : 17 Apr 2024 00:22
 Operator : MA/JU
 Sample : PB160240BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.874	2511	2514	2518	rBV4	1062	1343	0.11%	0.011%
78	17.921	2518	2522	2523	rBV4	1311	1537	0.13%	0.012%
79	18.174	2563	2565	2568	rVB3	2127	1847	0.15%	0.015%
80	18.198	2568	2569	2572	rBV3	1342	1403	0.12%	0.011%
81	18.274	2580	2582	2585	rVB2	1880	1928	0.16%	0.015%
82	18.333	2590	2592	2595	rBV4	1816	1675	0.14%	0.013%
83	18.427	2605	2608	2610	rVB4	1313	1328	0.11%	0.011%
84	18.574	2631	2633	2636	rVB4	1041	1220	0.10%	0.010%
85	18.604	2636	2638	2640	rBV2	1219	1522	0.13%	0.012%
86	18.774	2663	2667	2669	rBV5	1357	2156	0.18%	0.017%
87	18.962	2695	2699	2704	rBV5	6370	11835	0.98%	0.095%
88	19.033	2709	2711	2715	rVV3	4029	4322	0.36%	0.035%
89	19.121	2723	2726	2727	rBV2	1456	1687	0.14%	0.014%
90	19.215	2740	2742	2745	rVB4	1656	1561	0.13%	0.013%
91	19.280	2750	2753	2755	rBV4	2103	1758	0.15%	0.014%
92	19.398	2767	2773	2786	rVV	695656	953747	79.17%	7.664%
93	19.504	2790	2791	2794	rVB3	2523	1496	0.12%	0.012%
94	19.533	2794	2796	2799	rBV4	1624	2148	0.18%	0.017%
95	19.680	2819	2821	2824	rBV4	2083	1596	0.13%	0.013%
96	19.851	2849	2850	2851	rBV	3383	1603	0.13%	0.013%
97	20.133	2896	2898	2901	rBV4	2459	2936	0.24%	0.024%
98	21.203	3075	3080	3090	rBV	458555	675325	56.06%	5.427%
99	23.262	3423	3430	3437	rBV	664176	1204741	100.00%	9.681%
100	23.397	3447	3453	3468	rVB	409269	845446	70.18%	6.794%




Sum of corrected areas: 12444375

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045295.D
Acq On : 17 Apr 2024 00:22
Operator : MA/JU
Sample : PB160240BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

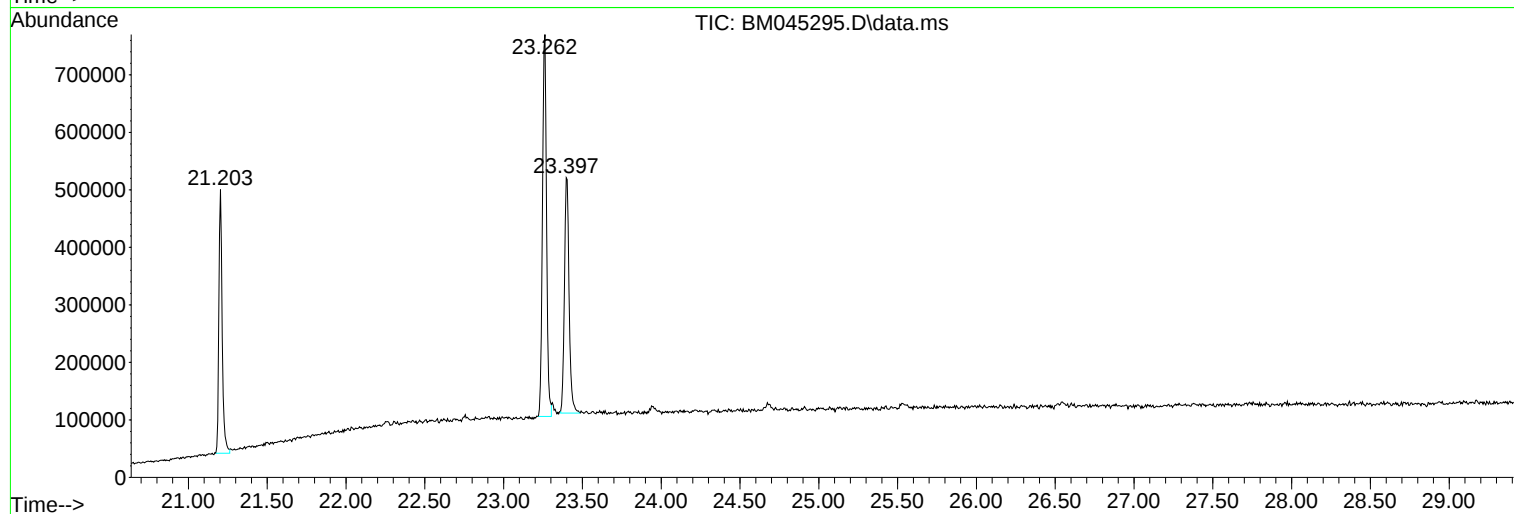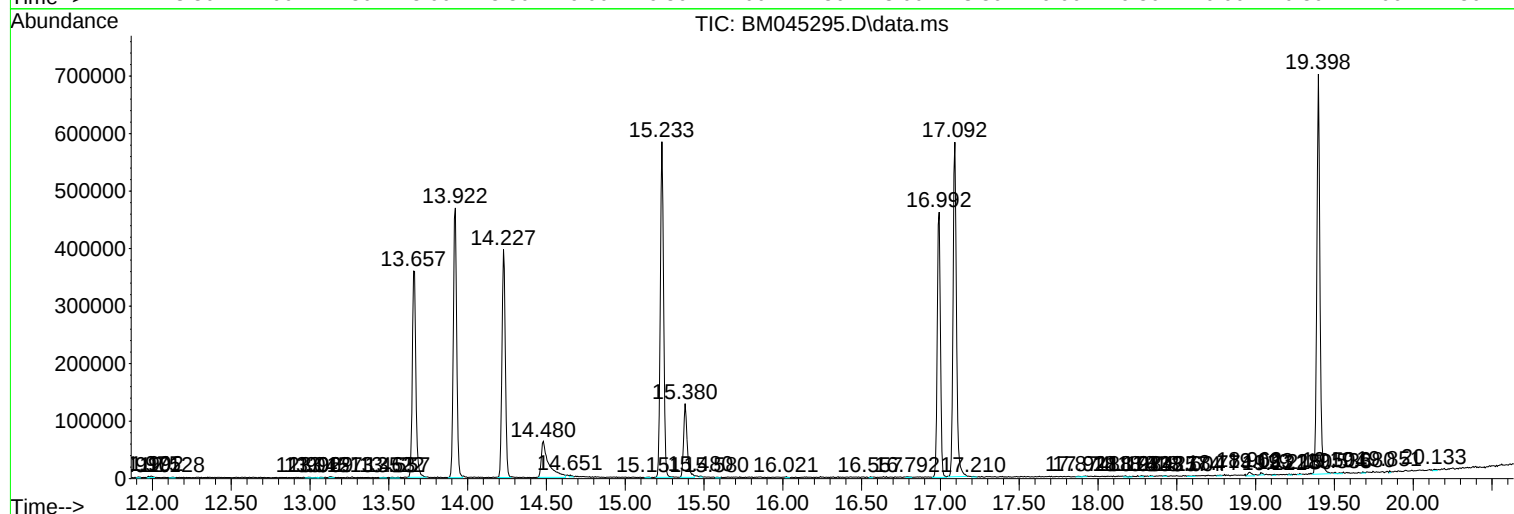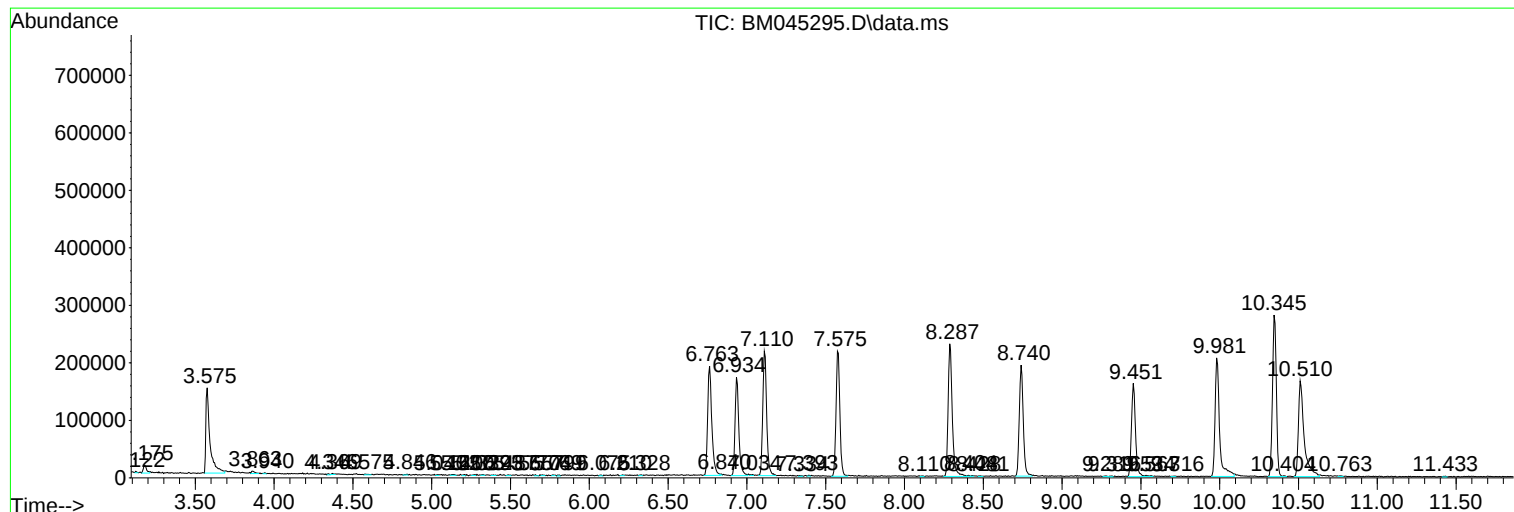

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045295.D
Acq On : 17 Apr 2024 00:22
Operator : MA/JU
Sample : PB160240BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045295.D
Acq On : 17 Apr 2024 00:22
Operator : MA/JU
Sample : PB160240BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK240

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc