

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045296.D
 Acq On : 17 Apr 2024 00:59
 Operator : MA/JU
 Sample : PB160241BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	21	rBV	15668	20069	1.65%	0.165%
2	3.322	38	40	42	rBV3	1613	1341	0.11%	0.011%
3	3.358	44	46	48	rBV3	1414	1631	0.13%	0.013%
4	3.569	80	82	98	rBV	150590	272024	22.32%	2.237%
5	3.775	115	117	119	rBV3	2020	1379	0.11%	0.011%
6	3.816	121	124	125	rBV2	1972	1647	0.14%	0.014%
7	3.869	130	133	136	rVB4	2737	3040	0.25%	0.025%
8	4.210	188	191	194	rVV4	1478	1993	0.16%	0.016%
9	4.352	212	215	217	rBV4	1562	2036	0.17%	0.017%
10	4.752	281	283	286	rVV4	1227	1245	0.10%	0.010%
11	4.840	296	298	301	rVV4	1532	1375	0.11%	0.011%
12	4.869	301	303	307	rVV5	1548	1377	0.11%	0.011%
13	4.928	309	313	316	rVB5	1624	2324	0.19%	0.019%
14	4.963	316	319	321	rBV4	1052	1307	0.11%	0.011%
15	5.075	336	338	341	rBV4	1687	1603	0.13%	0.013%
16	5.375	387	389	390	rVB2	2010	1246	0.10%	0.010%
17	5.610	427	429	432	rBV2	1626	1652	0.14%	0.014%
18	5.634	432	433	438	rVB4	1218	1299	0.11%	0.011%
19	6.051	502	504	506	rBV3	1582	1404	0.12%	0.012%
20	6.134	514	518	519	rBV4	987	1294	0.11%	0.011%
21	6.451	569	572	574	rBV4	1870	2041	0.17%	0.017%
22	6.587	591	595	596	rBV4	1354	1591	0.13%	0.013%
23	6.628	601	602	604	rBV3	2225	1677	0.14%	0.014%
24	6.651	604	606	612	rVB6	1436	1460	0.12%	0.012%
25	6.763	619	625	638	rBV	204905	364586	29.92%	2.998%
26	6.934	648	654	665	rBV	178753	290383	23.83%	2.388%
27	7.010	665	667	672	rVB4	1974	2595	0.21%	0.021%
28	7.110	678	684	697	rVB	232796	383202	31.45%	3.151%
29	7.369	726	728	731	rVB4	1739	1827	0.15%	0.015%
30	7.575	757	763	771	rVV	193101	312484	25.64%	2.570%
31	8.287	877	884	900	rBV	250509	432027	35.45%	3.553%
32	8.534	922	926	931	rBV6	1431	2326	0.19%	0.019%
33	8.740	954	961	971	rBV	204702	345495	28.35%	2.841%
34	9.104	1019	1023	1027	rVB3	901	1264	0.10%	0.010%
35	9.316	1056	1059	1060	rBV2	1369	1371	0.11%	0.011%
36	9.451	1075	1082	1094	rBV	167021	287182	23.57%	2.362%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045296.D
 Acq On : 17 Apr 2024 00:59
 Operator : MA/JU
 Sample : PB160241BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	9.981	1166	1172	1183	rBV	219835	401134	32.92%	3.299%
38	10.198	1207	1209	1211	rVB	1535	1230	0.10%	0.010%
39	10.345	1227	1234	1245	rBV	248450	414559	34.02%	3.409%
40	10.510	1254	1262	1281	rBV	174002	426904	35.03%	3.511%
41	10.663	1285	1288	1289	rVV3	1444	1683	0.14%	0.014%
42	11.363	1404	1407	1409	rBV2	1361	1395	0.11%	0.011%
43	11.598	1446	1447	1451	rVB2	1450	1245	0.10%	0.010%
44	11.639	1451	1454	1458	rBV3	1075	1573	0.13%	0.013%
45	11.986	1508	1513	1518	rVB4	2029	4039	0.33%	0.033%
46	13.127	1701	1707	1713	rBV6	2146	4534	0.37%	0.037%
47	13.557	1776	1780	1782	rBV	986	1288	0.11%	0.011%
48	13.657	1791	1797	1810	rBV	383477	584399	47.96%	4.806%
49	13.922	1835	1842	1853	rBV	486184	728430	59.77%	5.991%
50	14.227	1888	1894	1905	rVB	356451	510847	41.92%	4.201%
51	14.474	1930	1936	1948	rBV2	65197	185317	15.21%	1.524%
52	14.657	1966	1967	1969	rVB2	2411	1421	0.12%	0.012%
53	14.674	1969	1970	1974	rVV3	1642	1755	0.14%	0.014%
54	14.733	1977	1980	1983	rVB4	1288	1281	0.11%	0.011%
55	15.233	2059	2065	2075	rVV	598075	899974	73.85%	7.401%
56	15.310	2075	2078	2083	rVV6	1364	2517	0.21%	0.021%
57	15.380	2083	2090	2102	rVV	136244	218907	17.96%	1.800%
58	15.474	2104	2106	2113	rVB5	2403	4365	0.36%	0.036%
59	15.804	2158	2162	2167	rBV5	1030	2048	0.17%	0.017%
60	16.027	2197	2200	2202	rBV3	1261	1535	0.13%	0.013%
61	16.339	2248	2253	2255	rBV2	1052	1454	0.12%	0.012%
62	16.992	2357	2364	2372	rVV	381187	539868	44.30%	4.440%
63	17.092	2375	2381	2399	rVB2	604459	916868	75.24%	7.540%
64	17.657	2473	2477	2478	rBV3	1287	1693	0.14%	0.014%
65	17.727	2486	2489	2490	rBV2	1213	1356	0.11%	0.011%
66	18.280	2580	2583	2588	rVV4	1055	1847	0.15%	0.015%
67	18.339	2590	2593	2595	rVV3	1298	1401	0.11%	0.012%
68	18.474	2612	2616	2617	rBV2	1457	1474	0.12%	0.012%
69	18.521	2619	2624	2627	rVV5	832	1307	0.11%	0.011%
70	18.604	2636	2638	2640	rBV3	1262	1254	0.10%	0.010%
71	18.868	2679	2683	2684	rBV3	1510	1443	0.12%	0.012%
72	18.909	2688	2690	2692	rBV3	1398	1292	0.11%	0.011%
73	18.962	2695	2699	2702	rBV	5709	6503	0.53%	0.053%
74	19.039	2709	2712	2716	rBV2	3393	4901	0.40%	0.040%
75	19.174	2732	2735	2736	rBV2	1577	1280	0.11%	0.011%
76	19.215	2738	2742	2743	rVV2	1097	1256	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045296.D
Acq On : 17 Apr 2024 00:59
Operator : MA/JU
Sample : PB160241BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	19.286	2751	2754	2755	rBV3	1708	1600	0.13%	0.013%
78	19.398	2767	2773	2787	rVV	710407	993066	81.49%	8.167%
79	19.604	2806	2808	2811	rBV3	2371	2962	0.24%	0.024%
80	19.968	2868	2870	2871	rBV2	1884	1610	0.13%	0.013%
81	20.245	2913	2917	2919	rBV5	3008	3506	0.29%	0.029%
82	21.203	3075	3080	3090	rBV2	381107	584122	47.93%	4.804%
83	23.262	3423	3430	3438	rBV2	686567	1218628	100.00%	10.022%
84	23.397	3447	3453	3465	rBV	350728	713790	58.57%	5.870%




Sum of corrected areas: 12159658

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045296.D
Acq On : 17 Apr 2024 00:59
Operator : MA/JU
Sample : PB160241BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

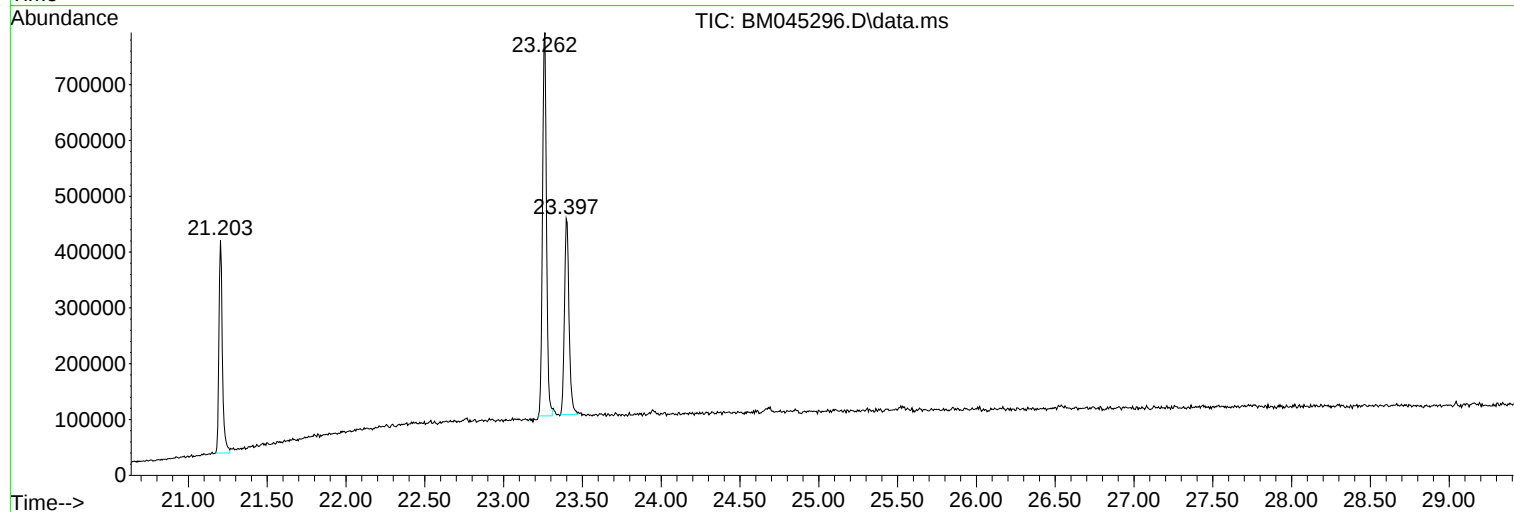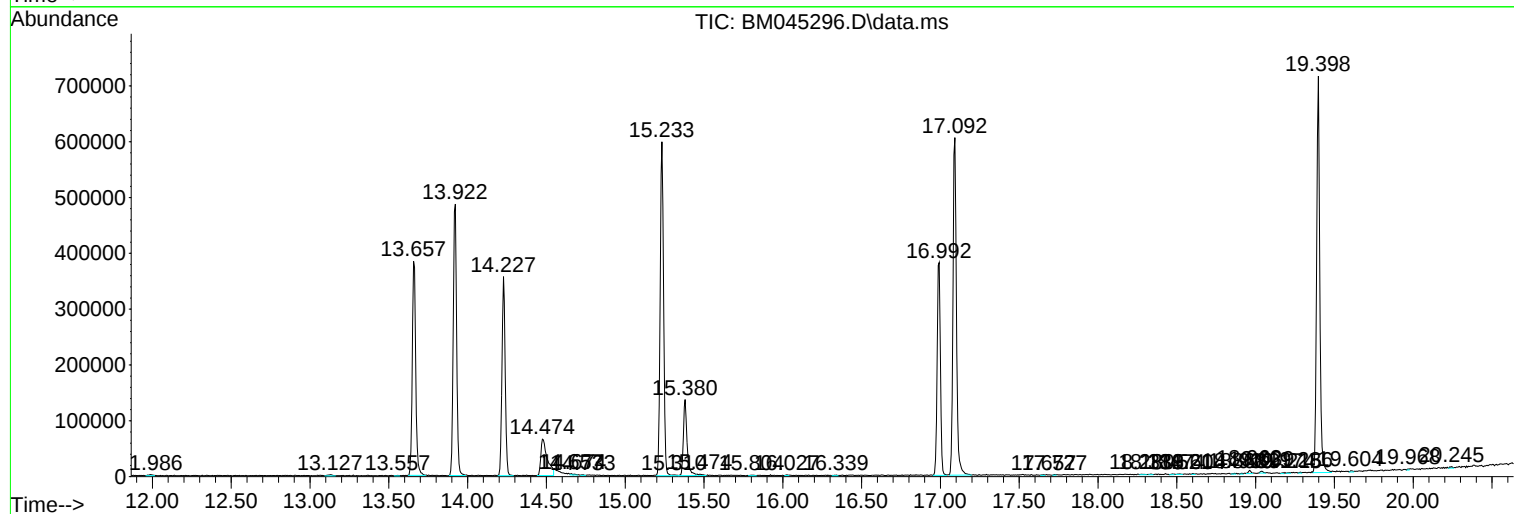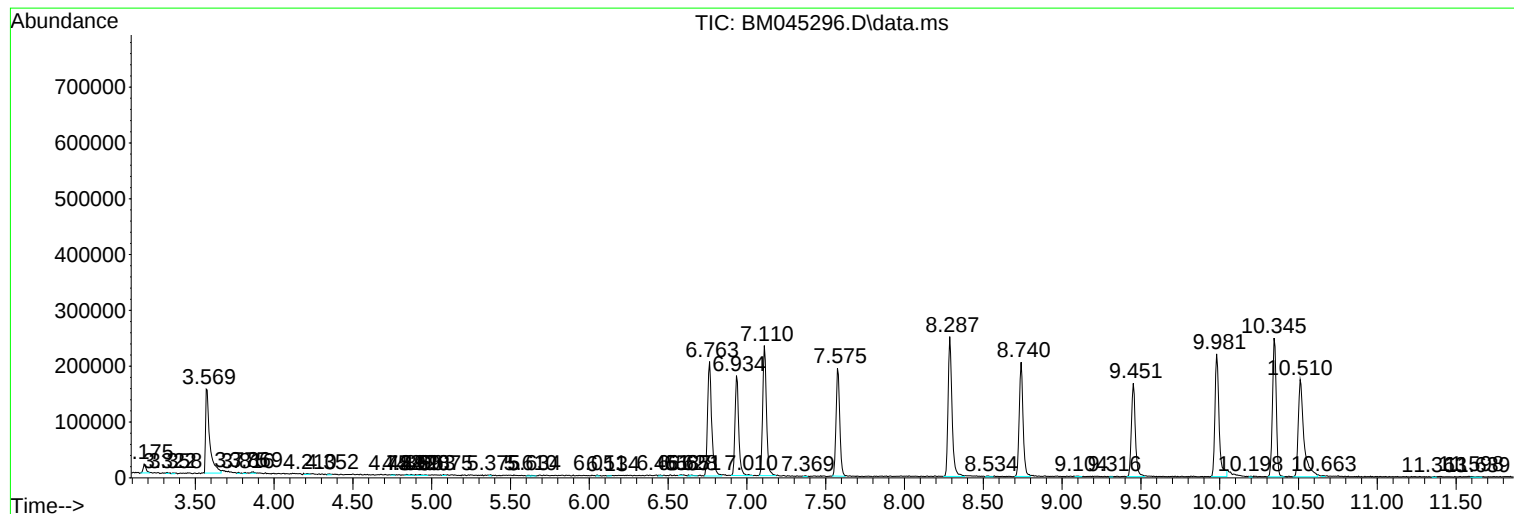

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045296.D
Acq On : 17 Apr 2024 00:59
Operator : MA/JU
Sample : PB160241BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045296.D
Acq On : 17 Apr 2024 00:59
Operator : MA/JU
Sample : PB160241BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------