

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045299.D
 Acq On : 17 Apr 2024 02:48
 Operator : MA/JU
 Sample : P2099-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	22	rBV3	10614	15604	0.79%	0.109%
2	3.587	82	85	97	rBV	33999	69686	3.54%	0.488%
3	3.863	129	132	136	rBV5	3181	4179	0.21%	0.029%
4	4.945	313	316	320	rBV6	4842	7202	0.37%	0.050%
5	5.281	370	373	376	rBV4	1470	2359	0.12%	0.017%
6	5.640	432	434	437	rVB2	2400	2527	0.13%	0.018%
7	5.740	448	451	454	rBV3	1545	2029	0.10%	0.014%
8	6.116	510	515	517	rBV4	1674	2848	0.14%	0.020%
9	6.669	607	609	613	rVB4	1903	2207	0.11%	0.015%
10	6.769	619	626	636	rBV	33812	65784	3.34%	0.461%
11	6.934	648	654	670	rVB	179584	299925	15.23%	2.101%
12	7.110	678	684	697	rBV	168297	289302	14.69%	2.027%
13	7.575	757	763	775	rVB	211246	344331	17.48%	2.412%
14	8.286	878	884	896	rBV	110063	205290	10.42%	1.438%
15	8.739	953	961	973	rBV	215717	367315	18.65%	2.573%
16	8.816	973	974	979	rVB3	2111	2650	0.13%	0.019%
17	9.192	1033	1038	1041	rBV4	1590	2346	0.12%	0.016%
18	9.451	1074	1082	1093	rBV	165919	291114	14.78%	2.040%
19	9.980	1165	1172	1191	rBV	191138	402464	20.44%	2.820%
20	10.345	1226	1234	1243	rBV	272843	459995	23.36%	3.223%
21	10.516	1257	1263	1288	rBV2	84525	227601	11.56%	1.595%
22	10.869	1320	1323	1327	rBV5	1302	2292	0.12%	0.016%
23	11.763	1470	1475	1482	rBV5	4891	8718	0.44%	0.061%
24	11.980	1508	1512	1514	rBV3	2081	2970	0.15%	0.021%
25	13.051	1689	1694	1702	rBV3	21410	32754	1.66%	0.229%
26	13.121	1702	1706	1712	rVB4	2862	4520	0.23%	0.032%
27	13.257	1724	1729	1734	rVB2	9467	15405	0.78%	0.108%
28	13.657	1791	1797	1807	rBV	473045	682703	34.67%	4.783%
29	13.915	1834	1841	1852	rBV	555825	828448	42.07%	5.804%
30	14.004	1853	1856	1865	rVB5	3677	6639	0.34%	0.047%
31	14.227	1885	1894	1904	rBV	424595	606859	30.82%	4.252%
32	14.533	1939	1946	1948	rBV5	7787	17528	0.89%	0.123%
33	15.233	2055	2065	2073	rBV	693394	1049107	53.27%	7.350%
34	15.309	2074	2078	2084	rVB3	8617	11157	0.57%	0.078%
35	15.374	2084	2089	2102	rBV	204652	315270	16.01%	2.209%
36	16.021	2197	2199	2203	rBV3	2589	2086	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045299.D
 Acq On : 17 Apr 2024 02:48
 Operator : MA/JU
 Sample : P2099-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	16.786	2324	2329	2333	rBV4	1877	3063	0.16%	0.021%
38	16.986	2358	2363	2371	rVV	512339	725319	36.83%	5.082%
39	17.086	2374	2380	2396	rVV2	805666	1240555	62.99%	8.691%
40	17.415	2434	2436	2439	rBV3	1945	1980	0.10%	0.014%
41	17.692	2479	2483	2487	rVB4	1610	2292	0.12%	0.016%
42	17.903	2513	2519	2527	rBV3	40123	63587	3.23%	0.445%
43	18.003	2533	2536	2542	rVB3	14015	18117	0.92%	0.127%
44	18.221	2569	2573	2575	rBV5	2542	2493	0.13%	0.017%
45	18.580	2630	2634	2637	rBV5	1747	3210	0.16%	0.022%
46	18.956	2694	2698	2704	rBV5	9031	14085	0.72%	0.099%
47	19.033	2707	2711	2712	rBV3	6671	7203	0.37%	0.050%
48	19.197	2734	2739	2744	rBV2	24070	34067	1.73%	0.239%
49	19.280	2752	2753	2758	rBV5	2388	3001	0.15%	0.021%
50	19.397	2766	2773	2782	rBV	1083908	1496205	75.98%	10.482%
51	19.674	2817	2820	2821	rBV2	2726	2448	0.12%	0.017%
52	19.703	2823	2825	2827	rVV3	2725	2016	0.10%	0.014%
53	20.039	2880	2882	2883	rBV2	3080	2845	0.14%	0.020%
54	20.444	2949	2951	2953	rBV3	3791	4057	0.21%	0.028%
55	20.933	3030	3034	3039	rBV6	22384	34402	1.75%	0.241%
56	21.203	3074	3080	3091	rBV	665484	904865	45.95%	6.339%
57	23.262	3422	3430	3446	rBV2	1025101	1969328	100.00%	13.797%
58	23.397	3447	3453	3463	rVB	548560	1085143	55.10%	7.603%




Sum of corrected areas: 14273495

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045299.D
Acq On : 17 Apr 2024 02:48
Operator : MA/JU
Sample : P2099-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

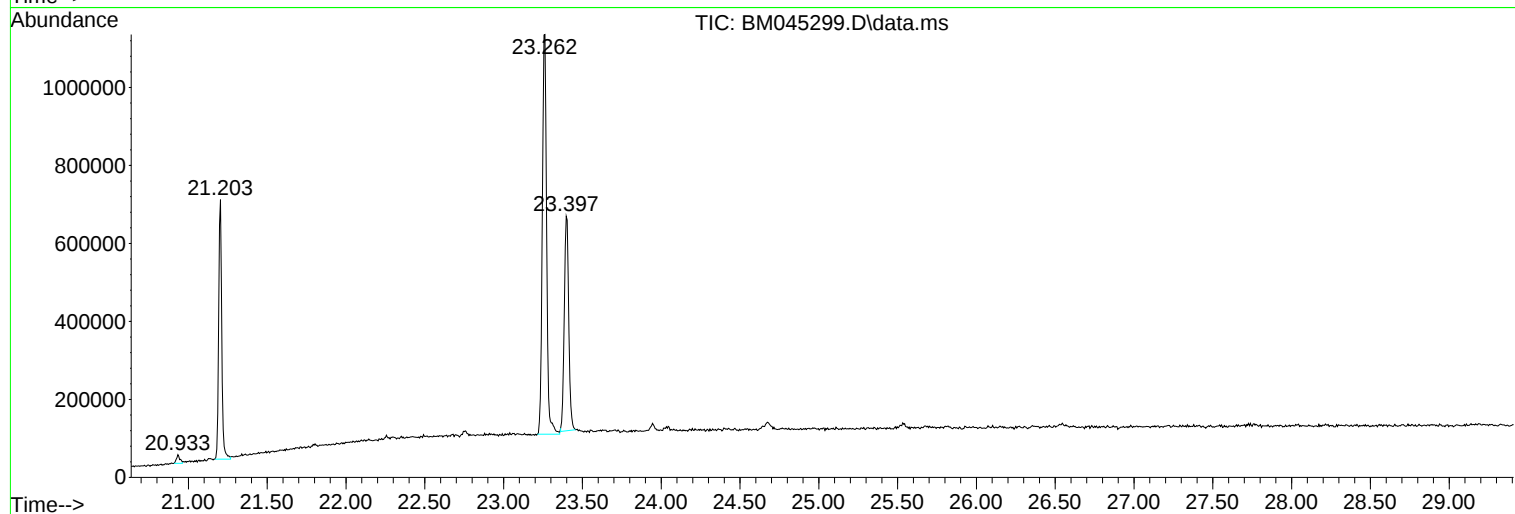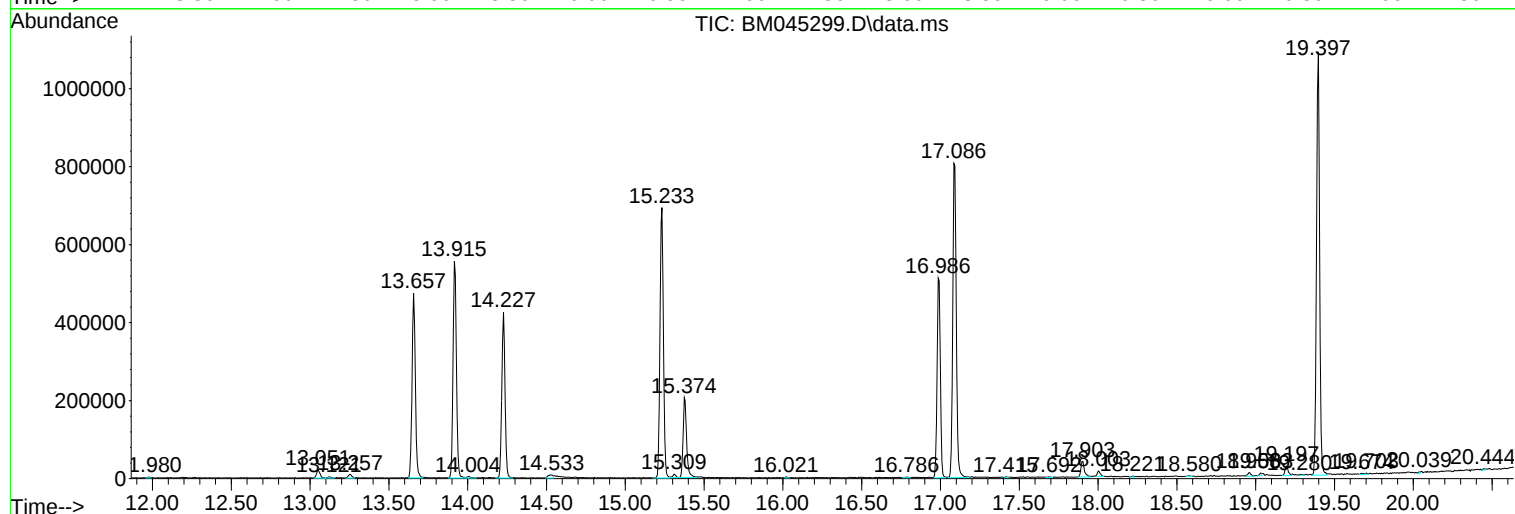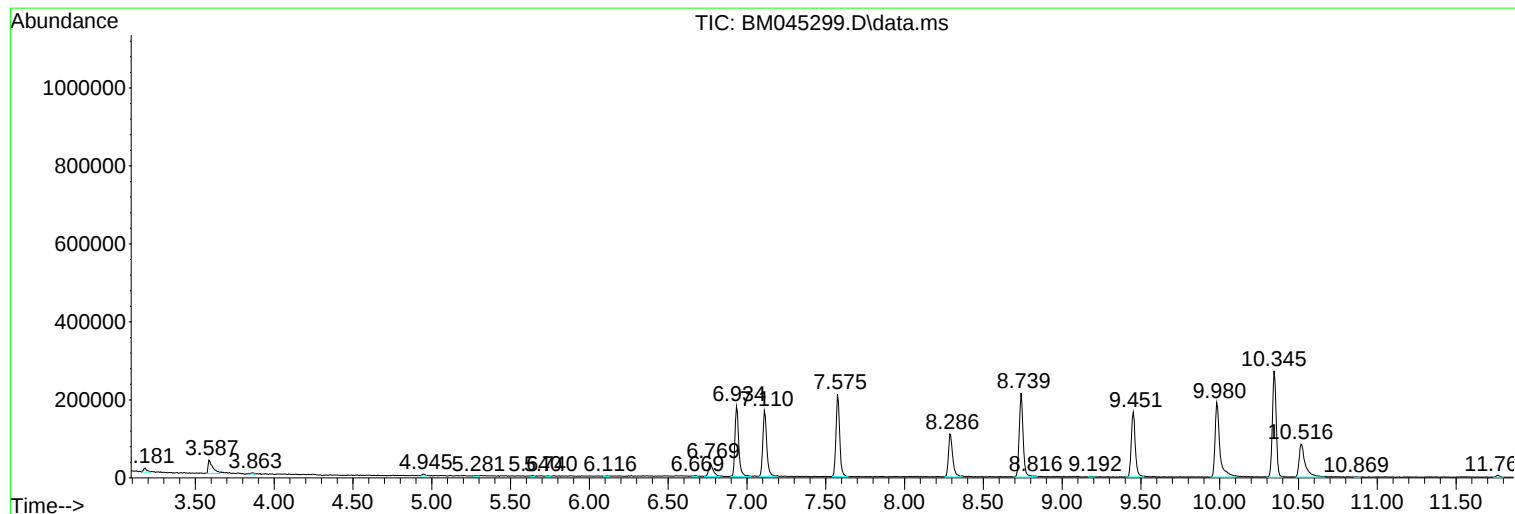

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045299.D
Acq On : 17 Apr 2024 02:48
Operator : MA/JU
Sample : P2099-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045299.D
Acq On : 17 Apr 2024 02:48
Operator : MA/JU
Sample : P2099-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc