

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045300.D
 Acq On : 17 Apr 2024 03:25
 Operator : MA/JU
 Sample : P2099-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	6	9	12	rBV4	1459	1898	0.12%	0.015%
2	3.181	12	16	22	rVV	7978	11787	0.77%	0.096%
3	3.505	69	71	74	rBV3	1491	1597	0.10%	0.013%
4	3.587	82	85	93	rBV	25911	52184	3.41%	0.423%
5	3.758	112	114	117	rVB4	2864	2854	0.19%	0.023%
6	3.869	130	133	134	rBV3	2762	2723	0.18%	0.022%
7	4.440	229	230	233	rVB3	2288	1623	0.11%	0.013%
8	4.710	274	276	279	rBV4	1583	1717	0.11%	0.014%
9	4.893	305	307	309	rBV2	1566	1587	0.10%	0.013%
10	4.934	313	314	317	rBV3	1984	1685	0.11%	0.014%
11	4.963	317	319	323	rVB5	1827	1657	0.11%	0.013%
12	5.616	428	430	433	rBV3	1336	1816	0.12%	0.015%
13	5.716	443	447	449	rBV4	1195	1723	0.11%	0.014%
14	6.093	508	511	512	rBV2	1740	1875	0.12%	0.015%
15	6.769	620	626	634	rBV2	27020	57047	3.73%	0.462%
16	6.934	648	654	666	rBV	160423	270508	17.70%	2.193%
17	7.016	666	668	672	rVB5	1544	1626	0.11%	0.013%
18	7.110	678	684	695	rBV	151413	263006	17.21%	2.132%
19	7.575	757	763	772	rVV	219609	364136	23.82%	2.952%
20	7.793	797	800	804	rBV5	1513	2403	0.16%	0.019%
21	8.293	878	885	894	rBV	94543	180644	11.82%	1.464%
22	8.740	951	961	974	rBV	185389	320667	20.98%	2.599%
23	8.910	986	990	993	rVB5	1502	1964	0.13%	0.016%
24	9.451	1075	1082	1094	rBV	152681	292769	19.15%	2.373%
25	9.987	1166	1173	1186	rBV	165478	356393	23.31%	2.889%
26	10.345	1225	1234	1243	rVV	286507	480009	31.40%	3.891%
27	10.522	1257	1264	1287	rBV3	72973	260458	17.04%	2.111%
28	11.104	1359	1363	1365	rVB2	1133	1537	0.10%	0.012%
29	11.963	1504	1509	1520	rVB3	2022	5639	0.37%	0.046%
30	13.063	1690	1696	1697	rBV4	1474	1789	0.12%	0.015%
31	13.122	1703	1706	1710	rBV2	1720	1971	0.13%	0.016%
32	13.657	1791	1797	1807	rBV	408096	589544	38.57%	4.779%
33	13.916	1835	1841	1849	rBV	466994	700783	45.84%	5.680%
34	14.227	1888	1894	1904	rBV	416653	599291	39.20%	4.858%
35	14.533	1942	1946	1947	rBV3	4894	5712	0.37%	0.046%
36	14.545	1947	1948	1954	rVV5	4080	7470	0.49%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045300.D
 Acq On : 17 Apr 2024 03:25
 Operator : MA/JU
 Sample : P2099-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORJ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.586	1954	1955	1958	rVB2	2035	2146	0.14%	0.017%
38	15.010	2022	2027	2028	rBV3	2482	3475	0.23%	0.028%
39	15.233	2057	2065	2076	rBV	615111	896052	58.62%	7.263%
40	15.380	2084	2090	2104	rBV	158724	252116	16.49%	2.044%
41	15.474	2104	2106	2110	rVB4	2899	3366	0.22%	0.027%
42	16.080	2205	2209	2213	rBV3	1123	1842	0.12%	0.015%
43	16.839	2335	2338	2344	rVB4	960	2091	0.14%	0.017%
44	16.986	2357	2363	2373	rBV	489352	677214	44.30%	5.489%
45	17.092	2374	2381	2391	rBV	699532	1035402	67.73%	8.393%
46	17.404	2432	2434	2437	rBV3	1286	1681	0.11%	0.014%
47	17.904	2514	2519	2527	rVV3	21457	34755	2.27%	0.282%
48	18.133	2556	2558	2562	rBV3	1083	1836	0.12%	0.015%
49	18.551	2627	2629	2631	rBV	1298	1563	0.10%	0.013%
50	18.845	2677	2679	2682	rBV3	1517	1853	0.12%	0.015%
51	18.962	2695	2699	2705	rVB4	6375	8640	0.57%	0.070%
52	19.039	2709	2712	2717	rVB3	5134	7782	0.51%	0.063%
53	19.133	2727	2728	2734	rVB3	1947	1535	0.10%	0.012%
54	19.198	2734	2739	2746	rBV4	20164	30824	2.02%	0.250%
55	19.398	2767	2773	2782	rVV	861436	1197175	78.32%	9.704%
56	19.509	2790	2792	2794	rBV3	1541	1634	0.11%	0.013%
57	19.598	2805	2807	2809	rBV3	1753	1659	0.11%	0.013%
58	19.768	2834	2836	2839	rBV4	2203	2637	0.17%	0.021%
59	19.962	2867	2869	2870	rBV2	2286	1722	0.11%	0.014%
60	20.209	2909	2911	2916	rVB4	3540	4627	0.30%	0.038%
61	20.927	3031	3033	3038	rBV4	8629	12775	0.84%	0.104%
62	21.203	3074	3080	3093	rBV	550776	792027	51.81%	6.420%
63	23.256	3423	3429	3438	rBV	837308	1528627	100.00%	12.391%
64	23.397	3446	3453	3463	rBV	487185	977913	63.97%	7.927%




Sum of corrected areas: 12337061

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045300.D
Acq On : 17 Apr 2024 03:25
Operator : MA/JU
Sample : P2099-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

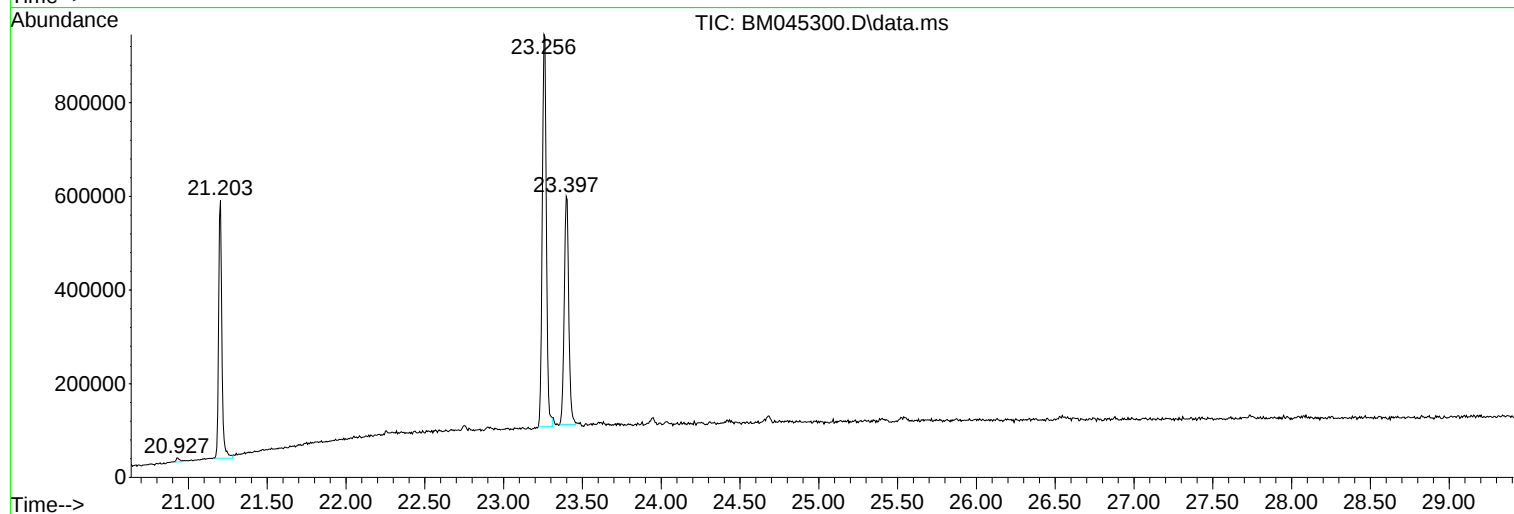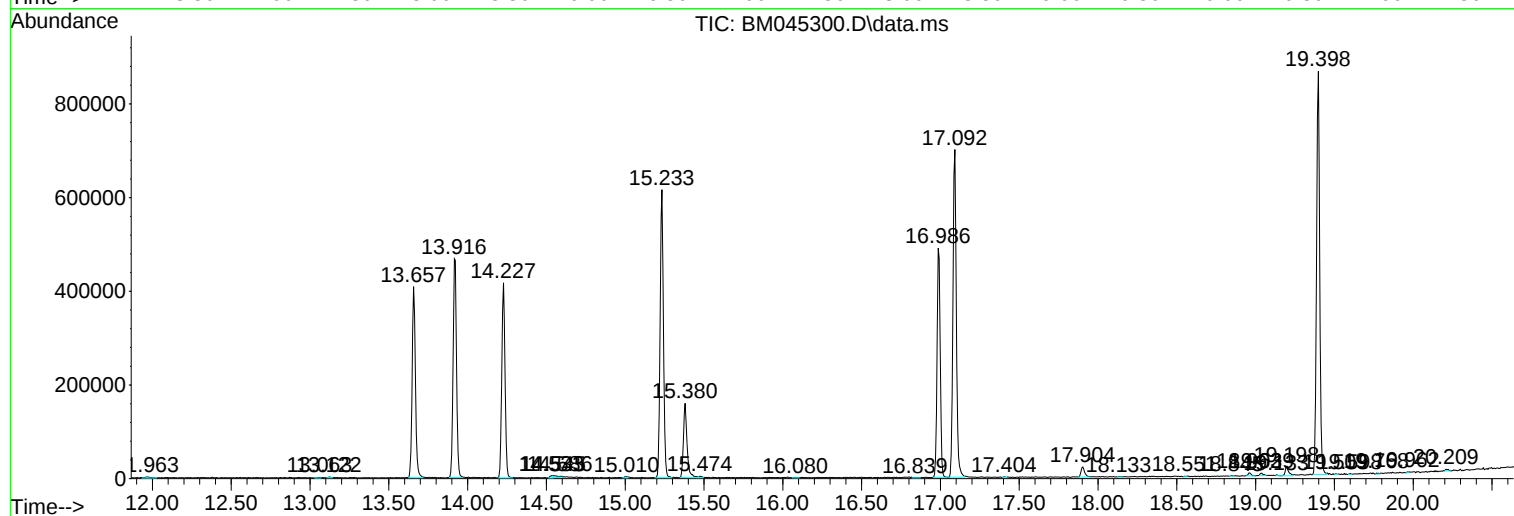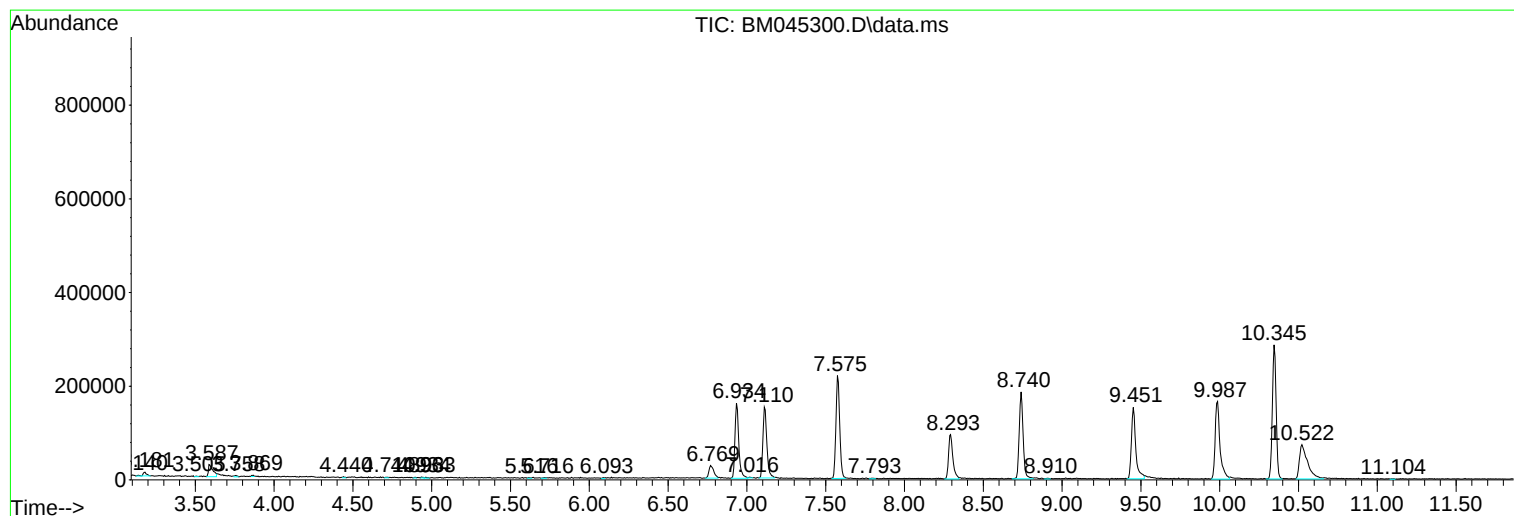

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045300.D
Acq On : 17 Apr 2024 03:25
Operator : MA/JU
Sample : P2099-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045300.D
Acq On : 17 Apr 2024 03:25
Operator : MA/JU
Sample : P2099-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc