

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045303.D
 Acq On : 17 Apr 2024 05:14
 Operator : MA/JU
 Sample : P2099-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0RA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB2	8371	10715	0.70%	0.087%
2	3.422	56	57	62	rBV5	1859	2321	0.15%	0.019%
3	3.469	64	65	68	rBV2	2012	1877	0.12%	0.015%
4	3.604	84	88	93	rBV2	10278	20610	1.35%	0.166%
5	3.710	103	106	107	rBV3	3086	2787	0.18%	0.022%
6	3.822	123	125	127	rBV2	1374	1810	0.12%	0.015%
7	3.869	129	133	136	rBV5	4173	6603	0.43%	0.053%
8	4.010	155	157	160	rVB3	3431	3094	0.20%	0.025%
9	4.040	160	162	163	rBV2	2613	2230	0.15%	0.018%
10	4.398	221	223	229	rVB5	1723	2323	0.15%	0.019%
11	4.963	318	319	324	rBV4	1158	1623	0.11%	0.013%
12	5.310	374	378	380	rBV3	2152	2320	0.15%	0.019%
13	5.675	438	440	444	rBV4	2280	3388	0.22%	0.027%
14	5.851	468	470	473	rVB3	1822	1542	0.10%	0.012%
15	6.251	535	538	542	rVV5	1212	1628	0.11%	0.013%
16	6.775	620	627	636	rBV2	27328	63243	4.13%	0.511%
17	6.934	648	654	664	rBV	181152	297929	19.46%	2.405%
18	7.110	677	684	695	rVV	168509	292308	19.09%	2.360%
19	7.187	695	697	703	rVV5	2444	4139	0.27%	0.033%
20	7.575	756	763	775	rBV	204901	342259	22.35%	2.763%
21	7.881	814	815	819	rBV4	1177	1640	0.11%	0.013%
22	8.092	846	851	852	rBV3	1330	1619	0.11%	0.013%
23	8.292	878	885	897	rBV	103176	189990	12.41%	1.534%
24	8.739	953	961	974	rBV	213468	359916	23.51%	2.906%
25	8.975	998	1001	1004	rVB4	1216	1815	0.12%	0.015%
26	9.098	1018	1022	1026	rVB3	1550	2551	0.17%	0.021%
27	9.451	1075	1082	1096	rBV	164315	290176	18.95%	2.343%
28	9.828	1141	1146	1150	rVB5	1388	2544	0.17%	0.021%
29	9.980	1165	1172	1188	rBV2	194555	387533	25.31%	3.129%
30	10.345	1227	1234	1244	rVV	261586	439680	28.72%	3.550%
31	10.516	1256	1263	1284	rBV	117353	309247	20.20%	2.497%
32	11.104	1359	1363	1367	rBV4	1289	2392	0.16%	0.019%
33	11.974	1509	1511	1518	rVB3	2309	3619	0.24%	0.029%
34	13.121	1702	1706	1707	rBV2	1807	1963	0.13%	0.016%
35	13.468	1760	1765	1769	rVB4	1374	2441	0.16%	0.020%
36	13.657	1791	1797	1808	rBV	411533	621561	40.59%	5.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045303.D
 Acq On : 17 Apr 2024 05:14
 Operator : MA/JU
 Sample : P2099-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.857	1826	1831	1834	rBV4	1006	1841	0.12%	0.015%
38	13.915	1834	1841	1850	rVV	516180	774804	50.60%	6.255%
39	13.980	1850	1852	1856	rVB2	1533	2077	0.14%	0.017%
40	14.227	1887	1894	1900	rBV	382789	545447	35.62%	4.403%
41	14.551	1942	1949	1952	rBV5	4432	11247	0.73%	0.091%
42	14.633	1962	1963	1967	rVB3	1588	1788	0.12%	0.014%
43	15.092	2038	2041	2044	rBV3	1763	2087	0.14%	0.017%
44	15.233	2056	2065	2073	rBV	618680	956837	62.49%	7.725%
45	15.380	2084	2090	2104	rBV	153251	261290	17.07%	2.109%
46	15.474	2104	2106	2110	rVB3	1804	2264	0.15%	0.018%
47	15.539	2115	2117	2119	rBV2	1717	1550	0.10%	0.013%
48	16.027	2197	2200	2203	rVB2	1600	1752	0.11%	0.014%
49	16.598	2294	2297	2303	rBV5	3436	4947	0.32%	0.040%
50	16.768	2321	2326	2329	rBV4	1027	1692	0.11%	0.014%
51	16.986	2357	2363	2374	rBV	446052	599349	39.14%	4.839%
52	17.086	2374	2380	2393	rVV	712753	1062687	69.41%	8.579%
53	17.298	2414	2416	2419	rBV4	1565	1846	0.12%	0.015%
54	17.492	2446	2449	2457	rVB6	2969	5728	0.37%	0.046%
55	17.551	2457	2459	2464	rVB3	999	1538	0.10%	0.012%
56	17.586	2464	2465	2469	rBV4	1497	2012	0.13%	0.016%
57	17.680	2480	2481	2486	rBV4	1589	2591	0.17%	0.021%
58	17.898	2510	2518	2532	rBV2	34295	58513	3.82%	0.472%
59	18.121	2553	2556	2559	rBV4	1468	1891	0.12%	0.015%
60	18.192	2567	2568	2573	rVB4	3261	2982	0.19%	0.024%
61	18.280	2579	2583	2585	rVB5	1726	2126	0.14%	0.017%
62	18.303	2585	2587	2590	rBV4	2054	2405	0.16%	0.019%
63	18.668	2647	2649	2654	rBV4	2119	2280	0.15%	0.018%
64	18.798	2666	2671	2673	rBV4	1064	1742	0.11%	0.014%
65	18.833	2675	2677	2681	rVB5	2907	3400	0.22%	0.027%
66	18.939	2693	2695	2696	rBV2	2035	1665	0.11%	0.013%
67	18.962	2696	2699	2703	rVB2	7090	8279	0.54%	0.067%
68	19.033	2707	2711	2716	rBV4	6326	12785	0.84%	0.103%
69	19.198	2733	2739	2746	rBV3	30010	47827	3.12%	0.386%
70	19.339	2762	2763	2767	rBV4	2645	2865	0.19%	0.023%
71	19.397	2767	2773	2785	rVV	870701	1228808	80.25%	9.920%
72	19.627	2809	2812	2813	rBV3	1578	1590	0.10%	0.013%
73	19.750	2831	2833	2834	rBV	2308	1640	0.11%	0.013%
74	19.874	2852	2854	2857	rVB4	2493	1693	0.11%	0.014%
75	19.962	2867	2869	2872	rVB3	2411	1990	0.13%	0.016%
76	21.203	3075	3080	3090	rBV	510934	676373	44.17%	5.460%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045303.D
Acq On : 17 Apr 2024 05:14
Operator : MA/JU
Sample : P2099-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	23.256	3423	3429	3436	rBV2	849467	1531135	100.00%	12.361%
78	23.397	3447	3453	3464	rVB	450504	865889	56.55%	6.990%


Sum of corrected areas: 12386688

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045303.D
Acq On : 17 Apr 2024 05:14
Operator : MA/JU
Sample : P2099-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

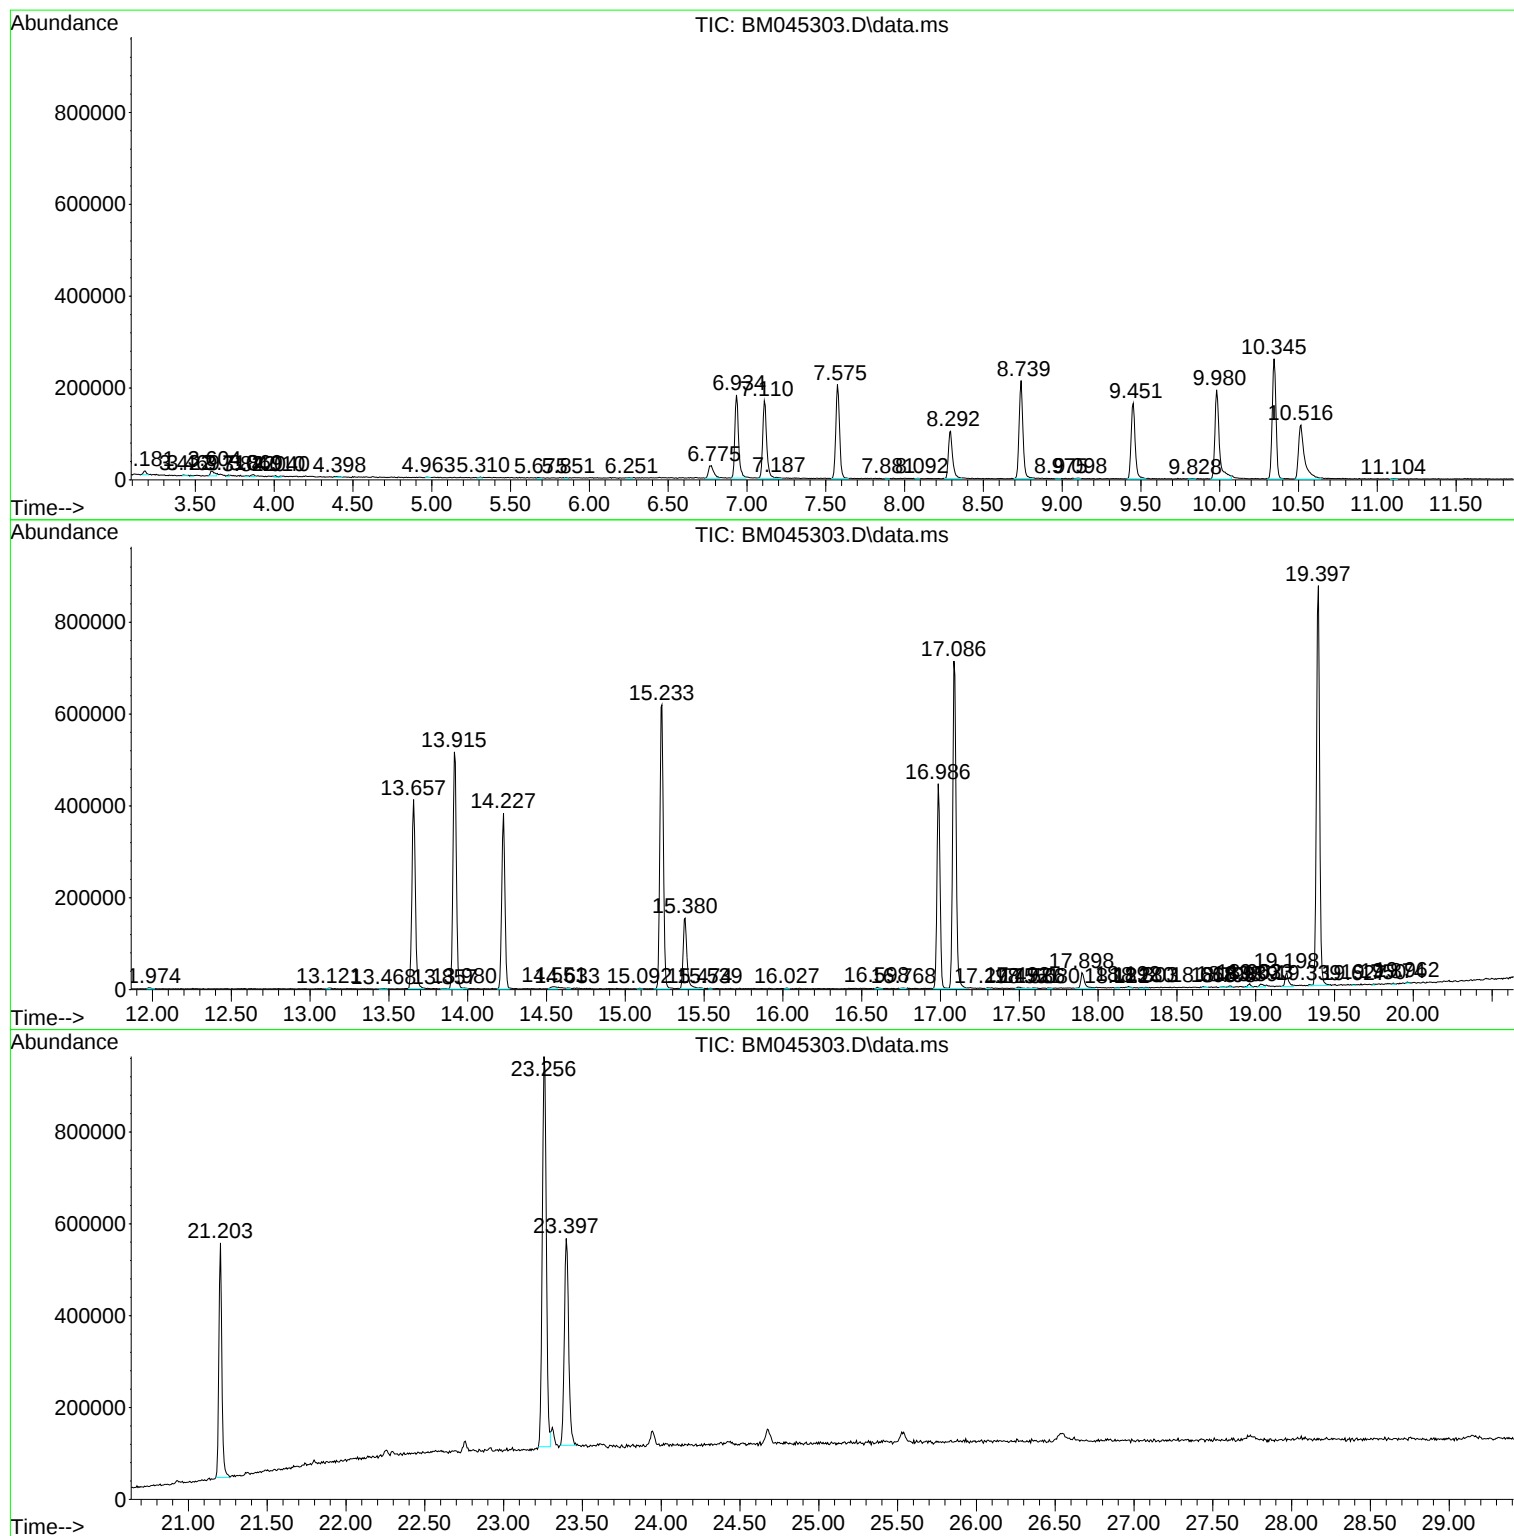

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045303.D
Acq On : 17 Apr 2024 05:14
Operator : MA/JU
Sample : P2099-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045303.D
Acq On : 17 Apr 2024 05:14
Operator : MA/JU
Sample : P2099-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------