

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045305.D
 Acq On : 17 Apr 2024 06:27
 Operator : MA/JU
 Sample : P2099-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	21	rVB	8615	13212	0.89%	0.109%
2	3.222	21	23	26	rBV3	1673	1605	0.11%	0.013%
3	3.357	45	46	50	rBV3	1683	1961	0.13%	0.016%
4	3.434	55	59	61	rVV4	2026	2508	0.17%	0.021%
5	3.481	63	67	69	rBV5	1856	2341	0.16%	0.019%
6	3.587	82	85	103	rBV	32684	75733	5.09%	0.625%
7	3.863	128	132	136	rBV5	3495	5110	0.34%	0.042%
8	3.993	152	154	157	rBV3	2002	2360	0.16%	0.019%
9	4.040	160	162	165	rVB2	1921	1717	0.12%	0.014%
10	4.157	179	182	183	rBV2	2100	1907	0.13%	0.016%
11	4.246	196	197	202	rVB3	2455	2679	0.18%	0.022%
12	4.334	211	212	215	rVB3	1729	1504	0.10%	0.012%
13	4.463	230	234	235	rBV4	1216	1516	0.10%	0.013%
14	4.816	290	294	296	rBV2	1717	1708	0.11%	0.014%
15	4.840	296	298	300	rVV3	1528	1573	0.11%	0.013%
16	4.875	302	304	307	rBV3	1753	1838	0.12%	0.015%
17	5.322	378	380	382	rVB	1806	1506	0.10%	0.012%
18	5.422	396	397	401	rVB3	1584	1607	0.11%	0.013%
19	6.298	545	546	551	rVB4	1038	1530	0.10%	0.013%
20	6.428	564	568	571	rVB4	1331	2069	0.14%	0.017%
21	6.769	620	626	637	rBV	33042	69678	4.68%	0.575%
22	6.934	648	654	664	rBV	189797	307211	20.65%	2.535%
23	7.110	677	684	700	rBV	176012	306039	20.57%	2.525%
24	7.575	756	763	772	rBV	210532	336008	22.58%	2.773%
25	7.998	832	835	839	rVB5	1436	1940	0.13%	0.016%
26	8.287	878	884	897	rVV	112536	206306	13.87%	1.702%
27	8.739	954	961	977	rBV	210890	363883	24.46%	3.003%
28	9.451	1075	1082	1099	rBV	169465	295162	19.84%	2.436%
29	9.616	1107	1110	1113	rVB3	1279	1540	0.10%	0.013%
30	9.981	1165	1172	1191	rBV	204930	405362	27.24%	3.345%
31	10.345	1228	1234	1244	rVB	266862	433631	29.14%	3.578%
32	10.510	1255	1262	1278	rBV	158332	382681	25.72%	3.158%
33	10.757	1302	1304	1308	rVB5	1411	1659	0.11%	0.014%
34	11.980	1508	1512	1518	rVB4	2730	5204	0.35%	0.043%
35	13.127	1699	1707	1711	rVV5	2052	3773	0.25%	0.031%
36	13.657	1791	1797	1807	rVV	425366	611688	41.11%	5.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045305.D
 Acq On : 17 Apr 2024 06:27
 Operator : MA/JU
 Sample : P2099-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.727	1807	1809	1812	rVV2	1890	2368	0.16%	0.020%
38	13.916	1834	1841	1853	rBV	527474	774946	52.08%	6.395%
39	14.227	1888	1894	1906	rVB	356827	526542	35.39%	4.345%
40	14.533	1941	1946	1947	rBV3	4797	5595	0.38%	0.046%
41	14.551	1947	1949	1952	rVB4	1769	2636	0.18%	0.022%
42	15.010	2021	2027	2032	rBV6	2515	3839	0.26%	0.032%
43	15.233	2058	2065	2074	rVV	615240	941366	63.27%	7.768%
44	15.380	2084	2090	2103	rVV	153413	251086	16.87%	2.072%
45	15.474	2105	2106	2110	rVB3	3075	2936	0.20%	0.024%
46	15.880	2172	2175	2178	rBV2	1093	1539	0.10%	0.013%
47	16.774	2323	2327	2331	rBV5	1002	1686	0.11%	0.014%
48	16.986	2358	2363	2373	rBV	421455	568969	38.24%	4.695%
49	17.086	2374	2380	2397	rVB	687702	1027636	69.06%	8.480%
50	17.904	2515	2519	2525	rBV3	13250	20918	1.41%	0.173%
51	18.086	2548	2550	2553	rBV3	1675	1585	0.11%	0.013%
52	18.151	2558	2561	2562	rVV2	2107	1726	0.12%	0.014%
53	18.174	2562	2565	2567	rVB3	1382	1743	0.12%	0.014%
54	18.209	2567	2571	2572	rBV3	1251	1574	0.11%	0.013%
55	18.333	2589	2592	2596	rVB3	1379	1761	0.12%	0.015%
56	18.798	2664	2671	2675	rVB4	1291	3390	0.23%	0.028%
57	18.962	2694	2699	2703	rVV5	7914	10274	0.69%	0.085%
58	19.033	2706	2711	2715	rVV7	4487	7201	0.48%	0.059%
59	19.109	2721	2724	2726	rBV4	1812	1886	0.13%	0.016%
60	19.198	2735	2739	2745	rBV7	8935	13154	0.88%	0.109%
61	19.398	2767	2773	2782	rVV	813086	1154078	77.56%	9.523%
62	19.792	2838	2840	2842	rBV3	1857	1522	0.10%	0.013%
63	19.856	2848	2851	2852	rBV3	2792	2177	0.15%	0.018%
64	19.927	2861	2863	2866	rBV4	1994	2189	0.15%	0.018%
65	20.774	3004	3007	3010	rBV4	7900	8735	0.59%	0.072%
66	21.203	3075	3080	3088	rBV	453082	636271	42.76%	5.250%
67	23.262	3423	3430	3437	rBV2	818975	1487961	100.00%	12.279%
68	23.397	3447	3453	3464	rVB	405858	791268	53.18%	6.530%




Sum of corrected areas: 12118306

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045305.D
Acq On : 17 Apr 2024 06:27
Operator : MA/JU
Sample : P2099-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

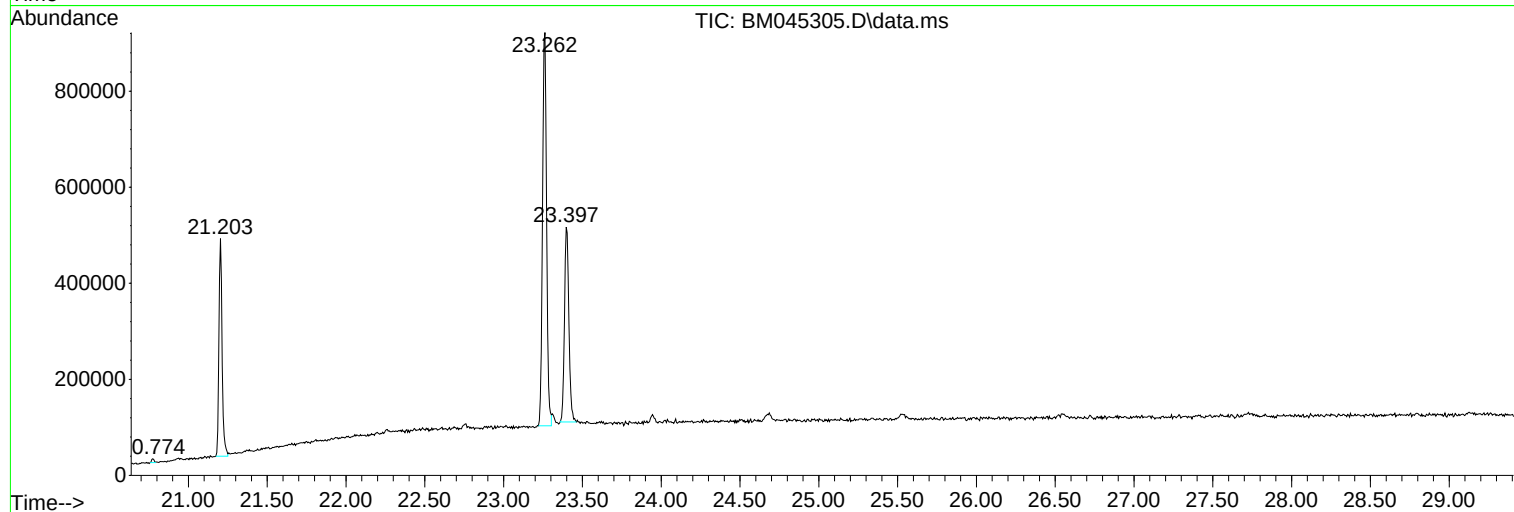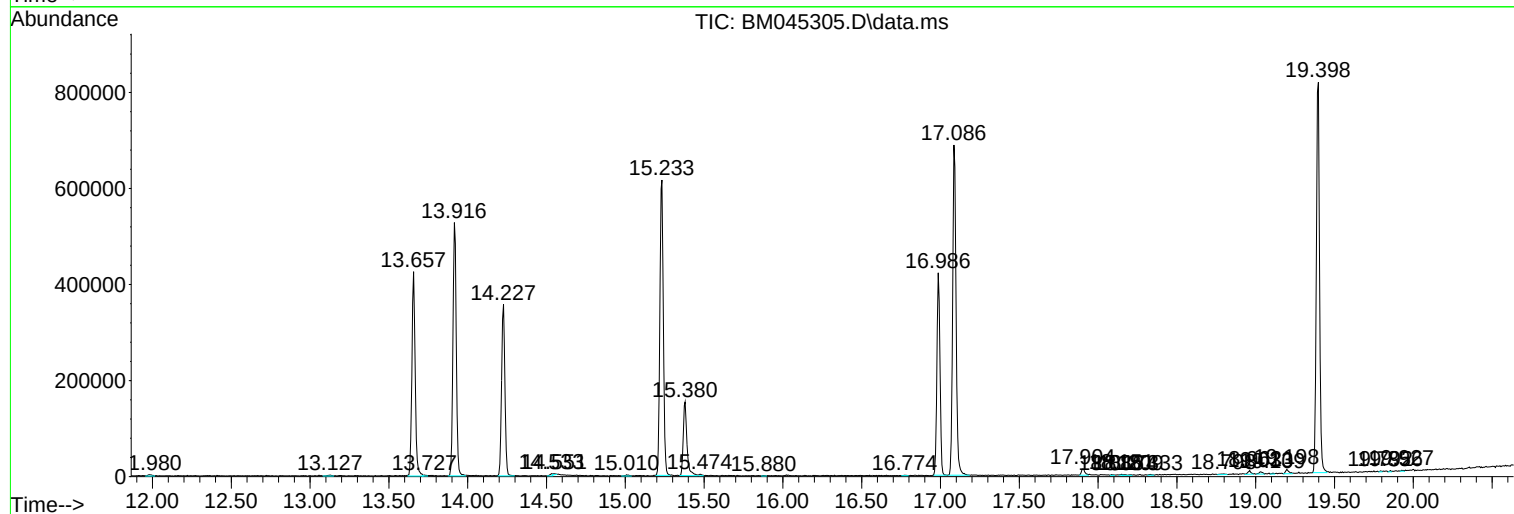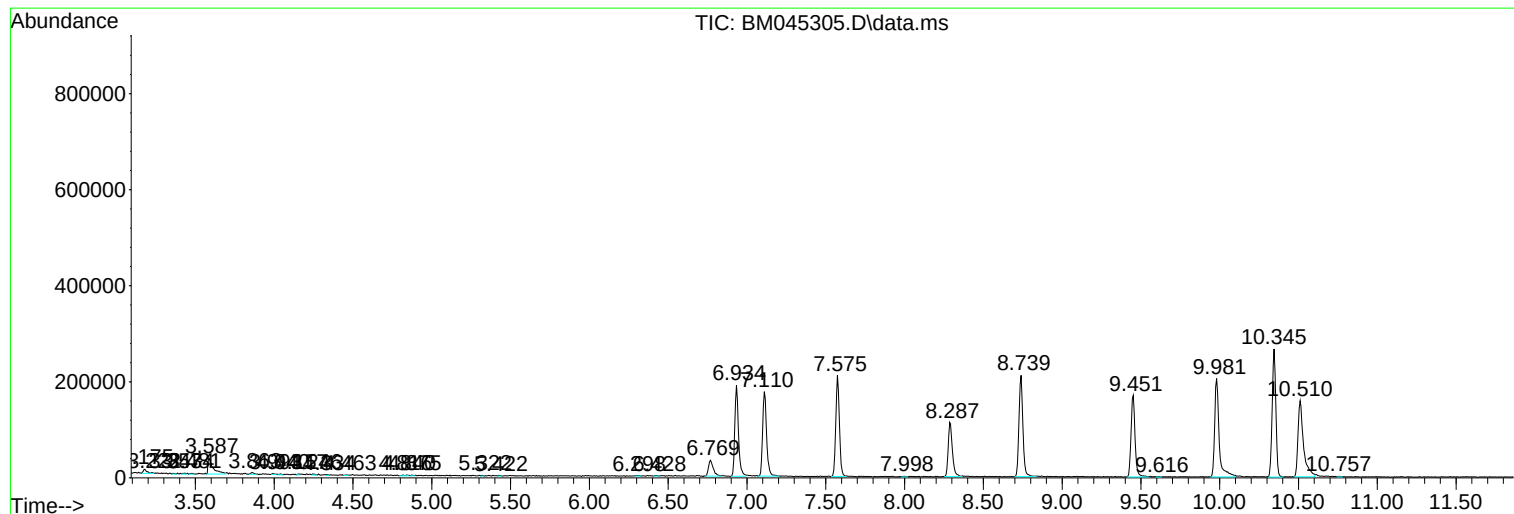

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045305.D
Acq On : 17 Apr 2024 06:27
Operator : MA/JU
Sample : P2099-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045305.D
Acq On : 17 Apr 2024 06:27
Operator : MA/JU
Sample : P2099-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------