

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045306.D
 Acq On : 17 Apr 2024 07:03
 Operator : MA/JU
 Sample : P2099-10
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	22	rVB	9270	12091	0.85%	0.108%
2	3.369	45	48	50	rBV4	1773	2479	0.18%	0.022%
3	3.475	64	66	68	rVB3	1965	1797	0.13%	0.016%
4	3.493	68	69	72	rBV3	1889	2089	0.15%	0.019%
5	3.587	82	85	96	rBV	36769	75240	5.31%	0.670%
6	3.863	129	132	136	rBV3	4015	5057	0.36%	0.045%
7	3.934	141	144	146	rBV4	1923	2328	0.16%	0.021%
8	4.457	230	233	236	rBV3	1863	2589	0.18%	0.023%
9	5.128	344	347	349	rBV4	1095	1549	0.11%	0.014%
10	5.304	372	377	379	rBV5	885	1470	0.10%	0.013%
11	5.445	397	401	403	rVV3	1252	1782	0.13%	0.016%
12	5.610	426	429	430	rBV3	1547	1663	0.12%	0.015%
13	5.751	452	453	456	rVB3	1903	1795	0.13%	0.016%
14	5.816	463	464	468	rBV3	1521	1853	0.13%	0.017%
15	5.934	482	484	487	rBV4	1822	2554	0.18%	0.023%
16	6.328	548	551	555	rBV4	1523	2612	0.18%	0.023%
17	6.622	597	601	602	rBV4	1056	1447	0.10%	0.013%
18	6.769	621	626	636	rBV	30792	63027	4.45%	0.562%
19	6.934	648	654	664	rBV	182498	293195	20.70%	2.613%
20	7.110	678	684	697	rBV	171291	290855	20.53%	2.592%
21	7.292	712	715	718	rVB3	1455	1492	0.11%	0.013%
22	7.575	756	763	772	rBV	162588	267585	18.89%	2.384%
23	8.286	878	884	896	rBV	109052	191755	13.54%	1.709%
24	8.739	954	961	971	rBV	200756	350782	24.76%	3.126%
25	8.804	971	972	978	rVB4	1774	2273	0.16%	0.020%
26	9.080	1015	1019	1021	rBV3	1080	1788	0.13%	0.016%
27	9.345	1062	1064	1069	rBV2	1015	1550	0.11%	0.014%
28	9.451	1075	1082	1094	rBV	159923	288797	20.39%	2.573%
29	9.786	1135	1139	1140	rBV2	1274	1721	0.12%	0.015%
30	9.980	1165	1172	1184	rBV	196020	373091	26.34%	3.325%
31	10.157	1199	1202	1204	rVB3	1671	1872	0.13%	0.017%
32	10.345	1227	1234	1251	rVB	211454	346370	24.45%	3.087%
33	10.510	1256	1262	1281	rBV	148940	356797	25.19%	3.179%
34	11.033	1348	1351	1354	rVB3	1589	1786	0.13%	0.016%
35	11.974	1505	1511	1512	rBV3	2587	2997	0.21%	0.027%
36	12.963	1672	1679	1680	rVB3	907	1828	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045306.D
 Acq On : 17 Apr 2024 07:03
 Operator : MA/JU
 Sample : P2099-10
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.121	1701	1706	1712	rBV2	22083	32580	2.30%	0.290%
38	13.657	1791	1797	1810	rBV	413449	602706	42.55%	5.371%
39	13.915	1835	1841	1854	rBV	518945	757612	53.48%	6.751%
40	14.021	1856	1859	1860	rBV2	1222	1437	0.10%	0.013%
41	14.227	1887	1894	1902	rBV	289206	421773	29.78%	3.758%
42	14.462	1928	1934	1937	rBV5	3953	7105	0.50%	0.063%
43	14.533	1942	1946	1951	rBV4	4733	10488	0.74%	0.093%
44	15.227	2056	2064	2075	rBV	629883	938947	66.28%	8.367%
45	15.380	2084	2090	2098	rBV	143587	232861	16.44%	2.075%
46	15.474	2104	2106	2109	rVB3	2440	2165	0.15%	0.019%
47	16.598	2293	2297	2302	rBV4	2210	3107	0.22%	0.028%
48	16.933	2350	2354	2356	rBV3	1748	2351	0.17%	0.021%
49	16.986	2357	2363	2370	rVV	339824	467742	33.02%	4.168%
50	17.086	2374	2380	2396	rVV	650656	991844	70.02%	8.838%
51	17.686	2479	2482	2487	rVB4	2277	2933	0.21%	0.026%
52	17.903	2514	2519	2526	rBV4	10806	18988	1.34%	0.169%
53	18.168	2562	2564	2568	rVV3	3311	4132	0.29%	0.037%
54	18.262	2578	2580	2585	rVB4	1334	1592	0.11%	0.014%
55	18.474	2614	2616	2618	rVB2	2143	1776	0.13%	0.016%
56	18.533	2624	2626	2630	rBV3	1514	1921	0.14%	0.017%
57	18.574	2630	2633	2637	rVV5	1036	1742	0.12%	0.016%
58	18.745	2660	2662	2664	rBV2	1584	1772	0.13%	0.016%
59	18.962	2695	2699	2702	rVV3	6188	8254	0.58%	0.074%
60	19.039	2706	2712	2718	rVB2	5068	8129	0.57%	0.072%
61	19.197	2736	2739	2748	rBV6	7005	10478	0.74%	0.093%
62	19.297	2751	2756	2758	rBV5	1635	2824	0.20%	0.025%
63	19.344	2761	2764	2766	rBV2	2040	2004	0.14%	0.018%
64	19.397	2766	2773	2781	rBV	799736	1109017	78.29%	9.883%
65	20.074	2886	2888	2891	rBV4	2204	2328	0.16%	0.021%
66	20.197	2907	2909	2912	rBV4	2416	2299	0.16%	0.020%
67	20.527	2963	2965	2967	rBV3	3084	3170	0.22%	0.028%
68	21.203	3075	3080	3092	rBV	373877	527614	37.25%	4.702%
69	23.262	3423	3430	3437	rBV2	780064	1416532	100.00%	12.623%
70	23.397	3447	3453	3466	rVB	328061	661781	46.72%	5.897%




Sum of corrected areas: 11221960

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045306.D
Acq On : 17 Apr 2024 07:03
Operator : MA/JU
Sample : P2099-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

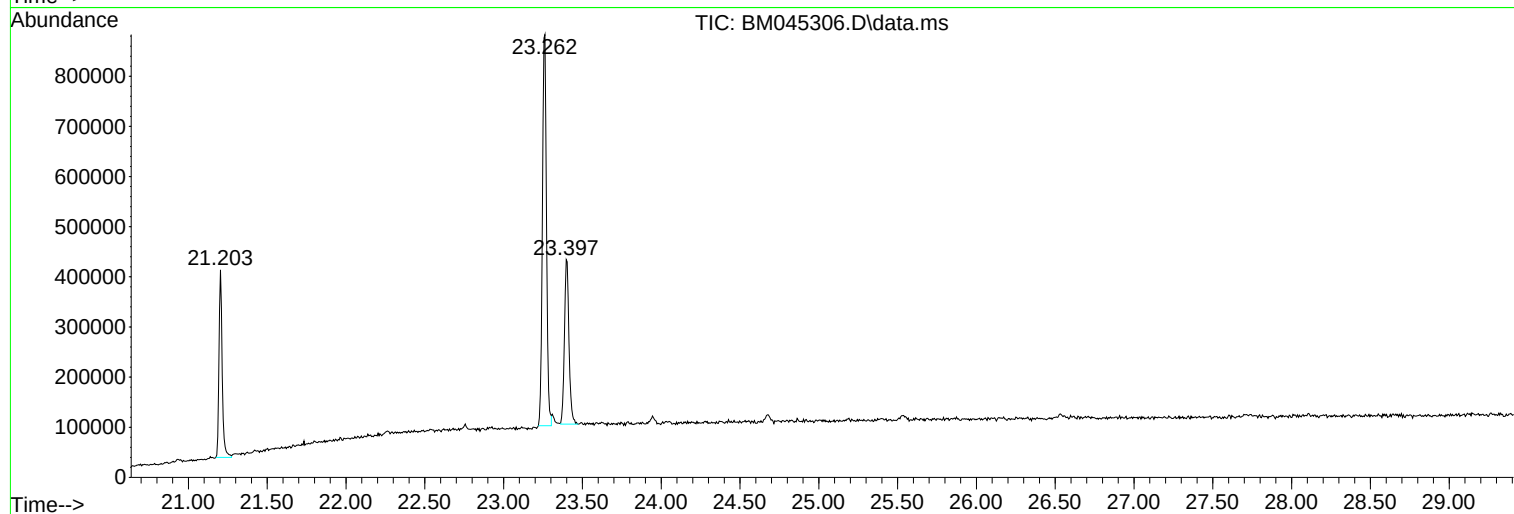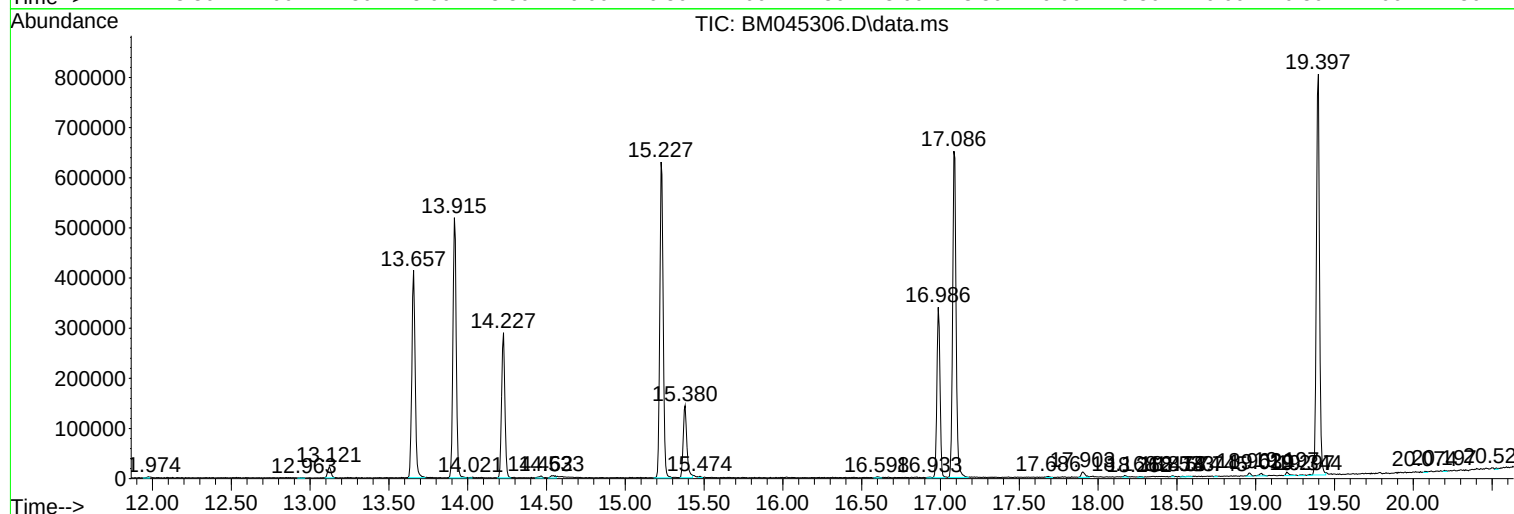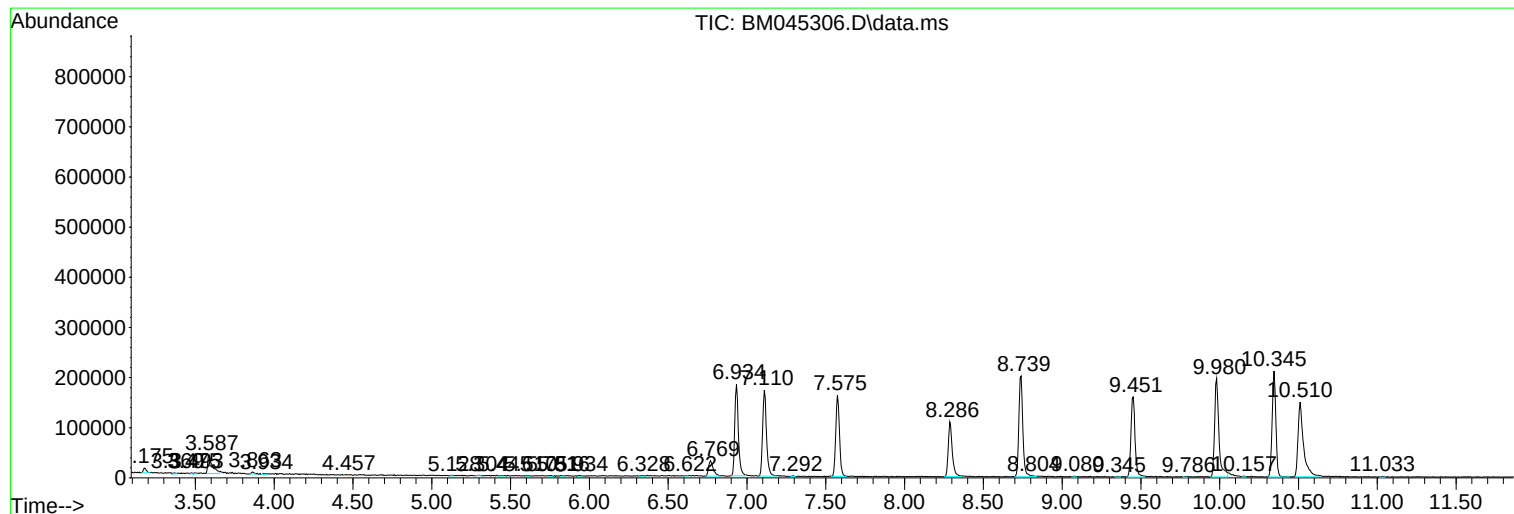

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045306.D
Acq On : 17 Apr 2024 07:03
Operator : MA/JU
Sample : P2099-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045306.D
Acq On : 17 Apr 2024 07:03
Operator : MA/JU
Sample : P2099-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc