

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
 Data File : BM049954.D
 Acq On : 16 Apr 2025 16:05
 Operator : RC/JU
 Sample : Q1806-01DL 4X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OR-03-041425DL

Manual Integrations
 APPROVED

Reviewed By :Rahul
 Chavli

Quant Time: Apr 16 16:45:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							04/17/2025
1) 1,4-Dichlorobenzene-d4	7.769	152	435300	20.000	ng	-0.01	Supervised By :Jagrut Upadhyay
21) Naphthalene-d8	10.563	136	1469118	20.000	ng	-0.01	
39) Acenaphthene-d10	14.410	164	897287	20.000	ng	-0.01	
64) Phenanthrene-d10	17.156	188	1665896	20.000	ng	0.00	
76) Chrysene-d12	21.397	240	1666327	20.000	ng	0.00	
86) Perylene-d12	24.403	264	1846834	20.000	ng	0.00	04/17/2025
System Monitoring Compounds							
5) 2-Fluorophenol	5.357	112	430145	16.780	ng	0.00	
7) Phenol-d6	6.951	99	531761	16.672	ng	0.00	
23) Nitrobenzene-d5	8.928	82	300433	11.388	ng	0.00	
42) 2,4,6-Tribromophenol	15.904	330	208473	15.973	ng	0.00	
45) 2-Fluorobiphenyl	13.033	172	717686	10.846	ng	-0.01	
79) Terphenyl-d14	19.780	244	831234	9.349	ng	-0.01	
Target Compounds							Qvalue
52) Acenaphthene	14.474	154	132517	2.728	ng		98
58) Fluorene	15.462	166	197696	3.063	ng		98
71) Phenanthrene	17.198	178	2427573	26.580	ng		100
72) Anthracene	17.292	178	640940	7.121	ng		99
73) Carbazole	17.562	167	240113	2.832	ng		99
75) Fluoranthene	19.215	202	4076708	36.303	ng		100
78) Pyrene	19.580	202	3436753	29.926	ng		99
81) Benzo(a)anthracene	21.380	228	1441132	13.013	ng		99
83) Chrysene	21.439	228	1284139	12.197	ng		98
87) Indeno(1,2,3-cd)pyrene	27.785	276	790733	5.744	ng		97
88) Benzo(b)fluoranthene	23.450	252	1537648	13.036	ng		99
89) Benzo(k)fluoranthene	23.509	252	590686m	5.168	ng		
90) Benzo(a)pyrene	24.256	252	1190865	11.490	ng		98
92) Benzo(g,h,i)perylene	28.838	276	789996	6.818	ng		100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049954.D
Acq On : 16 Apr 2025 16:05
Operator : RC/JU
Sample : Q1806-01DL 4X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-03-041425DL

Quant Time: Apr 16 16:45:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli

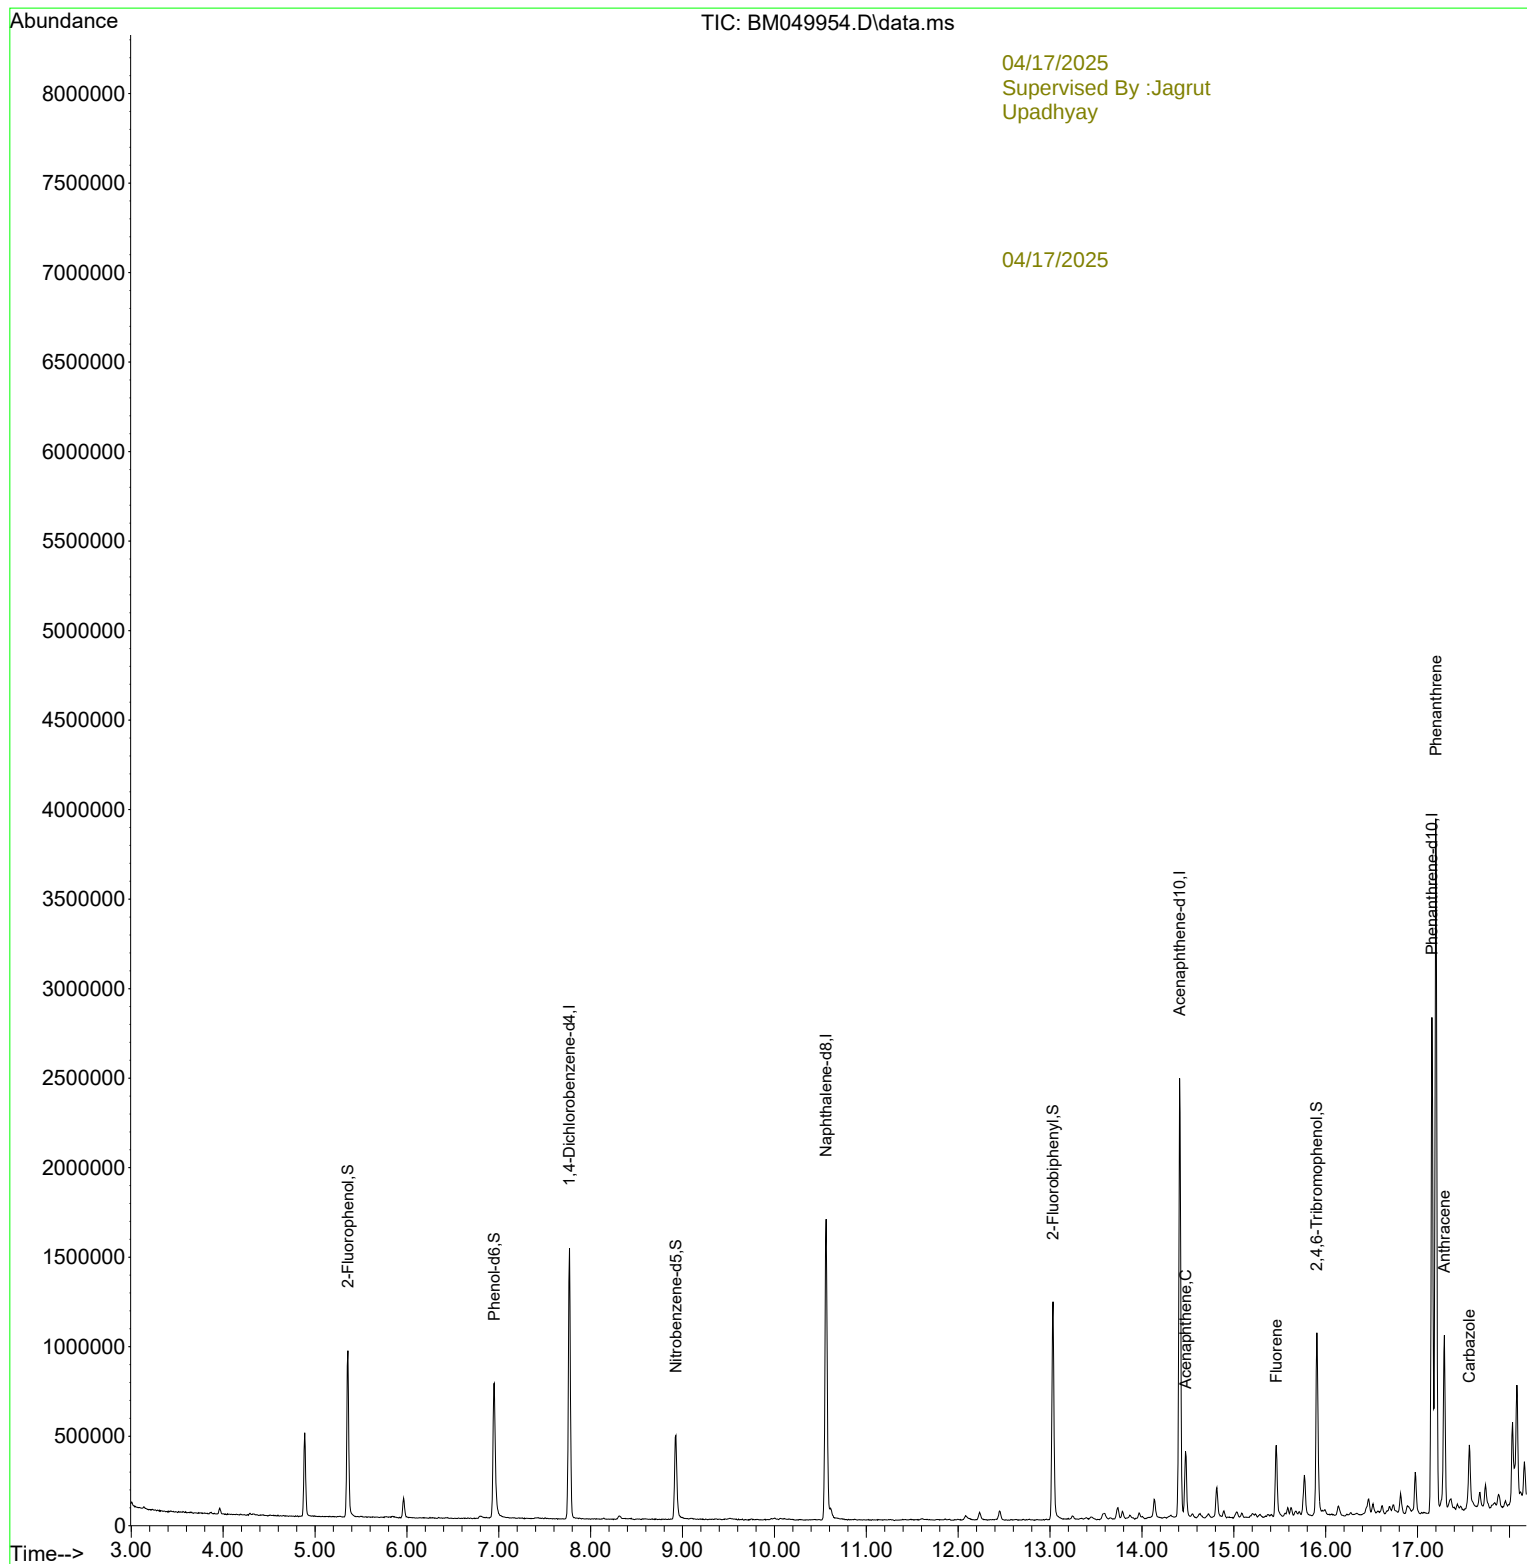

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049954.D
Acq On : 16 Apr 2025 16:05
Operator : RC/JU
Sample : Q1806-01DL 4X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-03-041425DL

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli

Quant Time: Apr 16 16:45:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

