
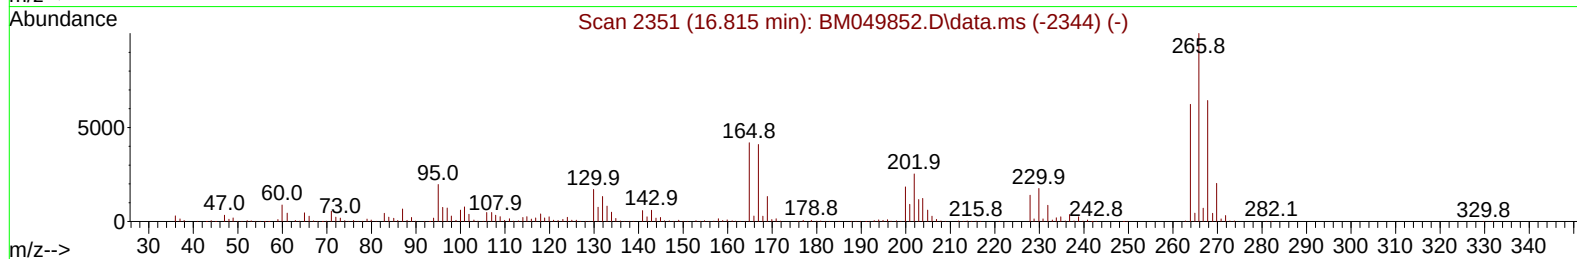
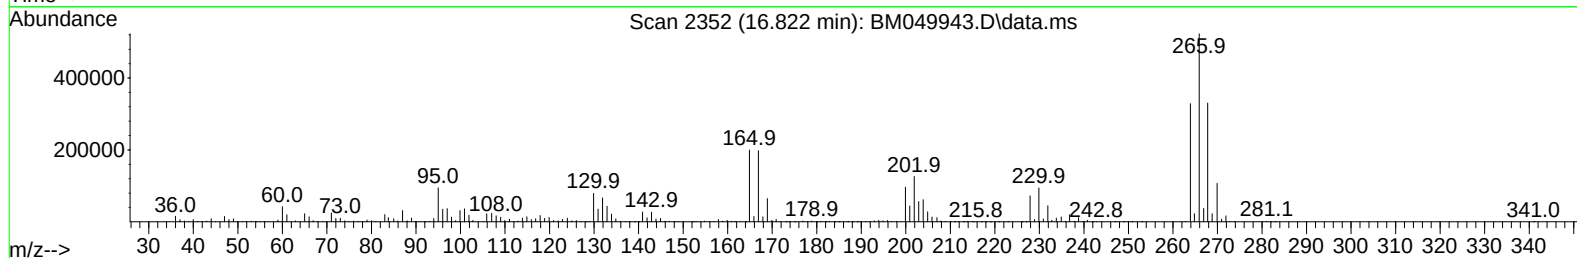


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049943.D
Acq On : 16 Apr 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 11:06:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

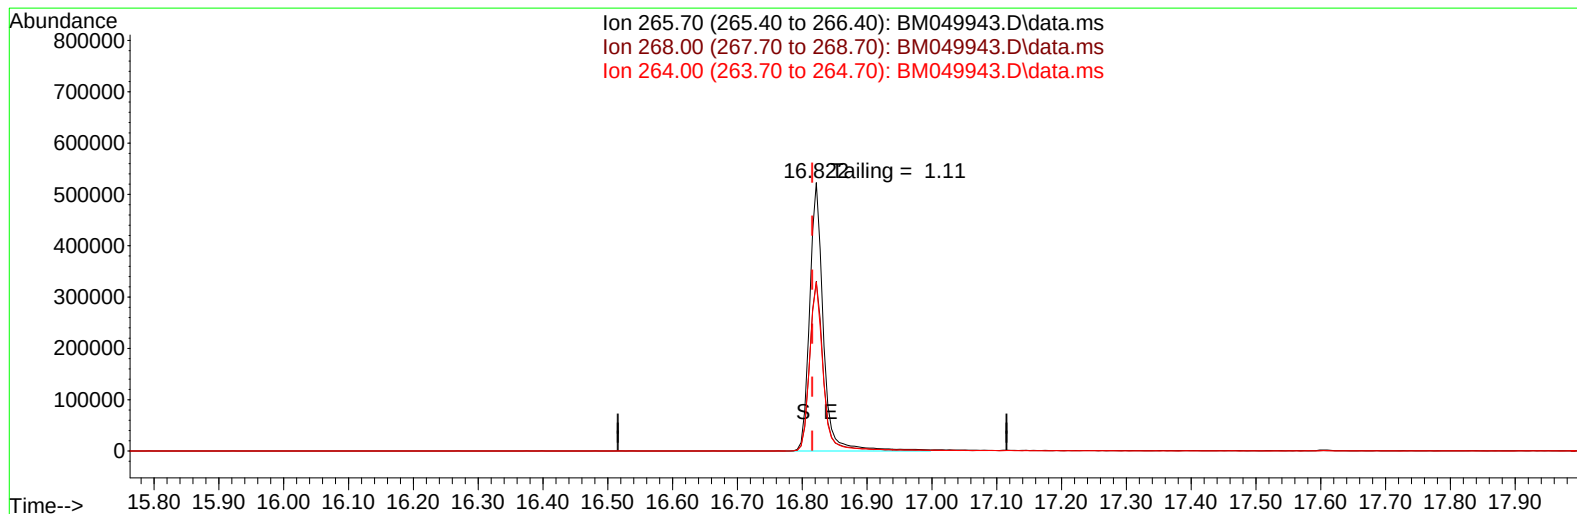

TIC: BM049943.D\data.ms

(70) Pentachlorophenol (C)




16.822min (+ 0.006) 1377107.60 ng

response 769504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.19
264.00	62.30	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049943.D
Acq On : 16 Apr 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 11:06:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

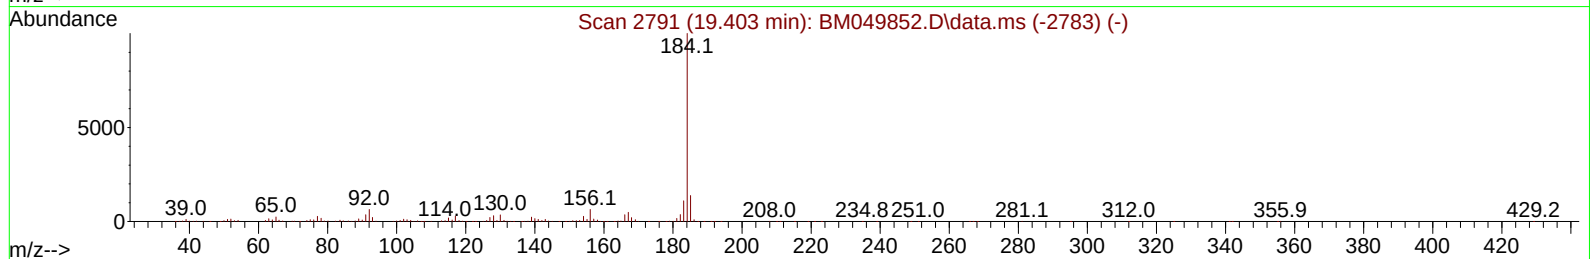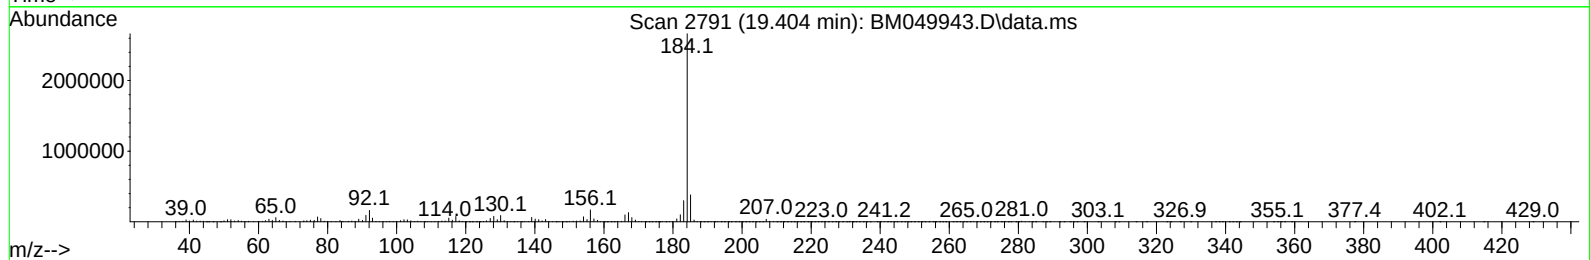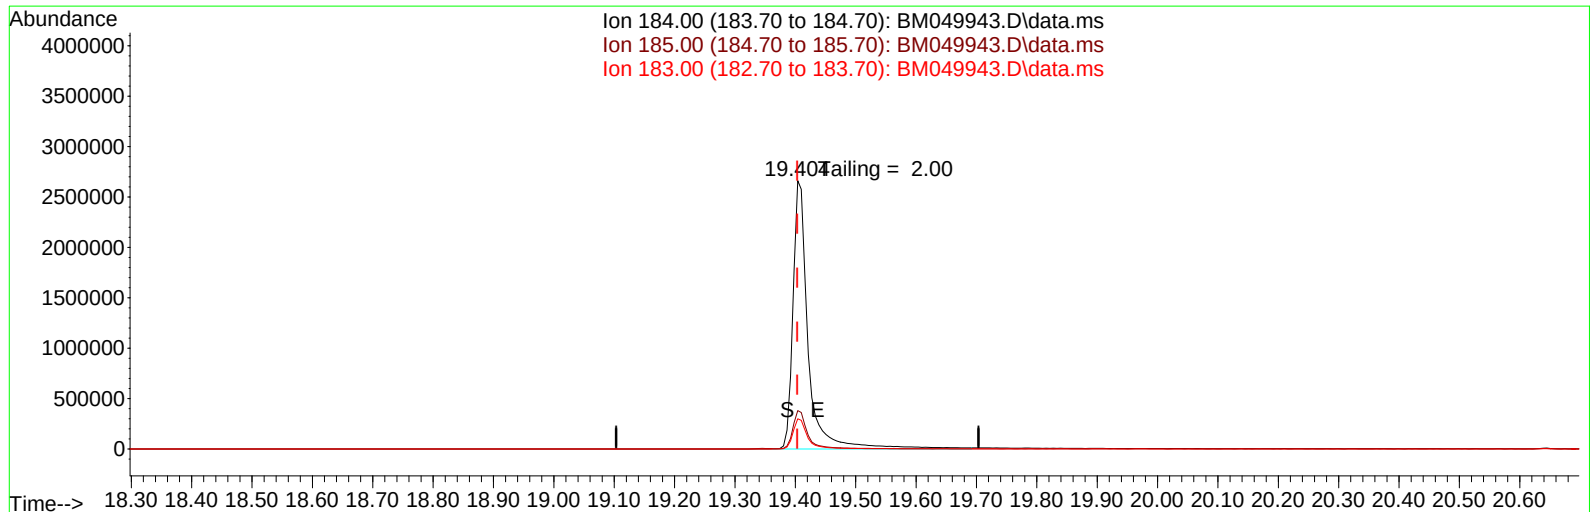

TIC: BM049943.D\data.ms

(77) Benzidine**19.404min (+ 0.000) 473739.12 ng****response 4713616**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.31
183.00	11.00	11.26
0.00	0.00	0.00