


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041715\
 Data File : BM001021.D
 Acq On : 16 Apr 2015 16:30
 Operator : TP/IZ
 Sample : DFTPP48
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP48

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM041715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 15:43:32 2015

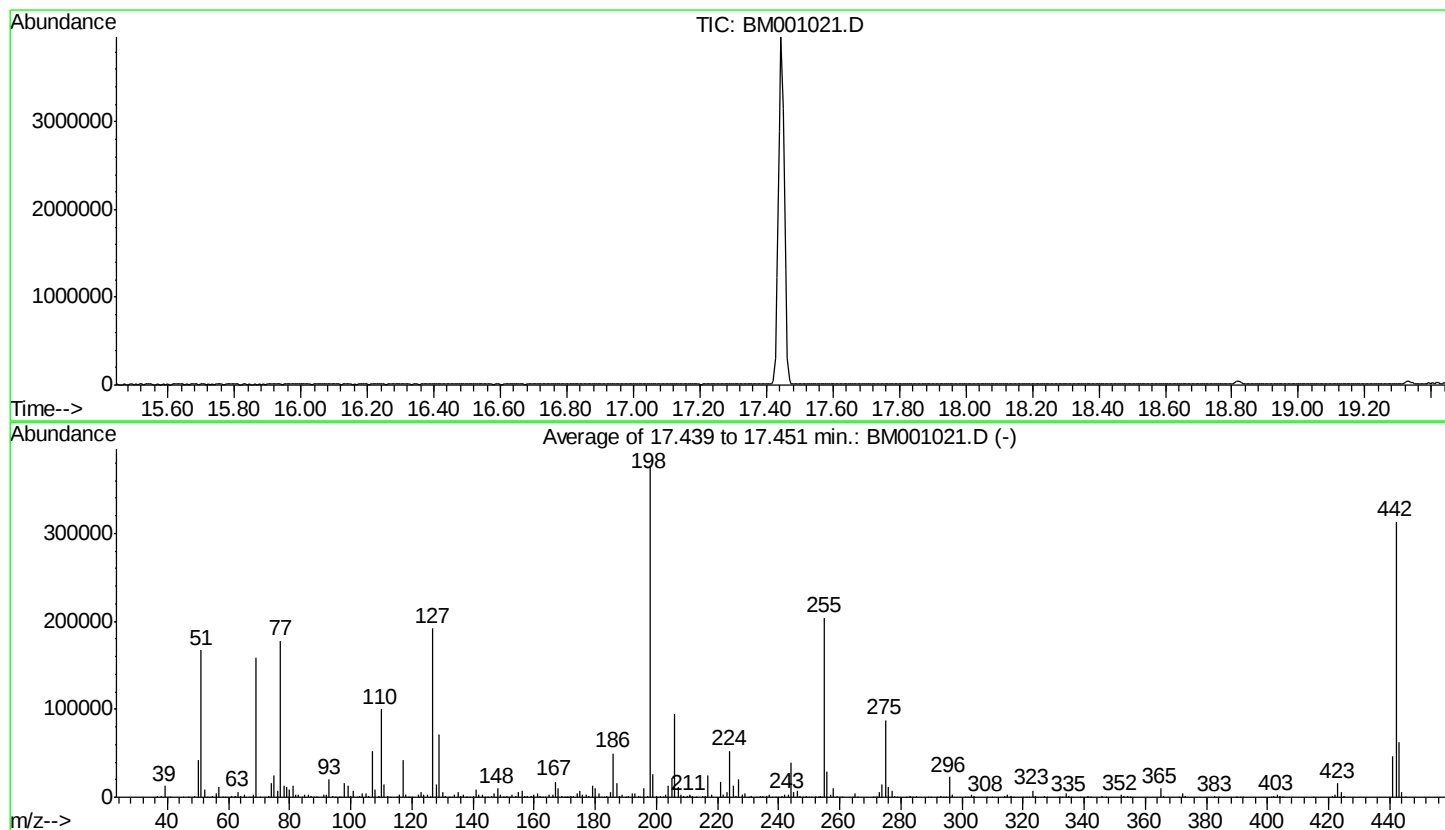

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	166890	PASS
68	69	0.00	2	1.5	2349	PASS
69	198	0.00	100	41.9	158029	PASS
70	69	0.00	2	0.5	757	PASS
127	198	10	80	50.9	191893	PASS
197	198	0.00	2	0.5	1880	PASS
198	198	100	100	100.0	377109	PASS
199	198	5	9	6.9	26186	PASS
275	198	10	60	23.2	87594	PASS
365	198	1	100	2.6	9927	PASS
441	443	0.01	100	75.2	46562	PASS
442	198	50	100	83.1	313472	PASS
443	442	15	24	19.8	61941	PASS

m/z	Abundance
37.00	1237.0
38.00	2021.0
39.10	12571.0
40.00	1689.0
41.00	403.0
44.00	6753.0
45.00	399.0
49.00	1369.0
50.10	44136.0
51.10	165504.0
52.10	9220.0
53.00	347.0
55.10	1000.0
56.00	4237.0
57.00	10785.0
58.00	867.0
61.10	1629.0
61.90	1918.0
63.00	7032.0
64.00	1225.0
65.00	2844.0
68.00	2041.0
69.00	157888.0
70.00	909.0
73.00	2177.0
74.10	15118.0
75.00	22912.0
76.00	7962.0
77.10	170432.0
78.00	12300.0
79.00	9760.0
80.10	9262.0
81.00	12208.0
82.10	3574.0
83.00	3020.0
83.90	501.0
85.00	2399.0
86.00	3364.0
87.00	1583.0
88.80	320.0
91.00	2856.0
91.90	3003.0
93.00	20920.0
94.00	1341.0
96.00	1159.0
96.70	372.0
98.00	14941.0
99.00	11626.0
100.00	1165.0
101.00	5860.0
102.90	2467.0
104.00	4027.0
105.00	3714.0
106.10	1076.0
107.00	49456.0
108.10	7415.0
109.00	1269.0
110.00	93304.0
111.00	13537.0
112.00	1683.0
112.90	796.0
116.10	2816.0
117.00	40264.0
118.00	3177.0
118.80	457.0
120.00	539.0
122.00	3351.0
123.00	5218.0
124.00	2960.0
125.00	2265.0
126.10	716.0
127.00	179200.0
128.00	14046.0
129.00	67320.0
130.00	5225.0
131.00	987.0
132.10	505.0
133.10	309.0
134.00	2073.0
135.00	6144.0
136.00	1992.0
137.00	2446.0
138.00	639.0
139.00	313.0
140.10	1093.0
141.00	8141.0
142.00	2524.0
142.90	2867.0
144.00	560.0
146.00	2032.0
147.00	4823.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

148.00	8972.0
149.00	2930.0
149.90	741.0
151.00	941.0
152.90	3371.0
154.00	1965.0
155.00	4243.0
156.00	6128.0
157.00	1033.0
157.90	1293.0
159.00	1095.0
159.90	1846.0
161.10	3748.0
162.00	1283.0
163.00	318.0
163.80	455.0
164.90	3074.0
166.00	2628.0
167.00	14574.0
168.00	11421.0
169.00	2012.0
170.00	370.0
171.10	625.0
172.00	1238.0
173.10	1658.0
174.10	3859.0
175.00	6477.0
175.90	2108.0
176.90	3378.0
178.00	1434.0
179.00	11040.0
180.00	9001.0
181.10	4289.0
182.00	419.0
183.90	924.0
185.00	4888.0
186.00	44616.0
187.00	13533.0
188.00	1084.0
188.90	2946.0
189.90	730.0
191.10	1102.0
191.90	3560.0
193.10	3779.0
194.10	1283.0
196.00	9012.0
197.00	1562.0
198.00	322560.0
199.00	23432.0
200.10	1867.0
201.40	1405.0
203.00	1938.0
204.00	9968.0
205.00	18024.0
206.10	80408.0
207.00	11688.0
208.00	3066.0
208.90	1103.0
209.90	967.0
210.80	2916.0
211.70	912.0
213.00	302.0
215.10	1139.0
216.10	1247.0
217.00	20792.0
218.00	3175.0
221.00	16688.0
222.00	2685.0
223.00	4385.0
224.10	44600.0
225.10	11343.0
225.90	1529.0
227.00	16512.0
228.00	2429.0
229.00	3052.0
230.10	554.0
231.00	1689.0
233.00	528.0
234.00	1137.0
235.10	1395.0
236.10	885.0
237.10	1936.0
238.00	360.0
239.10	612.0
240.00	739.0
241.10	835.0
242.10	1835.0
243.00	2652.0
244.10	32656.0
245.00	4876.0
246.00	5927.0
247.10	1515.0
249.00	1058.0
251.90	430.0
252.80	901.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

253.80	1082.0
254.10	1041.0
255.00	165248.0
256.00	24120.0
256.90	2311.0
258.00	8399.0
259.00	2028.0
261.00	379.0
265.00	3280.0
265.90	585.0
270.90	474.0
271.80	366.0
273.00	3993.0
274.00	11167.0
275.00	69840.0
276.00	9928.0
277.00	5532.0
278.00	1342.0
281.00	423.0
283.10	426.0
284.00	812.0
285.10	1189.0
288.80	356.0
291.80	312.0
293.10	1159.0
294.00	556.0
295.00	348.0
296.00	18792.0
297.00	2909.0
302.10	515.0
303.10	2646.0
304.00	750.0
308.00	319.0
314.10	1054.0
315.00	2145.0
315.90	873.0
321.10	521.0
323.10	6381.0
324.10	882.0
327.00	1063.0
328.10	590.0
331.80	491.0
333.00	519.0
334.00	2577.0
335.10	658.0
341.00	907.0
345.90	1085.0
346.90	361.0
352.00	1449.0
352.90	1161.0
354.10	1359.0
355.20	442.0
365.00	7293.0
366.00	949.0
372.10	2942.0
373.00	558.0
382.80	760.0
383.90	418.0
389.90	432.0
391.20	321.0
401.10	482.0
402.00	996.0
403.00	1332.0
403.90	492.0
404.90	361.0
414.90	315.0
421.10	1653.0
421.90	1836.0
423.10	9435.0
424.10	4235.0
425.10	1142.0
441.00	30088.0
442.00	202240.0
443.00	43304.0
444.00	4820.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z	Abundance
36.90	846.0
38.10	2202.0
39.10	15304.0
40.00	2205.0
41.10	547.0
44.00	5708.0
45.00	439.0
46.90	371.0
49.00	1193.0
50.10	49816.0
51.10	201088.0
52.10	10050.0
53.00	509.0
54.90	1153.0
56.00	6287.0
57.00	13619.0
58.00	591.0
59.10	301.0
61.00	3053.0
62.10	2673.0
63.00	7344.0
64.00	1108.0
65.10	4824.0
68.00	2778.0
69.00	188288.0
70.10	504.0
73.10	1467.0
74.00	18376.0
75.10	30408.0
76.10	9587.0
77.10	215104.0
78.10	15528.0
79.00	13768.0
80.00	11178.0
81.00	14620.0
82.00	3226.0
83.00	3370.0
83.90	906.0
85.10	2979.0
86.00	3931.0
87.00	2311.0
88.00	498.0
89.00	340.0
91.10	3214.0
92.00	4037.0
93.00	23696.0
93.90	1710.0
95.10	460.0
96.10	993.0
96.80	403.0
98.00	19504.0
99.00	14857.0
100.00	1288.0
101.00	8617.0
102.10	378.0
103.00	2233.0
104.00	5858.0
105.10	4686.0
105.90	1109.0
107.00	63608.0
108.00	9868.0
109.10	2076.0
110.00	117424.0
111.10	17888.0
112.10	2283.0
112.90	802.0
115.10	386.0
116.00	3174.0
117.00	48920.0
118.00	3622.0
119.10	548.0
120.10	707.0
122.00	4529.0
123.00	7150.0
123.90	2727.0
125.00	2288.0
126.10	701.0
127.00	230336.0
128.00	17096.0
129.00	86136.0
130.00	7409.0
130.90	1569.0
132.00	750.0
133.10	401.0
134.00	2852.0
135.00	7210.0
135.90	2600.0
137.00	4217.0
138.10	978.0
139.00	365.0
140.10	922.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

141.00	10862.0
142.10	2995.0
143.00	2452.0
144.00	572.0
145.00	673.0
146.10	1405.0
147.00	4910.0
148.00	12266.0
148.90	3192.0
150.10	474.0
150.90	1623.0
151.80	1121.0
153.00	3480.0
154.00	2096.0
155.00	7435.0
156.00	9808.0
157.10	2132.0
158.00	2542.0
159.00	1059.0
160.00	3147.0
161.10	4777.0
162.10	1877.0
163.90	517.0
165.00	3506.0
166.00	2933.0
167.00	22360.0
168.00	11971.0
169.10	2219.0
169.90	760.0
171.00	881.0
172.00	2538.0
172.90	2281.0
174.00	4929.0
175.10	8752.0
176.00	2648.0
176.90	4069.0
177.80	1503.0
179.00	15308.0
180.00	12390.0
181.00	5856.0
182.00	930.0
182.80	503.0
184.00	1344.0
185.00	6907.0
186.00	59368.0
187.00	19512.0
188.10	2225.0
189.00	3159.0
189.90	441.0
190.90	1900.0
192.00	4680.0
193.00	4610.0
194.10	1189.0
194.80	335.0
196.00	13600.0
197.00	2242.0
198.00	445184.0
199.00	31848.0
200.10	2731.0
201.40	2431.0
203.00	3535.0
204.10	16028.0
205.00	26816.0
206.10	113064.0
207.10	16239.0
208.00	3922.0
209.10	1533.0
210.00	1615.0
211.00	3853.0
211.80	1025.0
213.20	310.0
214.90	1035.0
216.00	2469.0
217.00	28576.0
218.00	3654.0
221.10	20440.0
221.80	4165.0
223.00	7575.0
224.10	64080.0
225.10	15906.0
226.00	2454.0
227.00	25816.0
227.90	3832.0
229.00	5077.0
230.00	770.0
231.00	2057.0
232.80	336.0
234.00	1252.0
235.00	2096.0
236.00	1217.0
237.10	2805.0
237.90	638.0
239.00	1007.0
240.00	547.0
241.10	1376.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

242.10	2950.0
243.10	3406.0
244.10	47736.0
245.10	6110.0
246.00	8552.0
247.00	1384.0
248.00	495.0
249.00	1350.0
250.10	431.0
252.10	646.0
252.90	692.0
253.90	1711.0
255.00	243264.0
256.00	33168.0
256.90	2910.0
258.00	12404.0
259.00	2590.0
259.90	576.0
261.00	725.0
265.00	4712.0
265.90	722.0
271.00	823.0
272.10	606.0
273.00	7535.0
274.00	17152.0
275.00	103512.0
276.10	13656.0
277.00	6808.0
277.90	1119.0
281.90	459.0
283.10	1043.0
284.00	651.0
285.10	1343.0
289.90	375.0
291.90	351.0
292.90	2172.0
294.00	375.0
294.90	571.0
296.00	26232.0
297.00	4025.0
301.00	359.0
302.10	619.0
303.00	3382.0
304.00	1142.0
308.10	681.0
309.80	341.0
313.90	1143.0
315.00	2669.0
316.10	1706.0
316.90	377.0
319.90	308.0
321.10	1107.0
322.00	771.0
323.00	9200.0
324.10	2083.0
327.00	1856.0
328.00	867.0
332.00	744.0
333.10	665.0
334.00	5953.0
335.00	1592.0
335.90	409.0
338.70	348.0
341.10	1368.0
342.00	306.0
345.90	1781.0
347.00	414.0
352.10	2903.0
353.00	1647.0
354.00	2519.0
354.90	625.0
365.00	11932.0
366.00	1510.0
371.00	869.0
372.10	4571.0
372.90	1685.0
382.90	1450.0
384.00	437.0
390.10	889.0
391.00	512.0
402.00	2354.0
403.10	2598.0
404.00	912.0
405.10	447.0
421.10	2442.0
422.00	3240.0
423.00	17864.0
424.10	6340.0
425.10	819.0
441.00	54832.0
442.00	363712.0
443.00	73432.0
444.10	5784.0
444.90	659.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z	Abundance
35.90	342.0
37.00	666.0
38.00	1615.0
39.10	10106.0
40.00	1658.0
41.00	472.0
44.00	5139.0
45.10	481.0
49.00	1114.0
50.10	34000.0
51.10	134080.0
52.10	6416.0
54.90	928.0
56.00	3975.0
57.10	8810.0
58.00	568.0
61.00	1401.0
62.10	1871.0
63.10	4711.0
64.00	661.0
65.00	2451.0
67.10	343.0
68.00	2229.0
69.00	127912.0
70.00	859.0
73.00	1264.0
74.00	13697.0
75.00	20464.0
76.10	6251.0
77.10	148032.0
78.10	10139.0
79.00	9812.0
80.00	8104.0
81.00	10918.0
82.00	2641.0
83.00	2262.0
84.00	400.0
85.00	1587.0
86.00	2853.0
87.00	1255.0
88.00	391.0
88.80	323.0
91.00	2680.0
92.00	2734.0
93.00	16371.0
94.00	1124.0
94.90	334.0
96.10	777.0
96.80	345.0
98.00	12588.0
99.00	11143.0
100.00	1432.0
101.00	6550.0
102.00	339.0
103.00	1648.0
103.90	4127.0
105.00	3105.0
106.00	1282.0
107.00	43336.0
108.00	6962.0
109.00	1056.0
110.00	89680.0
111.00	12688.0
112.00	1114.0
113.00	325.0
115.10	353.0
116.00	2155.0
117.00	35464.0
118.00	2944.0
118.90	602.0
120.20	490.0
122.00	3100.0
123.00	5072.0
123.90	1637.0
124.90	2265.0
125.80	414.0
126.10	413.0
127.00	166144.0
128.00	11183.0
129.00	61672.0
130.10	5127.0
130.90	1082.0
132.10	725.0
132.90	409.0
134.00	2022.0
135.00	4612.0
136.10	1881.0
137.10	2619.0
137.80	771.0
139.00	386.0
139.90	950.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

141.00	7949.0
142.00	2507.0
142.90	1923.0
143.90	518.0
144.80	351.0
146.10	1654.0
147.00	4001.0
148.00	8919.0
148.90	1788.0
150.10	833.0
151.00	1107.0
151.80	658.0
153.00	2450.0
153.90	1509.0
155.00	4699.0
156.00	7407.0
157.00	936.0
157.90	1710.0
159.00	1043.0
160.00	2694.0
161.00	4109.0
162.00	1164.0
163.80	511.0
165.00	2843.0
166.00	2347.0
167.00	17024.0
168.00	8913.0
169.00	1306.0
169.80	386.0
170.20	471.0
170.80	1101.0
172.00	1392.0
173.00	1276.0
173.90	3635.0
175.10	5671.0
176.10	2066.0
177.00	2419.0
177.90	1480.0
179.00	12745.0
180.00	9697.0
181.00	4131.0
182.00	690.0
184.00	683.0
185.00	5792.0
186.00	46072.0
187.00	15545.0
188.00	1397.0
189.00	2656.0
191.00	1465.0
192.00	4225.0
193.00	4301.0
194.10	1048.0
194.90	547.0
195.90	9629.0
197.10	1837.0
198.00	363584.0
199.00	23280.0
200.10	2089.0
201.50	1908.0
202.10	451.0
203.00	2559.0
204.00	11851.0
205.00	21968.0
206.10	89320.0
207.10	11979.0
207.90	2914.0
209.10	1243.0
210.00	1631.0
210.90	3091.0
211.80	1099.0
213.00	311.0
215.00	1441.0
216.10	1797.0
217.00	24968.0
218.00	2928.0
221.00	14536.0
223.00	5036.0
224.10	49584.0
225.00	12136.0
226.00	1386.0
227.00	18912.0
228.10	2951.0
229.00	4173.0
230.00	710.0
231.10	1937.0
233.00	546.0
233.90	1261.0
234.90	1411.0
236.10	971.0
237.00	2033.0
238.90	631.0
240.10	457.0
240.90	1330.0
242.00	2921.0
243.10	3112.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

244.10	39368.0
245.00	5880.0
246.00	7044.0
247.00	1514.0
248.00	583.0
248.90	2102.0
250.80	337.0
253.10	956.0
254.10	1219.0
255.00	204864.0
256.00	29608.0
257.00	2339.0
258.00	10894.0
259.00	1710.0
259.90	337.0
261.00	356.0
264.00	319.0
265.00	4179.0
266.00	668.0
271.00	337.0
272.00	520.0
273.00	6376.0
274.00	15445.0
275.00	89432.0
276.00	11917.0
277.00	8784.0
277.90	1383.0
278.90	363.0
281.10	407.0
283.10	919.0
285.00	1671.0
292.80	975.0
293.90	517.0
295.00	669.0
296.00	23360.0
297.00	3029.0
301.00	410.0
302.00	547.0
303.10	2743.0
304.00	773.0
308.00	322.0
309.90	348.0
314.10	1257.0
315.00	2759.0
316.00	1350.0
321.10	491.0
322.10	537.0
323.10	7725.0
323.90	1724.0
326.90	959.0
327.90	669.0
331.80	394.0
333.00	858.0
334.10	4763.0
335.00	1161.0
341.00	1032.0
342.00	356.0
345.90	1577.0
352.00	2924.0
353.00	1913.0
354.10	2748.0
354.90	511.0
365.00	10556.0
365.90	1082.0
371.00	740.0
372.10	4662.0
373.00	1209.0
383.00	1391.0
383.80	390.0
390.00	607.0
390.90	561.0
392.10	466.0
401.00	343.0
401.90	1859.0
403.00	3467.0
404.00	1098.0
421.00	2238.0
422.00	2898.0
423.00	18792.0
424.00	5221.0
424.90	780.0
441.00	54768.0
442.00	374464.0
443.00	69088.0
444.10	7464.0
445.00	346.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z	Abundance
36.00	384.0
40.00	1177.0
44.00	6678.0
73.00	573.0
83.90	320.0
96.20	317.0
193.00	300.0
207.10	1573.0
281.00	359.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48