


Data Path : Z:\HPCHEM1\BNA M\DATA\BM041717\
 Data File : BM009646.D
 Acq On : 17 Apr 2017 12:54
 Operator : SJ/MA
 Sample : DFTPP01
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP01

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
 Title : SVOA CALIBRATION
 Last Update : Wed Nov 30 00:32:18 2016

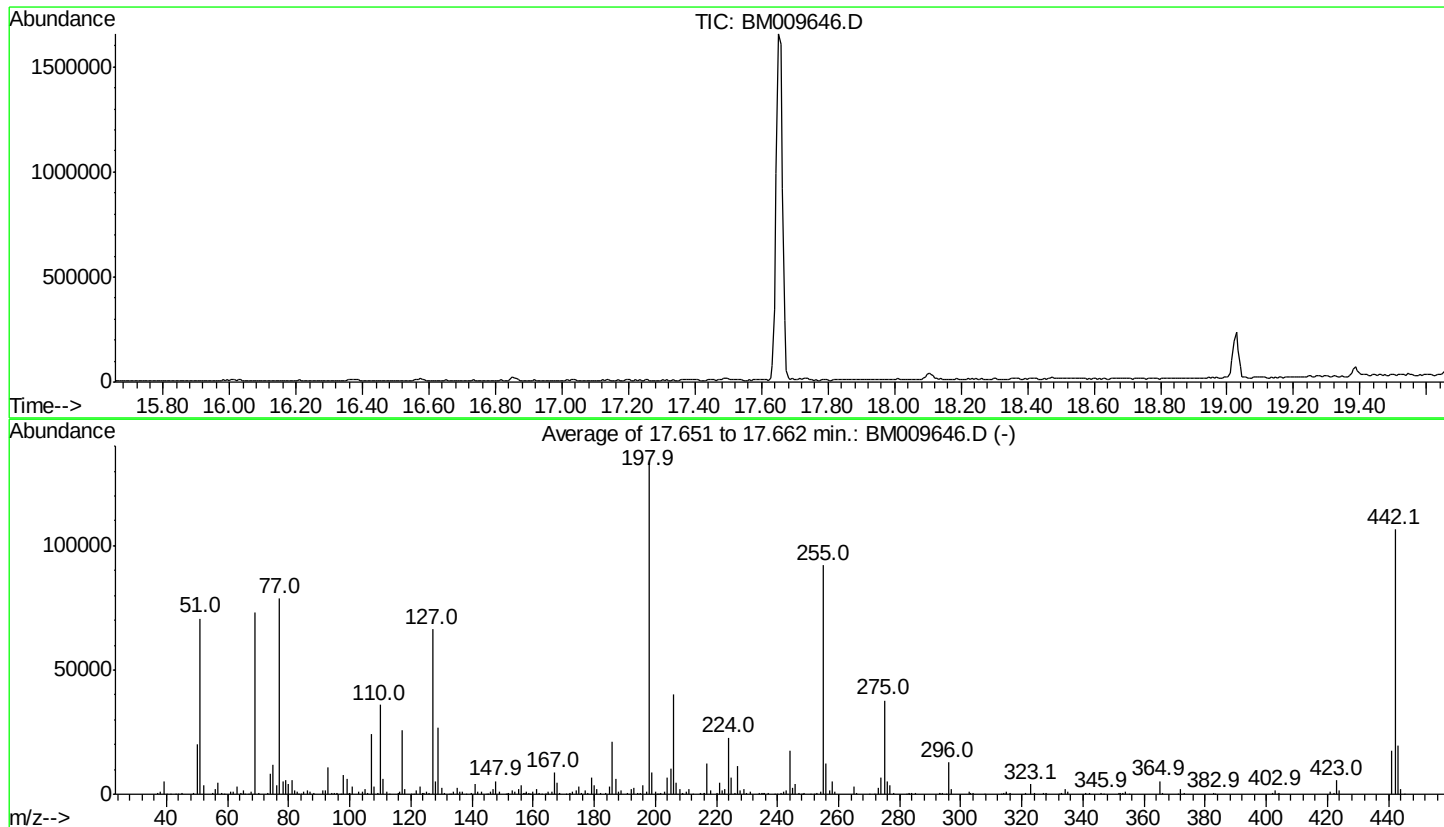

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	70622	PASS
68	69	0.00	2	1.7	1205	PASS
69	198	0.00	100	54.7	72924	PASS
70	69	0.00	2	0.8	619	PASS
127	198	10	80	49.7	66258	PASS
197	198	0.00	2	0.8	1117	PASS
198	198	100	100	100.0	133389	PASS
199	198	5	9	6.5	8707	PASS
275	198	10	60	28.2	37672	PASS
365	198	1	100	4.0	5380	PASS
441	443	0.01	100	88.3	17321	PASS
442	198	50	100	79.8	106381	PASS
443	442	15	24	18.4	19624	PASS

m/z	Abundance
39.20	430.0
40.00	637.0
41.00	431.0
42.90	516.0
44.00	1274.0
51.00	458.0
57.00	586.0
66.90	305.0
69.00	342.0
73.00	873.0
135.20	331.0
191.00	364.0
192.90	501.0
207.00	2093.0
209.10	407.0
281.10	579.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
37.00	812.0
38.10	1187.0
39.10	7587.0
40.00	1223.0
41.00	570.0
43.00	347.0
43.80	545.0
49.10	707.0
50.10	27488.0
51.00	91416.0
52.10	4827.0
55.10	945.0
56.00	2907.0
57.00	6982.0
58.00	457.0
60.90	1565.0
62.00	1764.0
63.00	3946.0
64.20	752.0
65.10	1626.0
67.00	363.0
67.90	1514.0
69.00	93064.0
70.00	968.0
73.10	1405.0
74.00	10306.0
75.00	15349.0
76.00	4652.0
77.00	104152.0
78.00	6809.0
79.00	6995.0
80.00	5954.0
81.00	7037.0
82.00	1511.0
82.90	1367.0
85.00	1840.0
86.00	2232.0
87.00	913.0
88.00	516.0
91.10	2833.0
92.00	2385.0
93.00	13690.0
94.10	572.0
94.90	567.0
95.80	738.0
98.00	10689.0
99.00	8128.0
100.10	732.0
101.00	3403.0
103.00	1843.0
104.10	1384.0
105.00	3093.0
105.90	457.0
107.00	29520.0
107.90	4611.0
109.10	598.0
110.00	45824.0
111.00	8791.0
112.00	1303.0
113.00	355.0
115.90	1673.0
117.00	31696.0
117.90	2289.0
120.10	350.0
121.10	536.0
122.00	2421.0
123.00	3425.0
123.90	2108.0
125.00	1138.0
126.00	396.0
127.00	86184.0
128.00	5486.0
129.00	33672.0
130.00	3011.0
131.10	312.0
132.80	636.0
134.00	1159.0
134.90	2466.0
136.10	1443.0
137.10	1771.0
138.10	331.0
140.00	303.0
141.00	4876.0
142.00	1611.0
143.00	1266.0
144.80	545.0
146.00	1194.0
146.90	2039.0
147.90	6307.0
148.90	1192.0
151.10	568.0
151.90	607.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

153.00	1748.0
154.00	1377.0
155.10	2697.0
156.00	4213.0
157.00	840.0
157.90	1138.0
158.80	853.0
160.00	1275.0
160.90	1851.0
162.00	757.0
162.90	350.0
164.00	329.0
165.10	1621.0
166.00	1019.0
167.00	11253.0
167.90	6117.0
168.90	875.0
170.90	324.0
171.90	1062.0
173.00	1475.0
174.00	1907.0
175.00	3469.0
175.90	1156.0
176.90	1986.0
177.90	635.0
179.00	7604.0
180.00	5293.0
181.00	2318.0
182.10	420.0
183.80	741.0
185.00	2587.0
186.00	26448.0
187.10	6748.0
187.90	1103.0
188.90	1545.0
191.00	1101.0
192.00	2509.0
193.00	3999.0
194.10	433.0
196.00	5115.0
196.90	1158.0
197.90	156288.0
199.00	11497.0
200.00	1338.0
200.70	345.0
201.40	676.0
203.00	1465.0
204.00	7835.0
205.00	12936.0
206.00	45312.0
207.00	8139.0
208.00	2754.0
208.80	938.0
210.30	967.0
211.10	1911.0
212.20	388.0
214.90	510.0
215.90	976.0
217.00	14380.0
218.00	2396.0
221.10	5575.0
221.90	1374.0
222.90	2432.0
224.00	23400.0
225.00	7732.0
225.90	643.0
226.90	12228.0
227.90	1203.0
229.00	1919.0
230.00	630.0
231.10	964.0
233.90	591.0
234.80	855.0
236.00	533.0
237.00	865.0
241.00	1154.0
242.00	1587.0
243.00	1992.0
244.00	19688.0
245.10	3974.0
245.90	4251.0
247.00	337.0
247.90	384.0
248.80	475.0
250.80	349.0
253.00	835.0
254.10	1061.0
255.00	108744.0
256.00	13089.0
257.00	1542.0
257.90	6602.0
258.90	1253.0
265.10	2859.0
271.90	366.0
273.00	2897.0
274.00	6239.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

275.00	40768.0
276.00	5418.0
277.00	4476.0
278.00	739.0
281.00	354.0
282.00	325.0
283.00	819.0
283.80	623.0
285.00	753.0
292.90	935.0
295.10	368.0
296.00	12530.0
296.90	2373.0
302.90	1785.0
304.00	436.0
307.90	374.0
313.90	372.0
314.80	1611.0
316.00	813.0
321.00	477.0
323.00	4420.0
324.10	1124.0
326.90	572.0
327.90	434.0
328.10	444.0
333.00	737.0
334.00	1900.0
335.10	816.0
341.10	662.0
342.20	520.0
346.00	868.0
351.90	1138.0
353.10	714.0
354.00	1289.0
355.20	395.0
364.90	5259.0
366.10	682.0
372.00	2131.0
373.00	539.0
382.90	664.0
402.10	503.0
402.90	1045.0
403.70	343.0
421.00	827.0
422.00	677.0
423.00	4751.0
424.00	1651.0
441.10	17856.0
442.10	104720.0
443.10	19432.0
444.10	2546.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
36.90	720.0
38.10	877.0
39.10	5306.0
40.00	935.0
41.20	345.0
43.00	708.0
44.00	820.0
44.90	464.0
49.00	869.0
50.00	22736.0
51.10	81976.0
52.10	3749.0
55.00	820.0
56.00	2478.0
57.00	5670.0
57.90	435.0
59.00	336.0
61.00	1221.0
62.00	1059.0
63.00	3424.0
64.10	532.0
65.00	1638.0
67.00	657.0
67.90	1596.0
69.00	84920.0
70.10	361.0
73.00	1617.0
74.00	9021.0
75.00	13206.0
76.00	4178.0
77.00	86432.0
78.10	5534.0
79.00	7006.0
80.00	3659.0
81.00	6528.0
82.10	1617.0
83.00	1282.0
84.80	821.0
86.00	1724.0
87.10	1039.0
88.10	624.0
91.00	2077.0
92.00	1652.0
93.00	12179.0
94.00	767.0
96.00	640.0
97.00	300.0
98.00	8854.0
99.00	7539.0
99.90	630.0
100.90	3209.0
103.00	734.0
103.90	1602.0
104.90	1990.0
106.00	712.0
107.00	28808.0
107.90	3337.0
108.90	962.0
110.00	40472.0
111.00	6606.0
111.90	720.0
116.10	1935.0
117.00	28952.0
117.90	2169.0
121.90	1349.0
122.90	3315.0
124.10	1138.0
124.80	1172.0
126.00	490.0
127.00	75272.0
128.00	6480.0
129.00	30408.0
130.00	3045.0
131.10	716.0
133.20	432.0
133.90	1311.0
135.00	3919.0
136.00	1589.0
136.90	1240.0
138.10	413.0
139.90	519.0
141.00	4627.0
142.10	983.0
143.00	1474.0
145.80	881.0
147.00	2782.0
147.90	6903.0
148.90	1089.0
152.00	738.0
153.00	1717.0
154.00	1391.0
155.00	2363.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

156.00	5293.0
157.20	536.0
157.90	1456.0
159.00	735.0
160.00	1392.0
161.00	2714.0
162.00	830.0
165.00	1808.0
166.00	1002.0
167.00	10171.0
167.90	4528.0
168.90	324.0
171.00	445.0
172.10	802.0
173.00	847.0
173.90	2325.0
175.10	3650.0
176.00	662.0
177.00	1578.0
178.00	757.0
179.00	7920.0
179.90	4056.0
180.90	2693.0
183.90	665.0
184.90	4584.0
186.00	25568.0
187.00	7939.0
188.00	1025.0
189.00	1919.0
191.00	1759.0
192.10	1852.0
192.90	3387.0
195.00	455.0
196.00	3923.0
197.00	1155.0
197.90	159616.0
198.90	9779.0
199.90	898.0
201.10	490.0
201.80	709.0
203.00	1530.0
204.00	8711.0
205.00	9703.0
206.00	46984.0
207.00	7532.0
208.00	1869.0
209.00	991.0
210.10	887.0
211.00	2571.0
212.20	318.0
215.00	1046.0
216.10	1438.0
217.00	14854.0
217.90	1712.0
220.10	986.0
221.00	5334.0
221.70	3203.0
222.90	2686.0
224.00	28256.0
225.00	6939.0
226.00	641.0
227.00	12721.0
227.90	2258.0
229.00	2633.0
229.90	530.0
231.10	995.0
233.90	512.0
235.10	1102.0
235.80	701.0
237.00	882.0
239.00	557.0
241.00	551.0
242.00	942.0
243.00	1799.0
244.00	22304.0
245.00	2500.0
246.00	4976.0
247.00	588.0
248.90	358.0
252.00	524.0
252.90	504.0
253.90	733.0
255.00	104408.0
256.00	14079.0
257.00	1844.0
258.00	5355.0
258.90	1429.0
264.90	3266.0
265.80	526.0
270.20	307.0
273.10	3458.0
274.00	8712.0
275.00	44200.0
276.00	6644.0
276.90	3930.0
277.90	1207.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

281.10	498.0
283.20	341.0
283.80	465.0
285.00	1024.0
293.10	742.0
294.10	724.0
296.00	16221.0
296.90	1813.0
302.90	2007.0
304.00	670.0
314.00	588.0
315.00	1975.0
316.00	1429.0
321.10	406.0
323.10	3801.0
323.90	795.0
326.90	851.0
328.00	448.0
331.90	568.0
333.00	508.0
334.00	2371.0
335.00	823.0
341.10	630.0
342.20	322.0
345.90	904.0
351.90	699.0
353.00	865.0
354.00	1177.0
365.00	5606.0
366.10	1016.0
370.90	572.0
372.00	2743.0
373.00	834.0
382.90	814.0
402.00	957.0
403.00	1657.0
404.00	674.0
421.10	1130.0
422.00	1093.0
423.00	6818.0
424.00	1738.0
441.10	18992.0
442.10	122816.0
443.10	23464.0
444.10	2500.0
445.00	396.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	413.0
39.00	4241.0
39.90	581.0
41.00	603.0
43.10	591.0
43.90	629.0
45.00	391.0
49.00	456.0
50.10	10486.0
51.00	39848.0
52.00	2257.0
55.00	560.0
56.00	1131.0
57.10	2752.0
60.90	641.0
62.00	653.0
63.10	1437.0
65.10	732.0
65.80	348.0
67.80	505.0
69.00	41816.0
70.00	530.0
73.10	898.0
74.10	6178.0
75.00	6334.0
75.90	2513.0
77.00	45384.0
78.00	3348.0
79.10	3651.0
80.10	2480.0
81.10	3224.0
82.00	934.0
82.90	478.0
83.30	431.0
84.00	358.0
85.10	449.0
86.00	1428.0
87.00	483.0
91.10	541.0
91.80	1024.0
92.90	6580.0
95.00	448.0
95.90	511.0
97.90	4192.0
99.00	3550.0
99.70	361.0
101.00	2011.0
103.10	800.0
103.80	894.0
104.90	1468.0
106.10	315.0
107.00	15088.0
108.00	1721.0
109.00	597.0
110.00	21208.0
110.90	3663.0
112.10	643.0
115.80	475.0
116.00	469.0
117.00	16776.0
118.00	1042.0
122.00	1326.0
122.80	2140.0
125.00	764.0
126.10	580.0
127.00	37320.0
128.00	3152.0
129.00	16752.0
130.00	1612.0
131.10	732.0
133.90	853.0
134.90	2015.0
136.10	658.0
136.90	721.0
139.90	512.0
141.00	2930.0
141.90	977.0
142.90	668.0
145.00	531.0
145.80	466.0
147.00	1246.0
147.90	2874.0
148.90	771.0
151.30	574.0
151.90	556.0
153.00	1028.0
153.80	549.0
155.00	1364.0
155.90	1939.0
157.10	588.0
157.80	318.0
159.90	918.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

161.10	994.0
162.00	444.0
164.20	315.0
164.80	800.0
166.10	646.0
166.90	4698.0
167.90	3907.0
168.80	1062.0
171.90	817.0
173.00	870.0
174.00	791.0
174.90	2024.0
176.00	503.0
176.80	918.0
177.80	622.0
178.90	4684.0
180.00	2271.0
181.00	1122.0
181.90	581.0
185.00	2381.0
186.00	11241.0
186.90	3551.0
187.90	428.0
189.00	1331.0
190.90	383.0
191.90	1953.0
193.00	1584.0
194.00	480.0
195.00	454.0
196.10	1554.0
197.10	1040.0
198.00	84264.0
198.90	4847.0
200.00	692.0
201.80	487.0
202.80	589.0
204.00	3972.0
205.00	9008.0
206.00	27752.0
207.00	4464.0
207.90	1380.0
208.90	746.0
210.10	666.0
211.10	1469.0
214.70	352.0
217.00	7681.0
218.00	533.0
221.00	3319.0
222.10	709.0
222.90	1283.0
224.00	16456.0
225.00	5144.0
226.10	373.0
226.90	9154.0
227.90	1790.0
228.80	1145.0
231.00	419.0
234.00	472.0
234.80	446.0
237.10	617.0
240.00	349.0
240.80	625.0
242.10	1058.0
243.00	693.0
244.00	10600.0
245.00	1650.0
246.00	2487.0
247.00	436.0
248.10	315.0
248.90	477.0
254.00	785.0
255.00	62816.0
256.00	10177.0
256.90	1363.0
258.00	3296.0
258.90	511.0
264.90	3176.0
265.80	736.0
272.90	2005.0
274.00	5860.0
275.00	28048.0
276.00	3445.0
277.00	2482.0
281.00	627.0
283.00	674.0
293.00	480.0
294.10	301.0
296.00	9715.0
296.90	1524.0
303.10	1136.0
304.00	375.0
313.00	360.0
313.90	733.0
314.90	1037.0
315.70	429.0
321.10	562.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

323.00	3802.0
323.90	427.0
326.80	780.0
332.70	421.0
334.00	1858.0
335.00	803.0
340.90	387.0
345.90	482.0
346.90	306.0
352.10	1099.0
353.10	355.0
354.00	681.0
365.00	5276.0
366.10	529.0
372.10	1820.0
382.70	417.0
383.10	432.0
403.00	1213.0
404.10	376.0
421.10	901.0
421.80	502.0
423.00	5137.0
424.00	1068.0
441.00	15116.0
442.10	91608.0
443.00	15978.0
444.10	1607.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01