

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
 Data File : BM014715.D
 Acq On : 17 Apr 2018 10:12
 Operator : SJ/JU
 Sample : J2313-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 17 13:53:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 14 01:12:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.57	152	443921	20.00	ng/ul	0.00
18) Naphthalene-d8	11.42	136	1974885	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.17	164	1118562	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.88	188	2549766	20.00	ng/ul	0.00
77) Chrysene-d12	21.96	240	2508003	20.00	ng/ul	0.00
85) Perylene-d12	24.47	264	2210248	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.69	96	36087	3.91	ng/uL	0.00
5) Phenol-d5	7.69	99	260687	7.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.87	67	730312	32.79	ng/ul	0.00
9) 2-Chlorophenol-d4	8.09	132	783085	26.81	ng/ul	0.00
13) 4-Methylphenol-d8	9.26	113	514245	17.78	ng/ul	0.00
19) Nitrobenzene-d5	9.75	128	470645	37.06	ng/ul	0.00
22) 2-Nitrophenol-d4	10.48	143	491465	43.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.02	165	898986	30.82	ng/ul	0.00
29) 4-Chloroaniline-d4	11.53	131	156249	4.74	ng/ul	0.00
43) Dimethylphthalate-d6	14.56	166	2937935	33.24	ng/ul	0.00
46) Acenaphthylene-d8	14.87	160	3701287	32.97	ng/ul	0.00
51) 4-Nitrophenol-d4	15.32	143	105976	7.39	ng/ul	0.00
57) Fluorene-d10	16.14	176	2507563	32.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.24	200	425721	39.11	ng/ul	0.00
70) Anthracene-d10	17.97	188	3833571	31.92	ng/ul	0.00
78) Pyrene-d10	20.21	212	4179251	32.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.31	264	3420215	31.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.62	163	86184	1.012	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
Data File : BM014715.D
Acq On : 17 Apr 2018 10:12
Operator : SJ/JU
Sample : J2313-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 17 13:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 14 01:12:03 2018
Response via : Initial Calibration

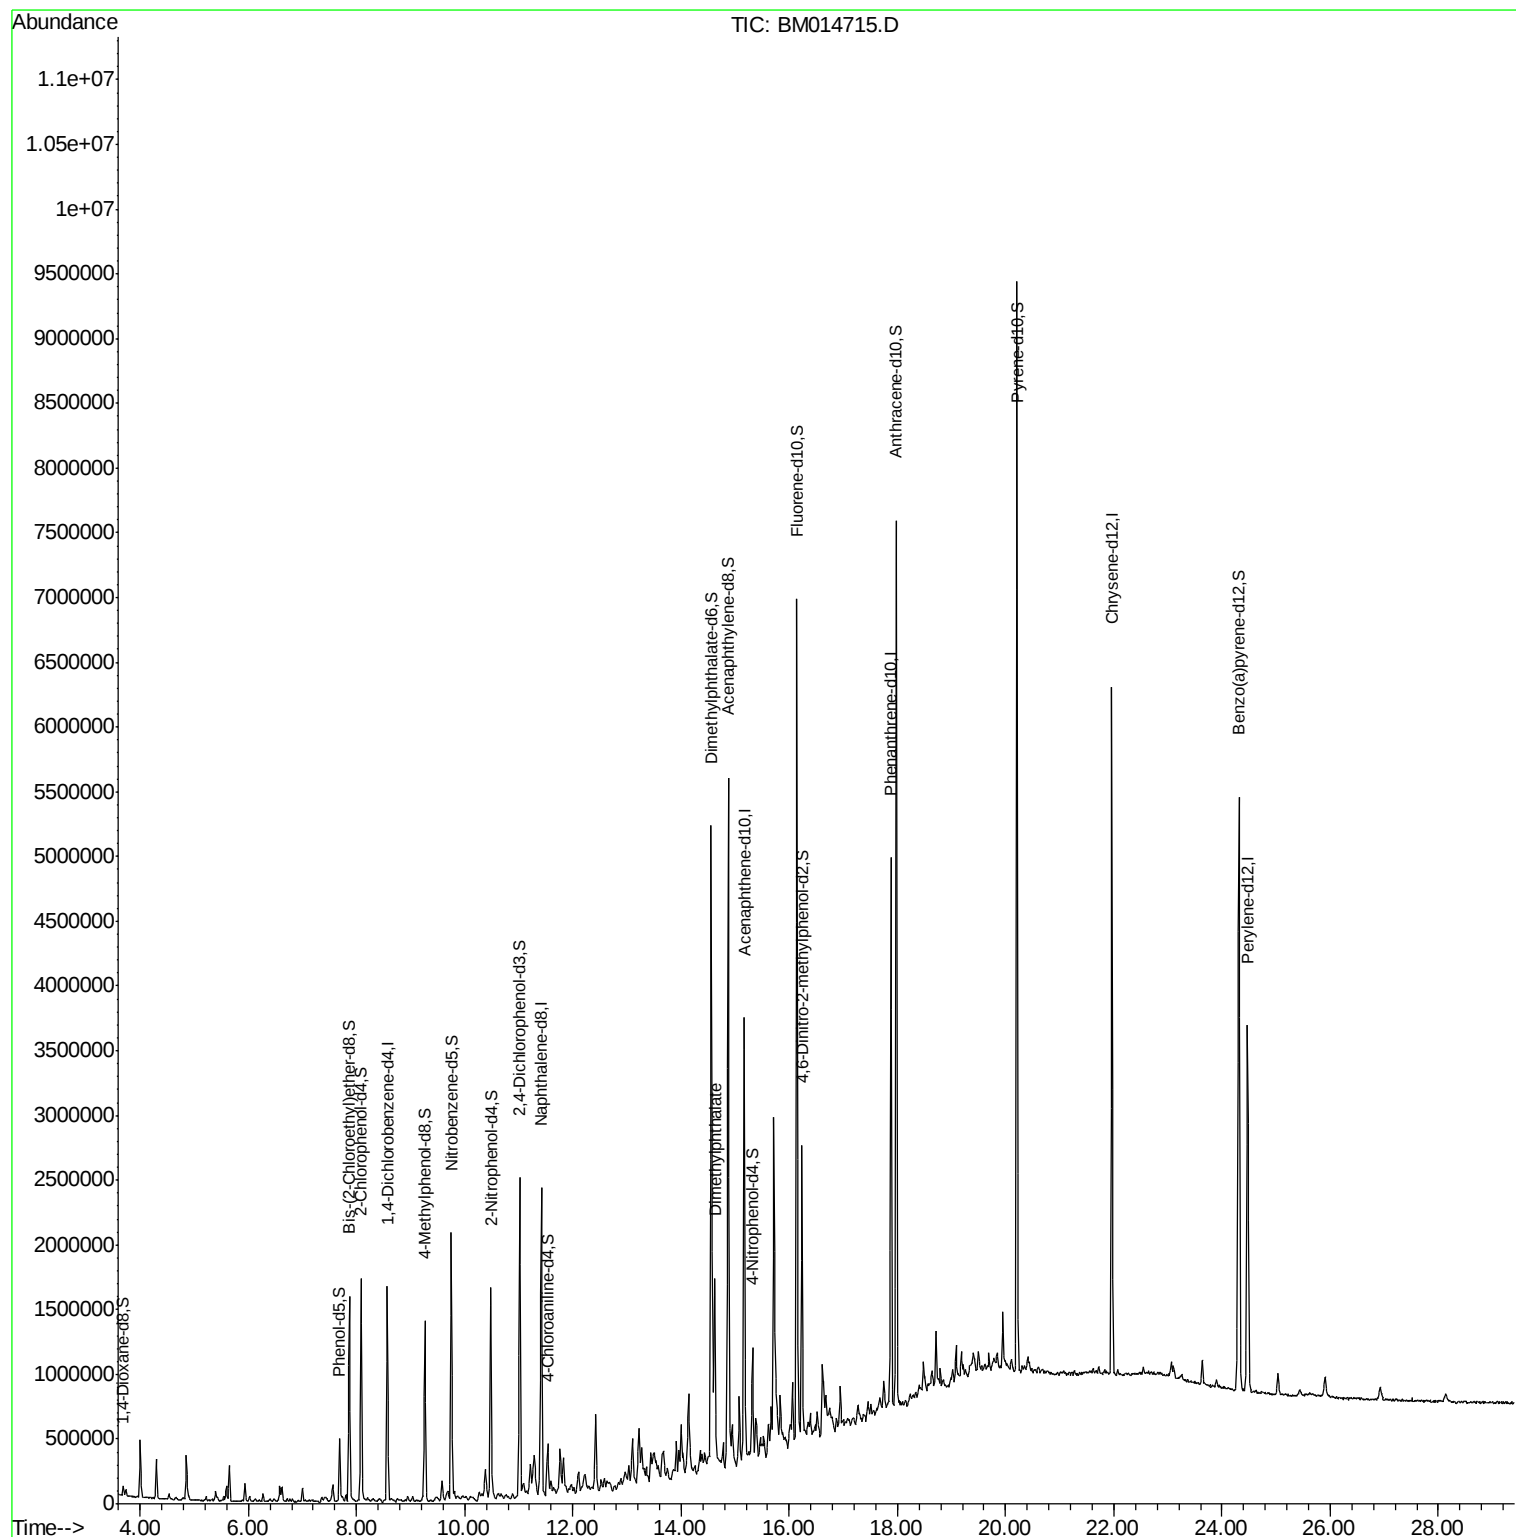

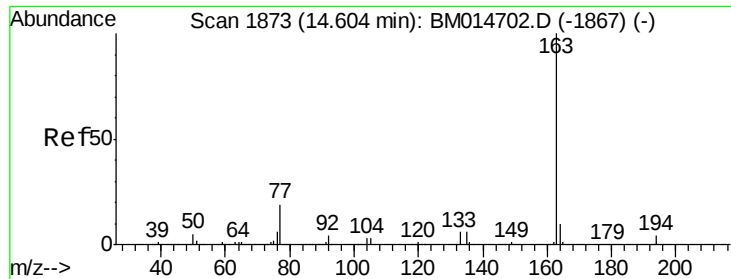

#44

Dimethylphthalate

Concen: 1.012 ng/ul

RT: 14.62 min Scan# 1875

Delta R.T. 0.01 min

Lab File: BM014715.D

Acq: 17 Apr 2018 10:12

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 86184

Ion Ratio Lower Upper

163 100

194 0.9 3.2 4.8#

164 18.7 7.8 11.8#

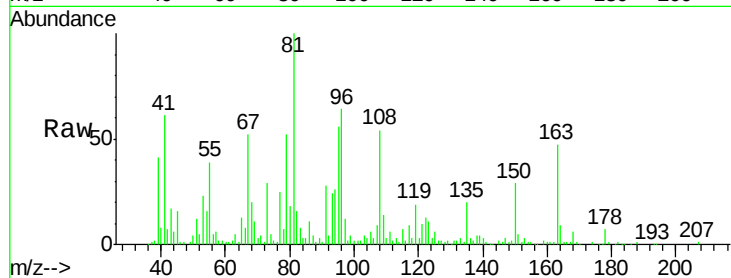

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

