

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
 Data File : BM014717.D
 Acq On : 17 Apr 2018 11:23
 Operator : SJ/JU
 Sample : J2313-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 17 13:53:46 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 14 01:12:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.57	152	542678	20.00	ng/ul	0.00
18) Naphthalene-d8	11.42	136	2339287	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.17	164	1278000	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.88	188	2483509	20.00	ng/ul	0.00
77) Chrysene-d12	21.96	240	1744515	20.00	ng/ul	0.00
85) Perylene-d12	24.47	264	1601602	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.69	96	77323	6.86	ng/uL	0.00
5) Phenol-d5	7.69	99	269285	6.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.87	67	817160	30.02	ng/ul	0.00
9) 2-Chlorophenol-d4	8.09	132	859948	24.08	ng/ul	0.00
13) 4-Methylphenol-d8	9.26	113	538648	15.24	ng/ul	0.00
19) Nitrobenzene-d5	9.75	128	525800	34.95	ng/ul	0.00
22) 2-Nitrophenol-d4	10.48	143	557813	41.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.02	165	963972	27.90	ng/ul	0.00
29) 4-Chloroaniline-d4	11.53	131	130783	3.35	ng/ul	0.00
43) Dimethylphthalate-d6	14.56	166	2864124	28.36	ng/ul	0.00
46) Acenaphthylene-d8	14.87	160	3775545	29.44	ng/ul	0.00
51) 4-Nitrophenol-d4	15.33	143	85179	5.20	ng/ul	0.00
57) Fluorene-d10	16.15	176	2426741	27.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.24	200	395898	37.34	ng/ul	0.00
70) Anthracene-d10	17.97	188	3372643	28.83	ng/ul	0.00
78) Pyrene-d10	20.21	212	3061756	34.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.32	264	2185640	27.79	ng/ul	0.00


Target Compounds				Ovalue	
17) Hexachloroethane	9.69	117	37884	2.651	ng/ul# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
Data File : BM014717.D
Acq On : 17 Apr 2018 11:23
Operator : SJ/JU
Sample : J2313-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 17 13:53:46 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 14 01:12:03 2018
Response via : Initial Calibration

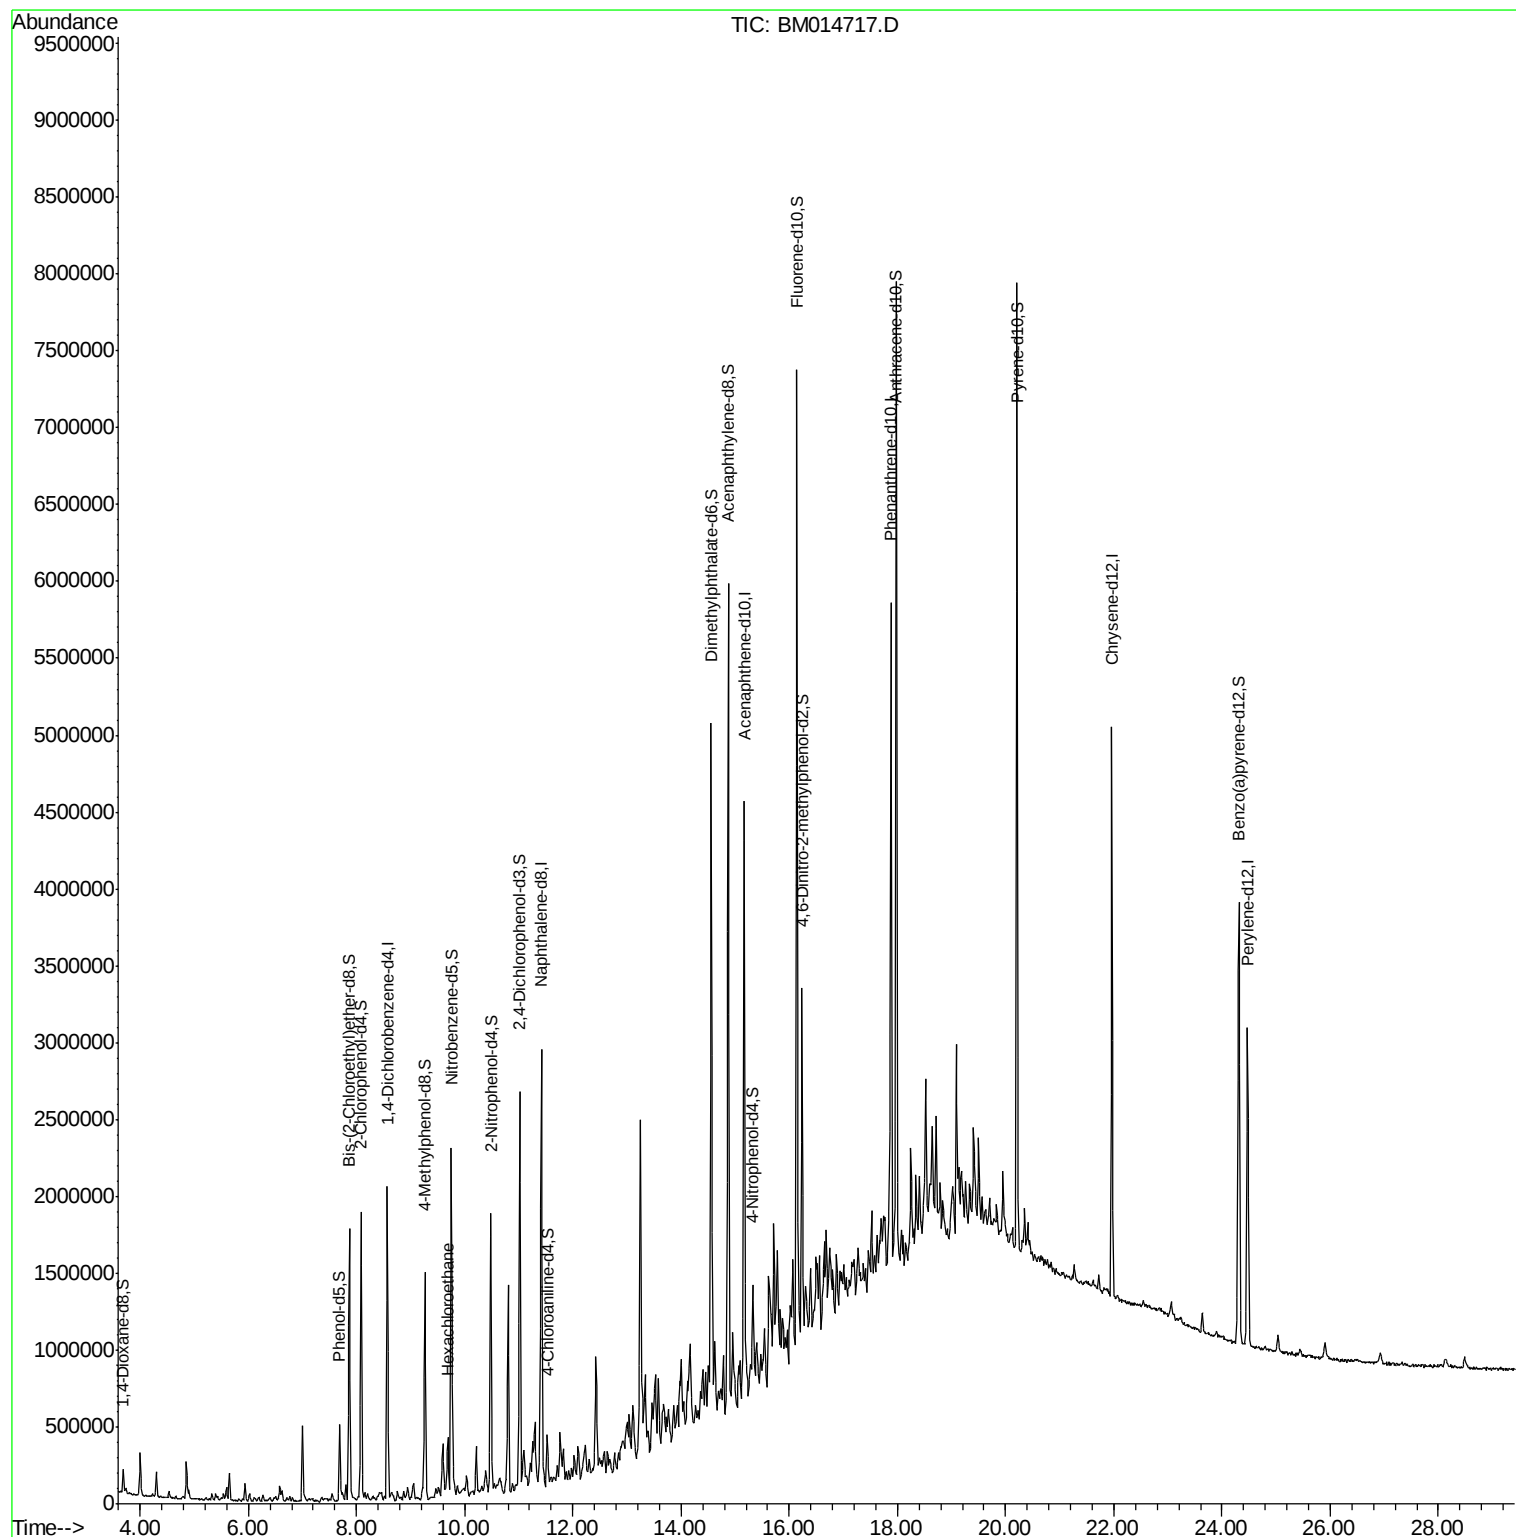

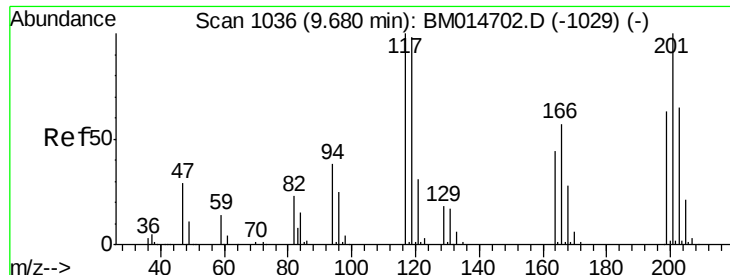

#17

Hexachloroethane

Concen: 2.651 ng/ul

RT: 9.69 min Scan# 1038

Delta R.T. 0.01 min

Lab File: BM014717.D

Acq: 17 Apr 2018 11:23

Instrument :

BNA_M

ClientSampleId :


Tot Ion:117 Resp: 37884

Ion Ratio Lower Upper

117 100

201 0.0 81.5 122.3#

199 0.0 50.6 76.0#

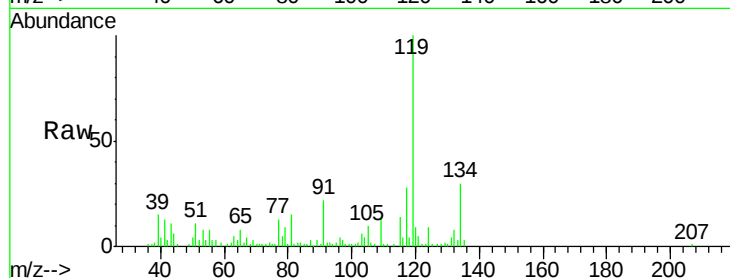

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

