

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
 Data File : BM014714.D
 Acq On : 17 Apr 2018 09:36
 Operator : SJ/JU
 Sample : PB108285BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032818MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	13	17	25	rVB	127141	191955	1.59%	0.151%
2	7.687	690	697	711	rBV	2165920	3479475	28.79%	2.729%
3	7.869	721	728	737	rBV	1706336	2724547	22.54%	2.137%
4	8.087	757	765	778	rVB	2102141	3470748	28.72%	2.722%
5	8.569	839	847	855	rVB	1748222	2916017	24.13%	2.287%
6	9.263	957	965	977	rBV	2772146	4518965	37.39%	3.544%
7	9.752	1039	1048	1056	rBV	2154003	3624258	29.99%	2.842%
8	10.481	1163	1172	1186	rBV	1661724	2826122	23.38%	2.216%
9	11.016	1255	1263	1274	rBV	2620450	4467381	36.97%	3.503%
10	11.416	1323	1331	1339	rVB	2548737	4429415	36.65%	3.474%
11	11.534	1342	1351	1363	rBV	2845624	4937740	40.86%	3.872%
12	14.557	1858	1865	1872	rBV	5424306	7435262	61.52%	5.831%
13	14.869	1910	1918	1931	rBV	6010321	8895645	73.61%	6.976%
14	15.169	1961	1969	1977	rBV2	3804041	5892745	48.76%	4.621%
15	15.322	1988	1995	2008	rBV	2395064	3556250	29.43%	2.789%
16	16.145	2127	2135	2142	rBV	7228372	10796135	89.33%	8.467%
17	16.239	2144	2151	2164	rBV	2054828	2817789	23.32%	2.210%
18	16.381	2169	2175	2180	rVB	86554	130027	1.08%	0.102%
19	17.880	2423	2430	2438	rVB2	4524281	6579369	54.44%	5.160%
20	17.975	2439	2446	2462	rBV2	7879561	11371848	94.10%	8.918%
21	20.210	2820	2826	2836	rBV	9130437	12085211	100.00%	9.477%
22	21.962	3118	3124	3131	rBV	4574561	6113197	50.58%	4.794%
23	24.315	3516	3524	3538	rVB2	4345892	9312632	77.06%	7.303%
24	24.474	3544	3551	3561	rVB2	2337450	4943060	40.90%	3.876%


Sum of corrected areas: 127515793

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041718\
Data File : BM014714.D
Acq On : 17 Apr 2018 09:36
Operator : SJ/JU
Sample : PB108285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

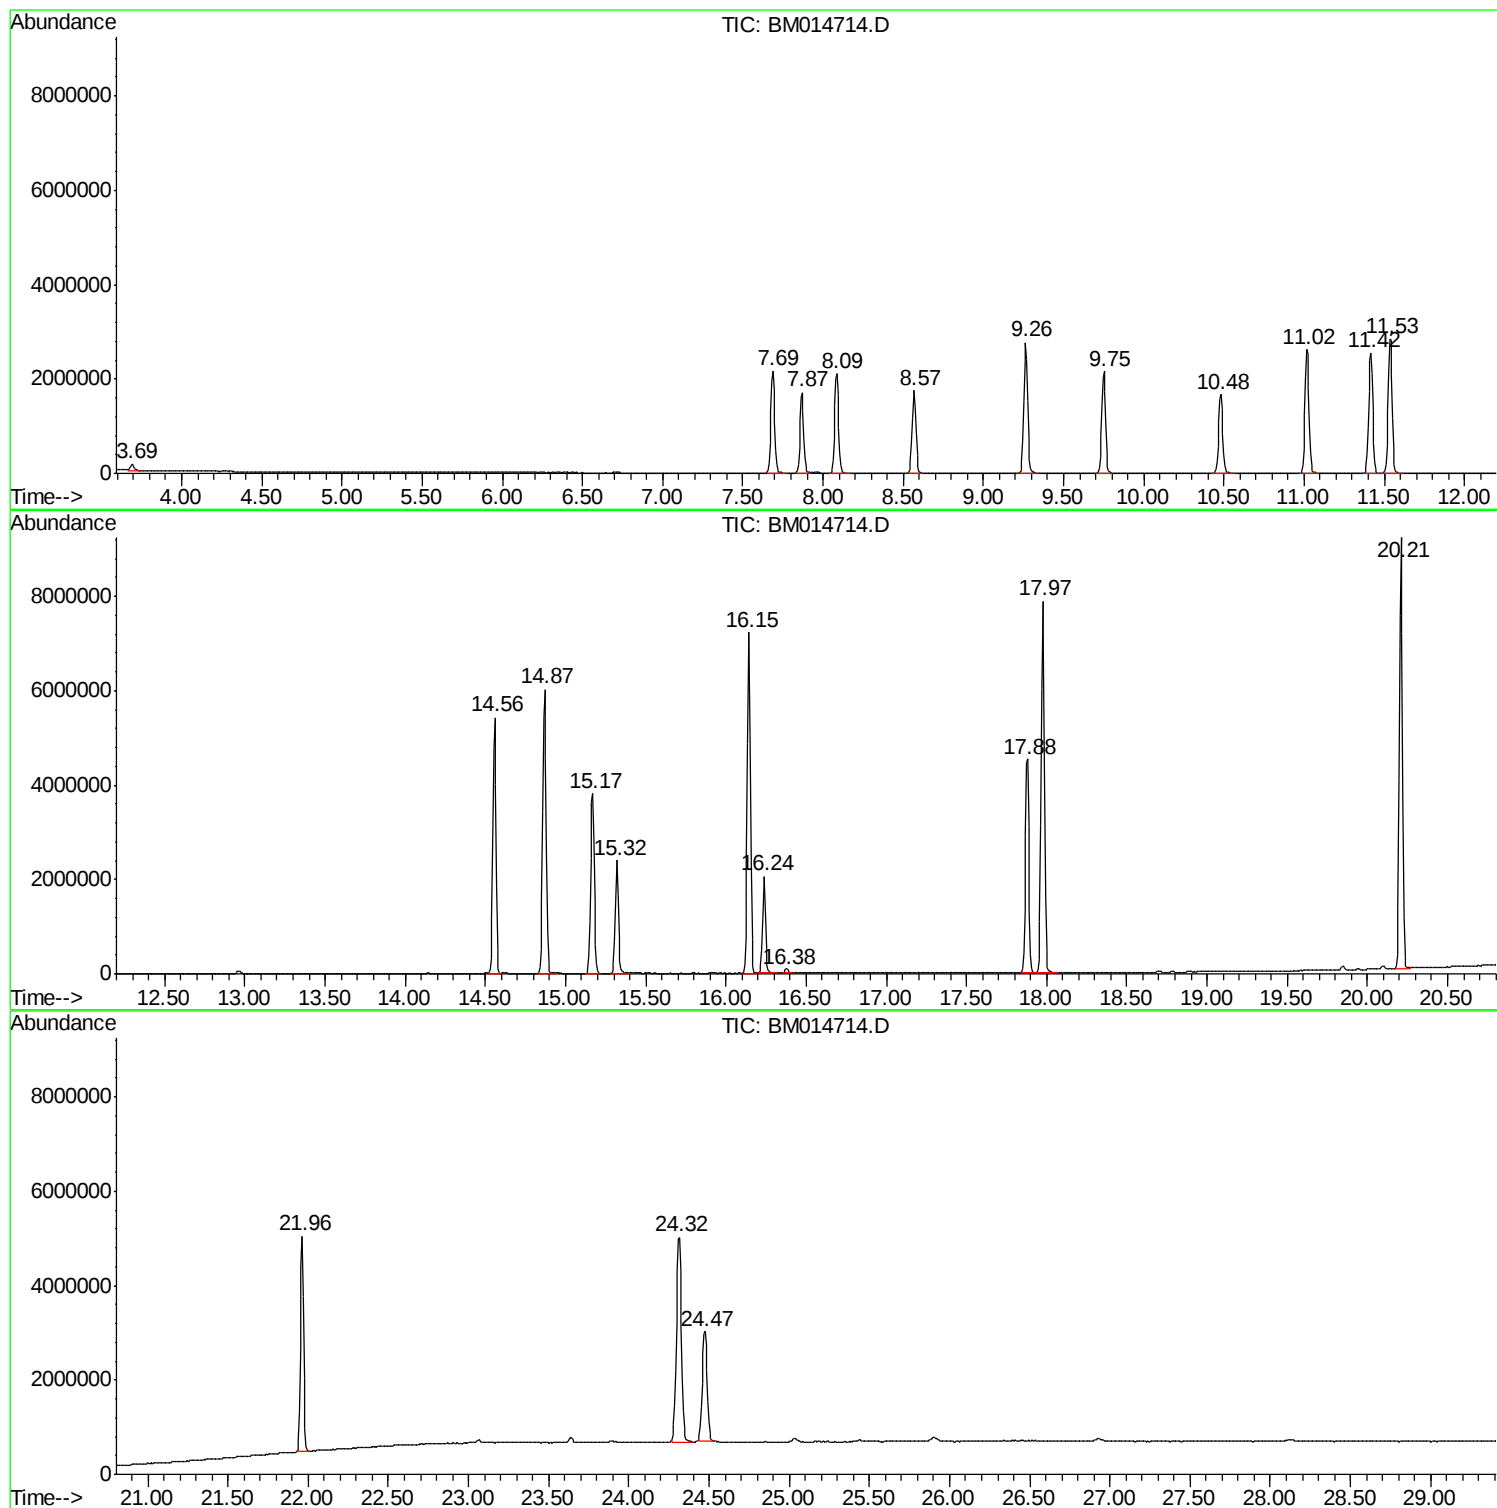

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041718\
Data File : BM014714.D
Acq On : 17 Apr 2018 09:36
Operator : SJ/JU
Sample : PB108285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041718\
Data File : BM014714.D
Acq On : 17 Apr 2018 09:36
Operator : SJ/JU
Sample : PB108285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc