
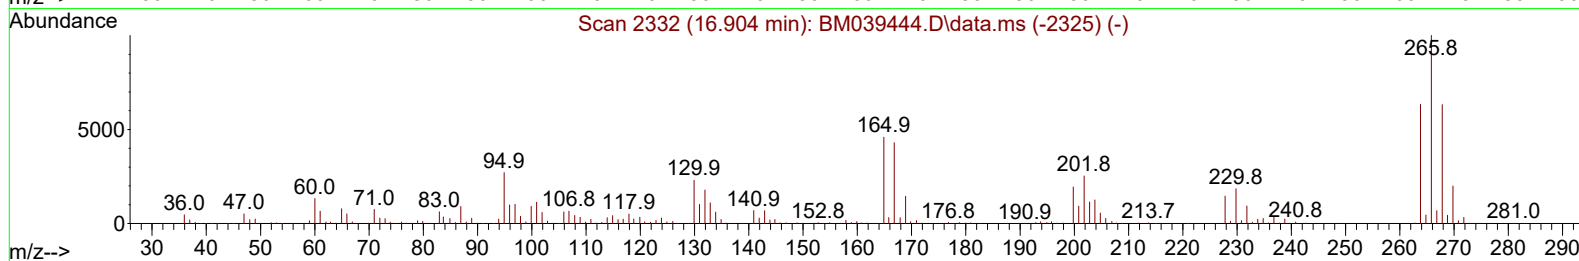
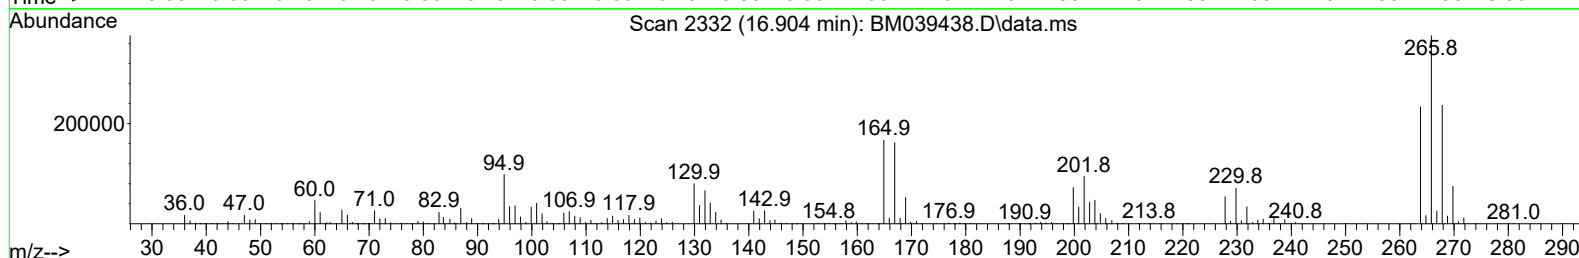


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041723\
Data File : BM039438.D
Acq On : 17 Apr 2023 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 06:50:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 03:04:14 2023
Response via : Initial Calibration

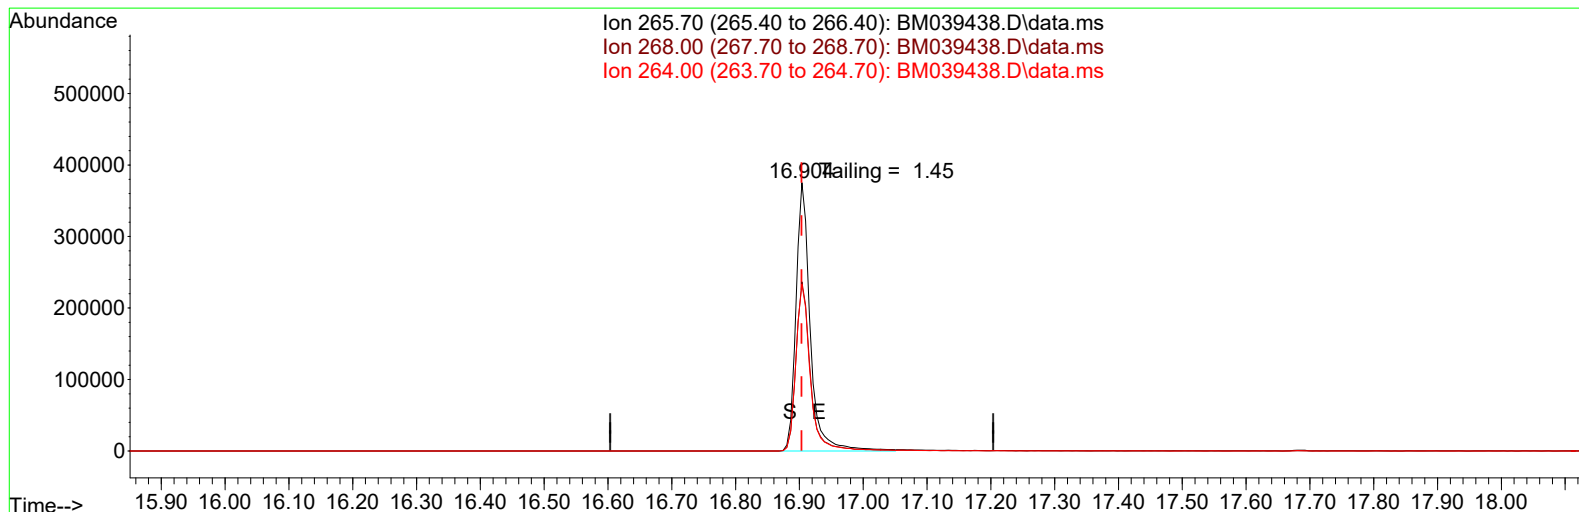

TIC: BM039438.D\data.ms

(70) Pentachlorophenol (C)




16.904min (+ 0.000) 1372167.47 ng

response 591459

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.00
264.00	63.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041723\
Data File : BM039438.D
Acq On : 17 Apr 2023 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 06:50:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 03:04:14 2023
Response via : Initial Calibration

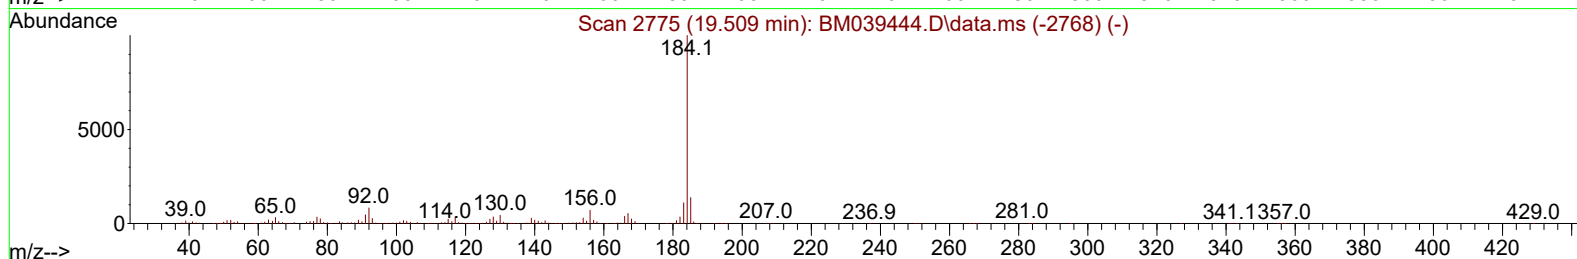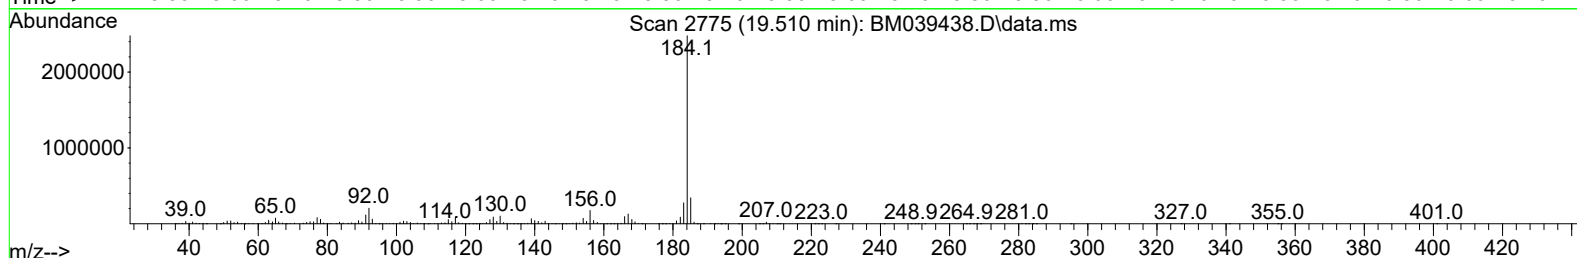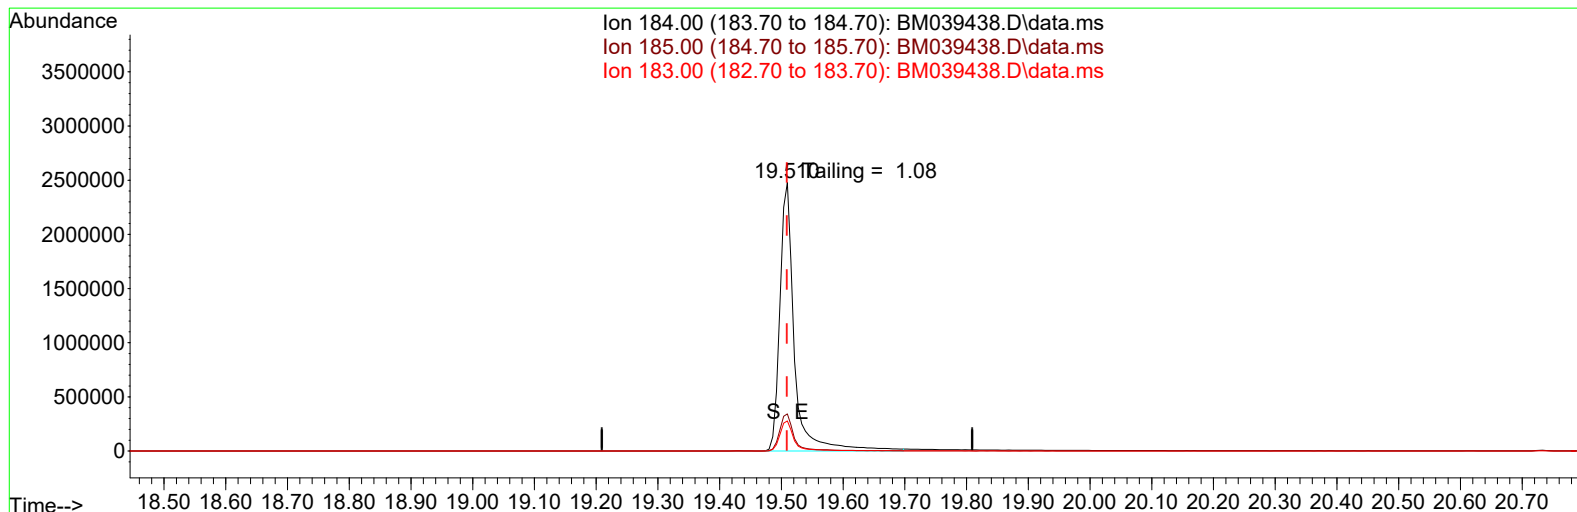

TIC: BM039438.D\data.ms

(77) Benzidine**19.510min (+ 0.000) 114950.11 ng****response 4141508**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.84
183.00	11.00	11.20
0.00	0.00	0.00