
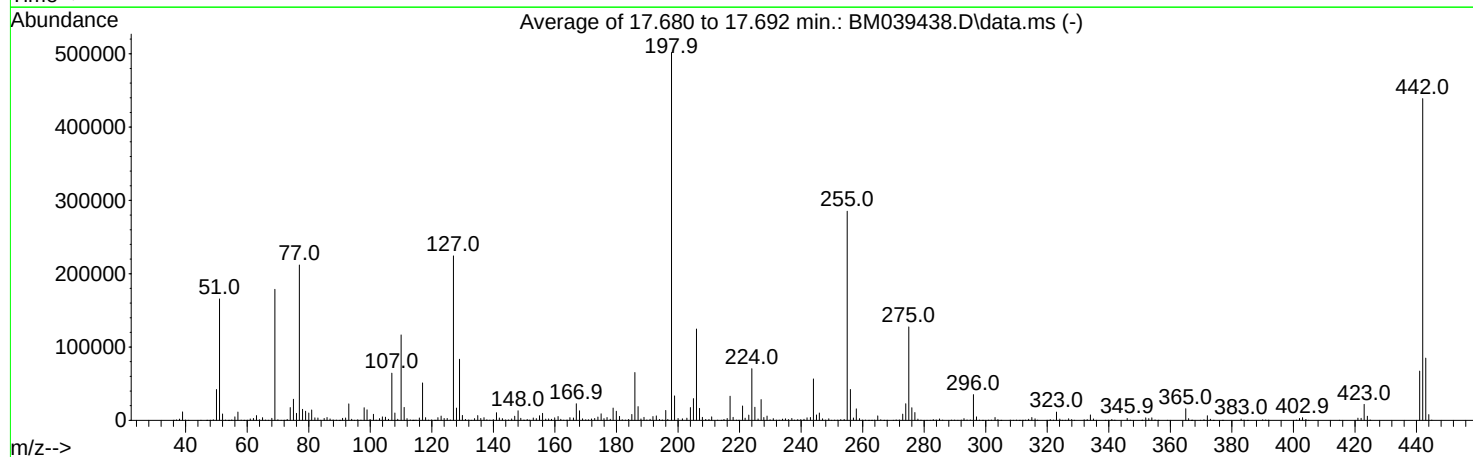


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041723\
Data File : BM039438.D
Acq On : 17 Apr 2023 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 18 03:04:14 2023

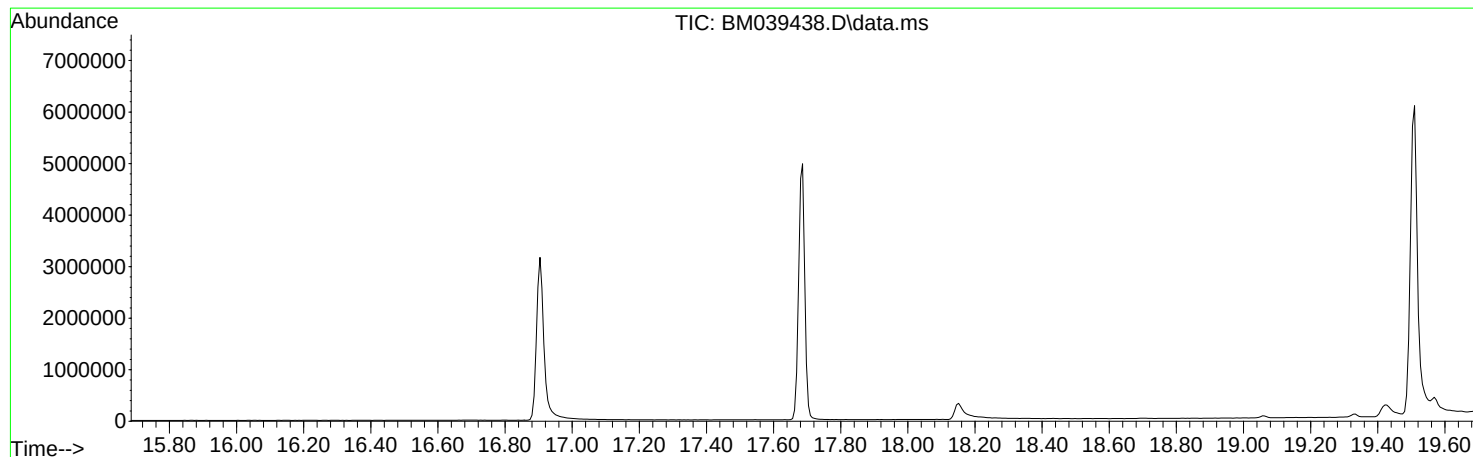

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	165758	PASS
68	69	0.00	2	1.5	2766	PASS
69	198	0.00	100	35.6	178702	PASS
70	69	0.00	2	0.5	977	PASS
127	198	10	80	44.7	224277	PASS
197	198	0.00	2	0.3	1352	PASS
198	198	100	100	100.0	501781	PASS
199	198	5	9	6.7	33467	PASS
275	198	10	60	25.4	127573	PASS
365	198	1	100	3.2	16008	PASS
441	198	0.01	100	13.4	67347	PASS
442	442	50	100	100.0	439019	PASS
443	442	15	24	19.3	84893	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/17/2023	BNA_M	<u>BM039438.D</u>
Compound Name	Response	Retention Time
DDT	1722063	20.733
DDD	24767	20.339
DDE	1434	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26201	1748264	1.50

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041723\
Data File : BM039438.D
Acq On : 17 Apr 2023 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 18 06:50:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 03:04:14 2023
Response via : Initial Calibration

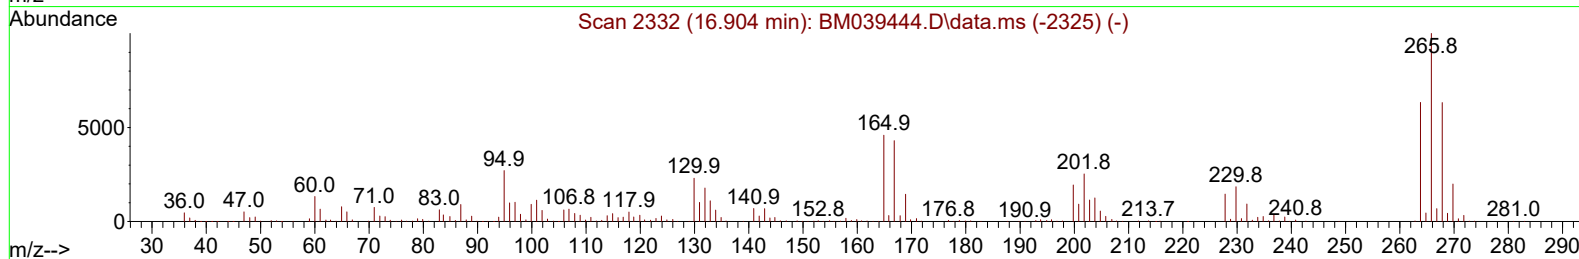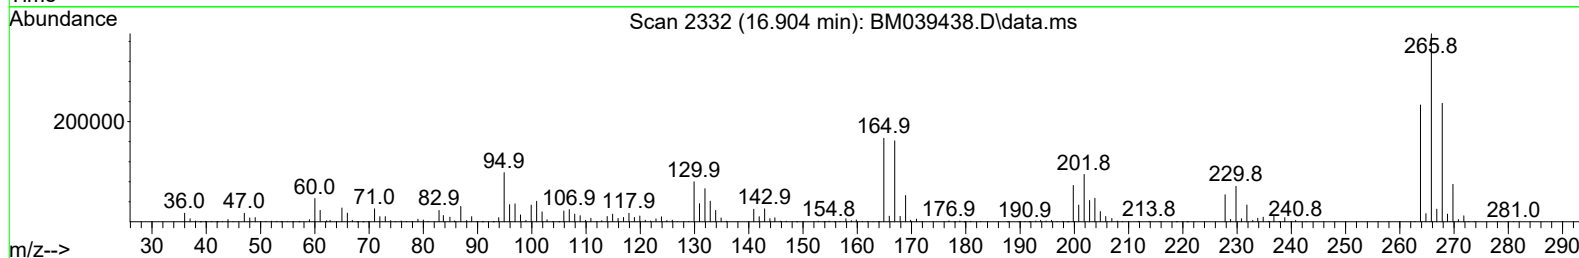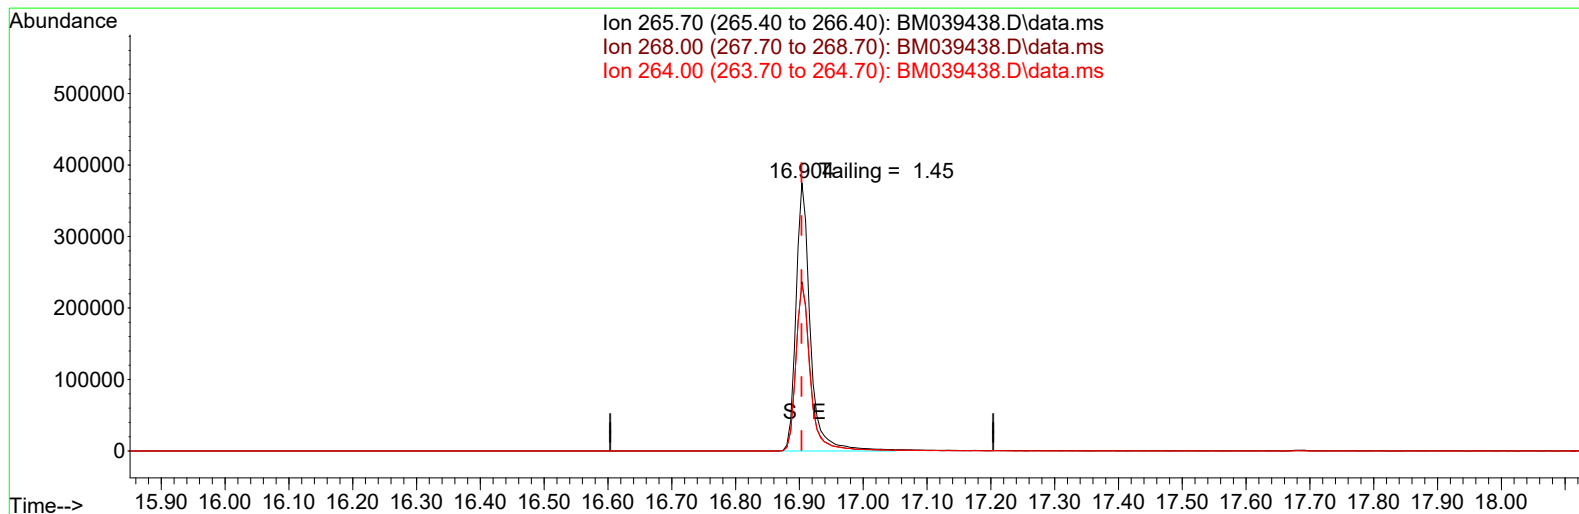

TIC: BM039438.D\data.ms

(70) Pentachlorophenol (C)

16.904min (+ 0.000) 1372167.47 ng




response 591459

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.00
264.00	63.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041723\
 Data File : BM039438.D
 Acq On : 17 Apr 2023 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 18 06:50:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 03:04:14 2023
 Response via : Initial Calibration

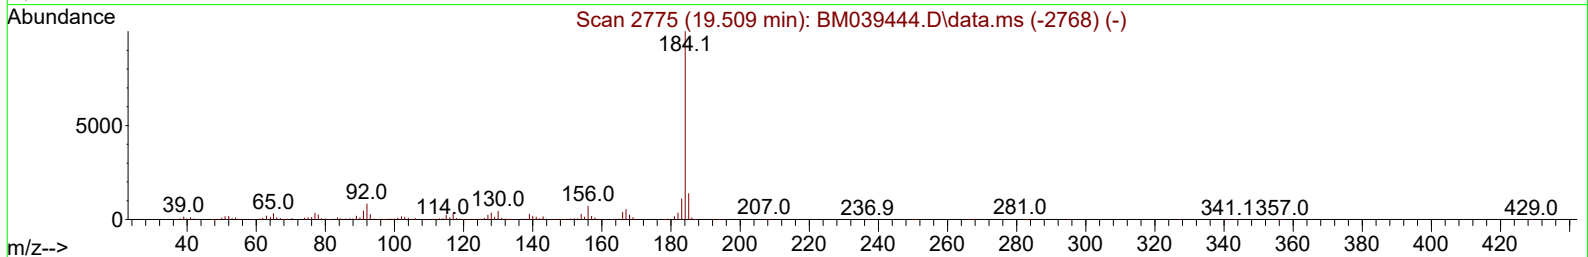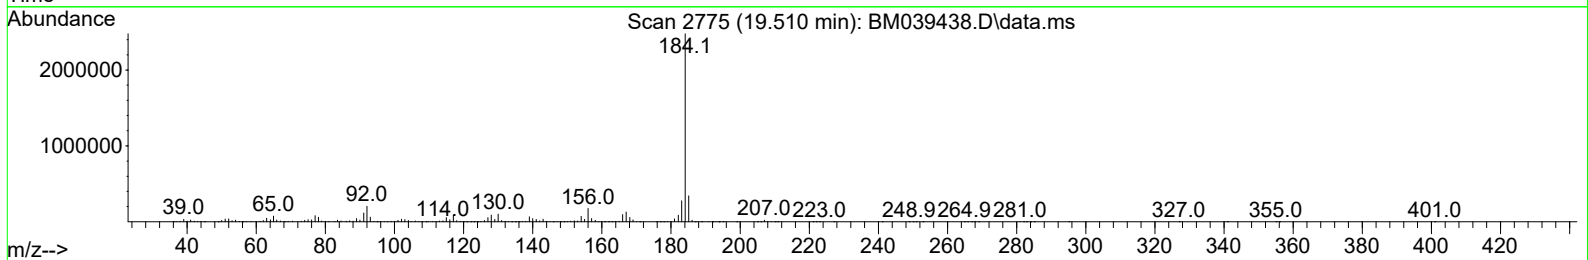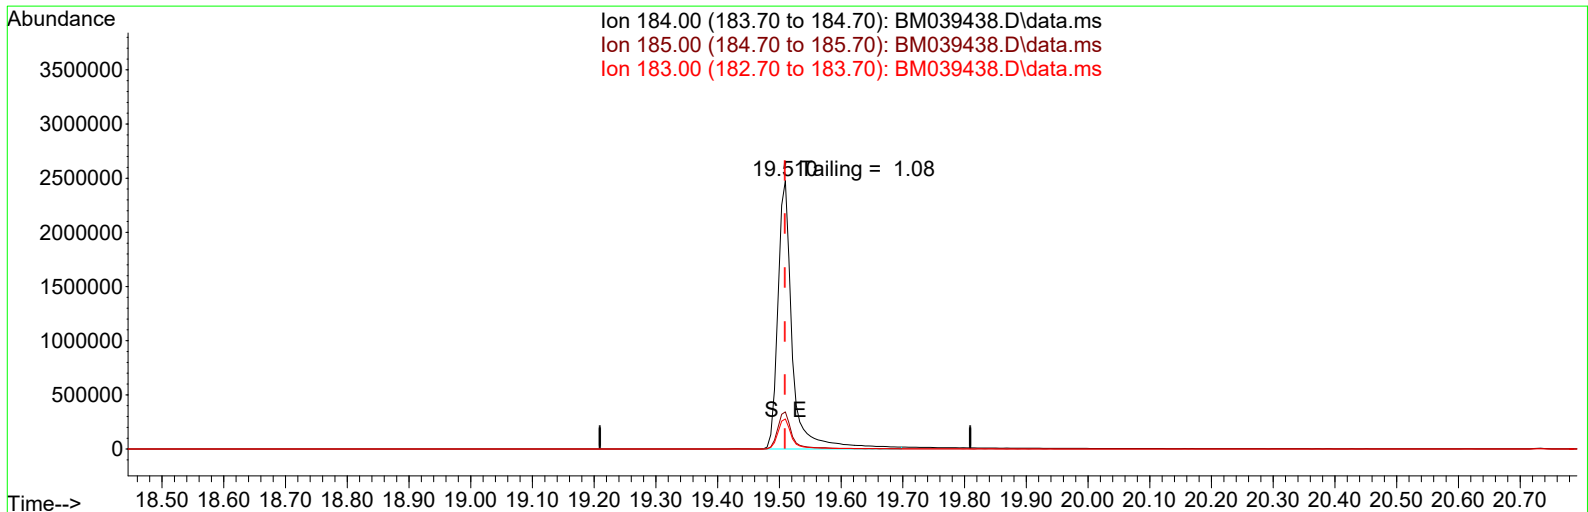

TIC: BM039438.D\data.ms

(77) Benzidine

19.510min (+ 0.000) 114950.11 ng

response 4141508

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.84
183.00	11.00	11.20
0.00	0.00	0.00