




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045356.D
Acq On : 18 Apr 2024 15:29
Operator : MA/JU
Sample : P2079-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/25/2024

Quant Time: Apr 18 16:00:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 12:42:01 2024
Response via : Initial Calibration

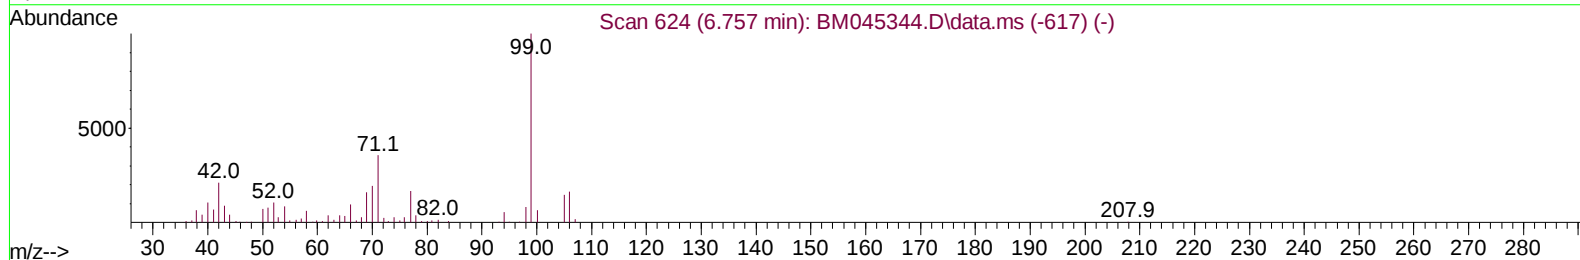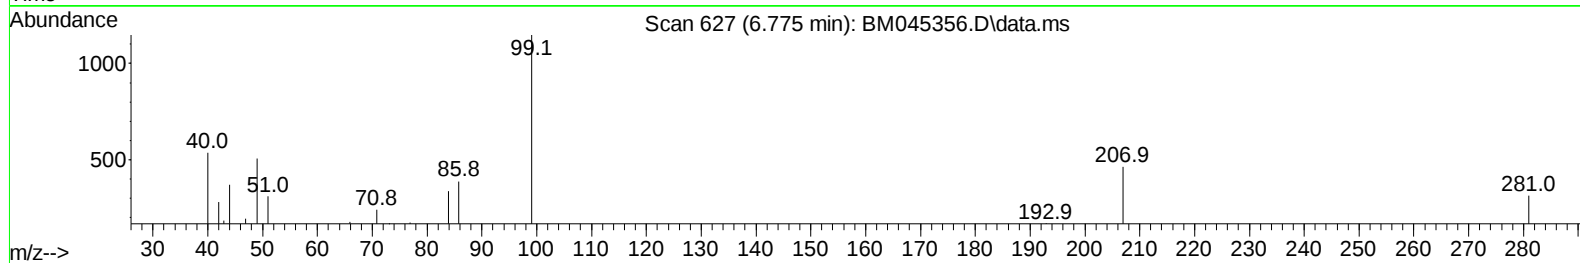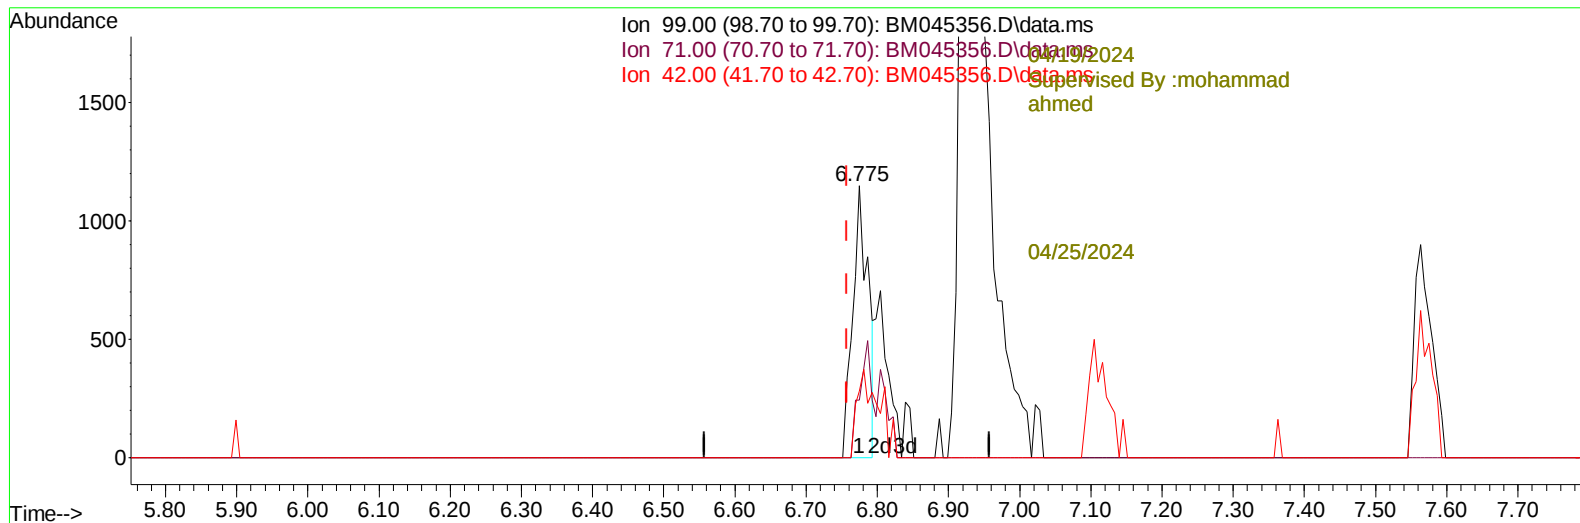

TIC: BM045356.D\data.ms

(7) Phenol-d5 (S)

6.775min (+ 0.018) 0.52 ng/u1

response 1737

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	32.50	20.99#
42.00	18.30	24.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045356.D
Acq On : 18 Apr 2024 15:29
Operator : MA/JU
Sample : P2079-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK6DL

Manual IntegrationsAPPROVED

Quant Time: Apr 18 16:00:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 12:42:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/25/2024

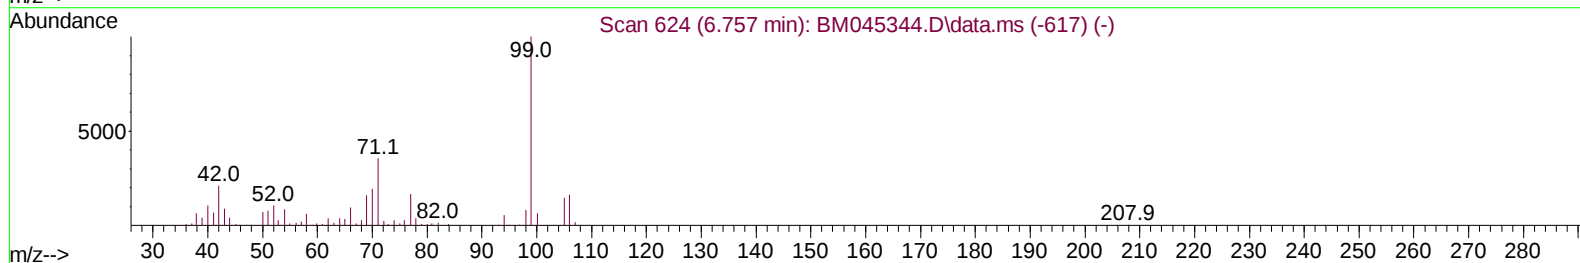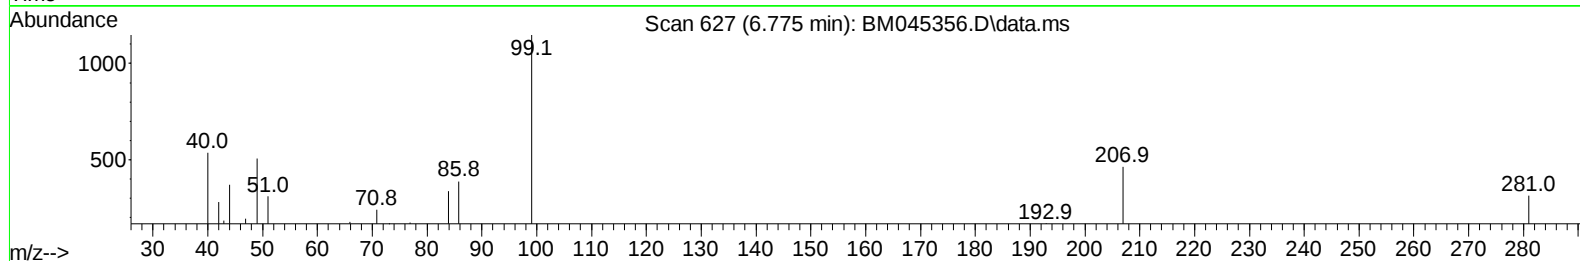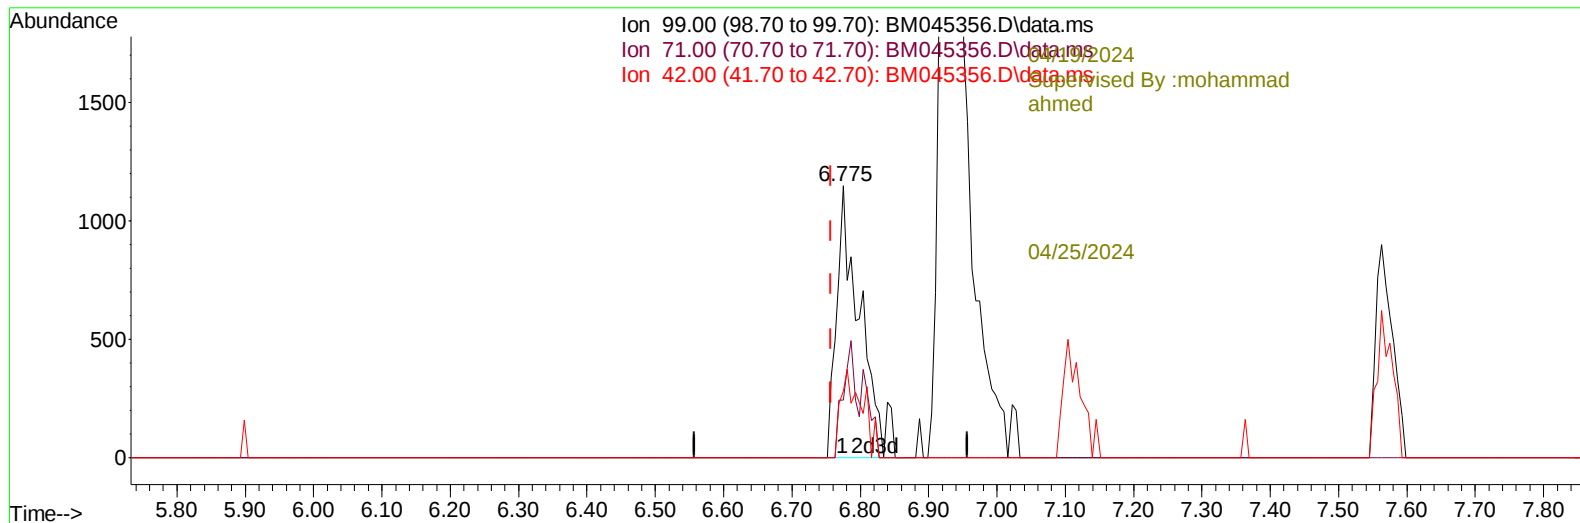

TIC: BM045356.D\data.ms

(7) Phenol-d5 (S)

6.775min (+ 0.018) 0.82 ng/ul m

response 2763

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	32.50	20.99#
42.00	18.30	24.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045356.D
Acq On : 18 Apr 2024 15:29
Operator : MA/JU
Sample : P2079-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK6DL

Manual IntegrationsAPPROVED

Quant Time: Apr 18 16:00:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 12:42:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/25/2024

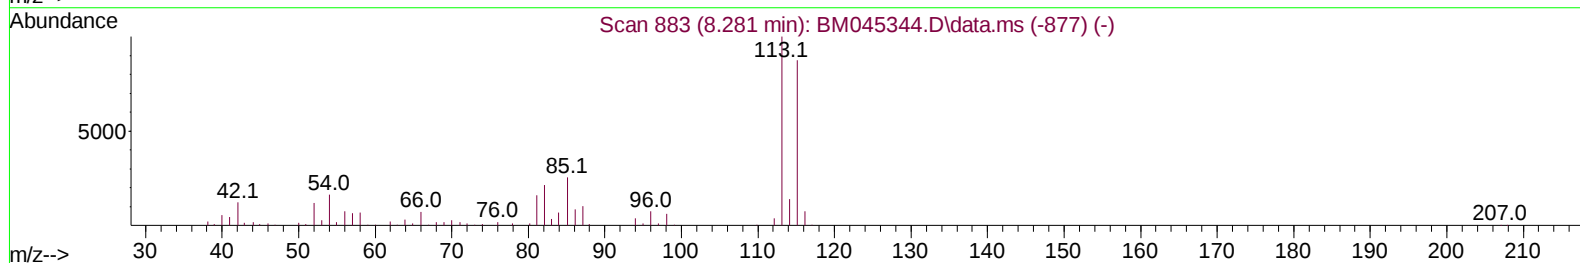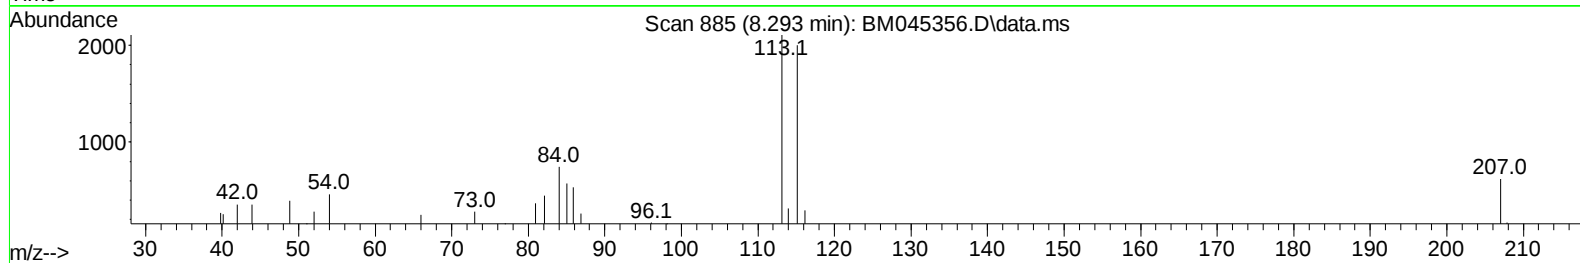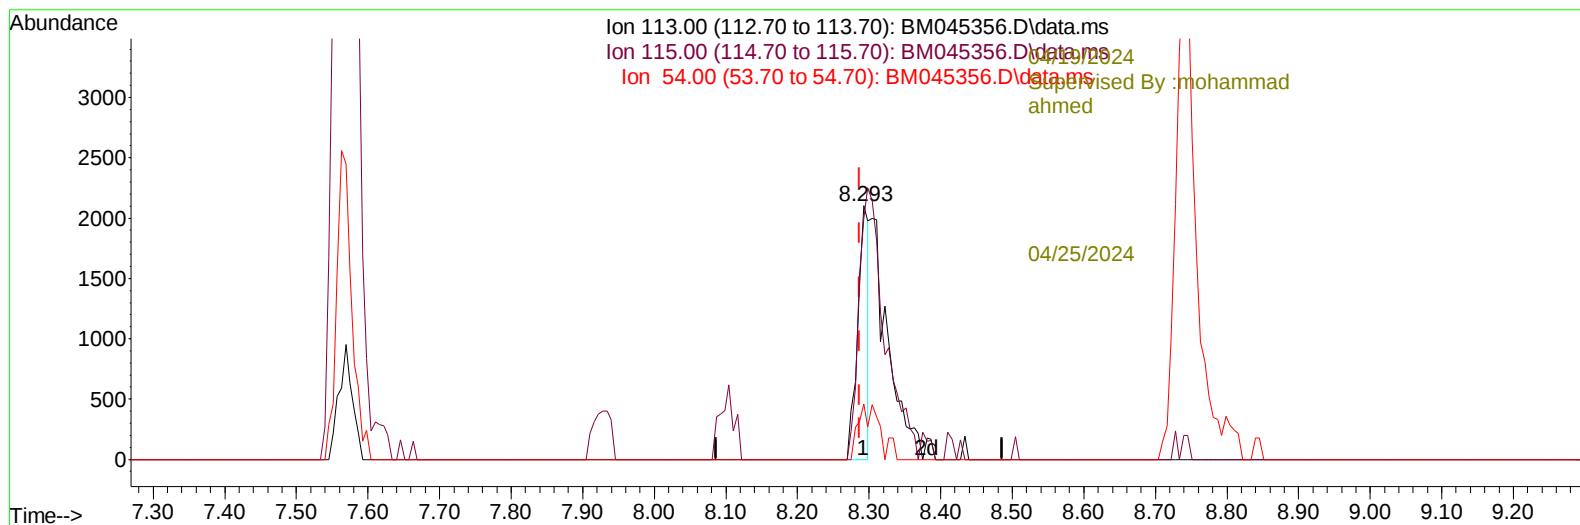

TIC: BM045356.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.293min (+ 0.006) 0.88 ng/u1

response 2312

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	91.20	94.92
54.00	13.00	21.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045356.D
Acq On : 18 Apr 2024 15:29
Operator : MA/JU
Sample : P2079-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK6DL

Manual IntegrationsAPPROVED

Quant Time: Apr 18 16:00:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 12:42:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/25/2024

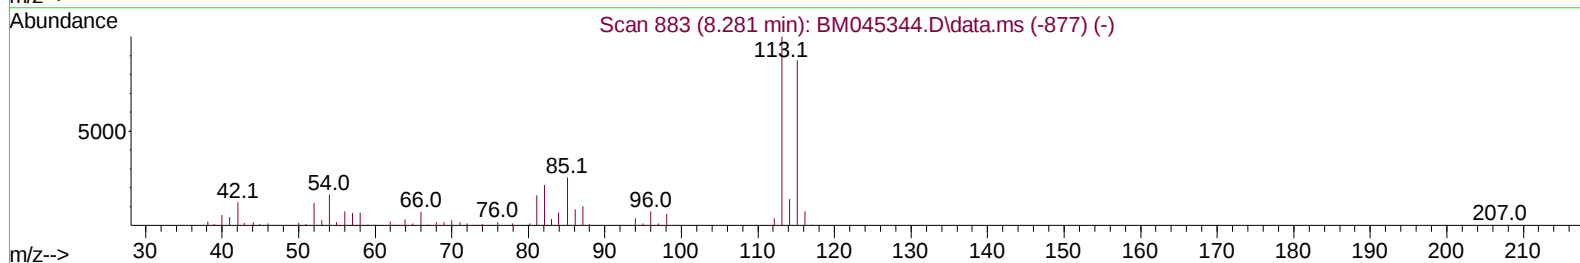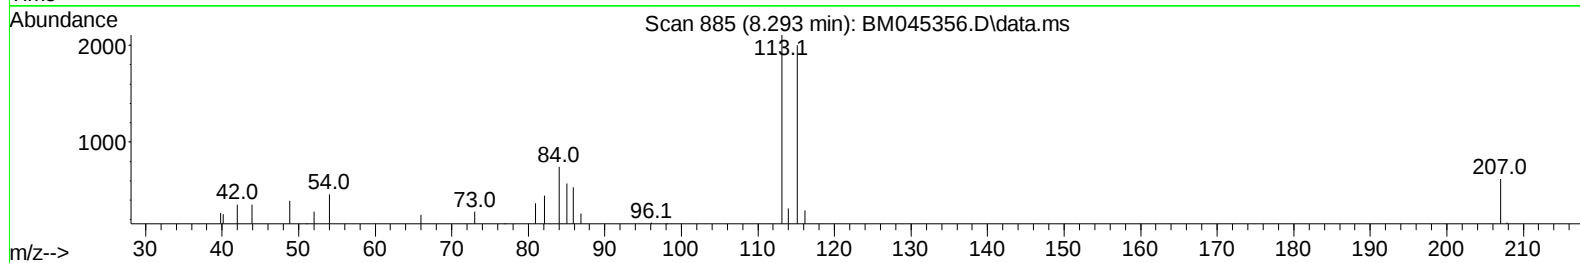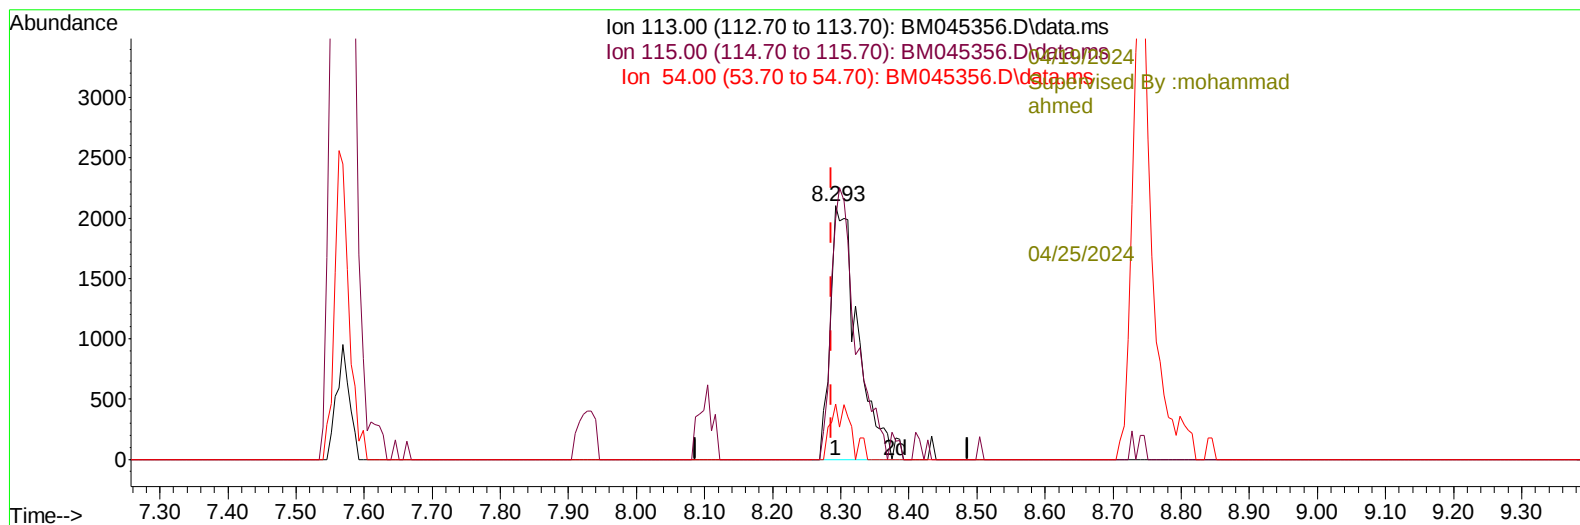

TIC: BM045356.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.293min (+ 0.006) 2.23 ng/u1 m

response 5900

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	91.20	94.92
54.00	13.00	21.84#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045356.D
 Acq On : 18 Apr 2024 15:29
 Operator : MA/JU
 Sample : P2079-01DL 5X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/25/2024

Quant Time: Apr 19 00:26:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 12:42:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/19/2024						
Supervised By :mohammad ahmed						
-----04/25/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	39783	20.000	ng/ul	0.00
20) Naphthalene-d8	10.339	136	165707	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.216	164	103064	20.000	ng/ul	-0.01
64) Phenanthrene-d10	16.980	188	218513	20.000	ng/ul	0.00
79) Chrysene-d12	21.198	240	234311	20.000	ng/ul	0.00
88) Perylene-d12	23.392	264	319766	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	1047	0.983	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.775	99	2763m	0.819	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.928	67	11138	5.543	ng/ul	0.00
11) 2-Chlorophenol-d4	7.110	132	10519	3.981	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	5900m	2.235	ng/ul	0.00
21) Nitrobenzene-d5	8.745	128	6203	4.873	ng/ul	0.00
24) 2-Nitrophenol-d4	9.451	143	5987	4.456	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.992	165	11165	4.533	ng/ul	0.02
31) 4-Chloroaniline-d4	10.534	131	11227	2.863	ng/ul	0.02
46) Dimethylphthalate-d6	13.651	166	50733	7.070	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	54409	6.418	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.221	176	45138	7.055	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.380	200	4958	3.827	ng/ul	0.00
73) Anthracene-d10	17.080	188	69109	7.031	ng/ul	0.00
81) Pyrene-d10	19.386	212	85061	7.373	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.250	264	104160	6.677	ng/ul	-0.01
Target Compounds						
						Qvalue
30) Naphthalene	10.387	128	21915	2.498	ng/ul	95
52) Acenaphthene	14.286	153	192930	29.201	ng/ul	98
61) Fluorene	15.280	166	60323	7.916	ng/ul	98
77) Carbazole	17.404	167	16543	1.426	ng/ul	96
80) Fluoranthene	19.051	202	32421	2.383	ng/ul	99
82) Pyrene	19.415	202	18183	1.238	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045356.D
Acq On : 18 Apr 2024 15:29
Operator : MA/JU
Sample : P2079-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK6DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:26:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 12:42:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/25/2024

