

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045312.D
Acq On : 17 Apr 2024 12:10
Operator : MA/JU
Sample : PB160236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BM045312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	9	11	12	rBV2	1987	1483	0.13%	0.013%
2	3.175	12	15	22	rVB	13827	19226	1.68%	0.168%
3	3.428	56	58	62	rBV5	2455	3307	0.29%	0.029%
4	3.505	69	71	73	rVB3	1900	1290	0.11%	0.011%
5	3.575	80	83	101	rBV	136614	261557	22.88%	2.285%
6	3.863	129	132	136	rBV5	4163	5311	0.46%	0.046%
7	3.893	136	137	140	rVB2	2422	1626	0.14%	0.014%
8	3.922	140	142	145	rBV4	1658	2341	0.20%	0.020%
9	4.393	221	222	225	rVB3	2045	1500	0.13%	0.013%
10	4.452	229	232	233	rBV3	1605	1251	0.11%	0.011%
11	4.528	242	245	246	rBV2	1616	1521	0.13%	0.013%
12	4.787	286	289	291	rBV3	1815	1470	0.13%	0.013%
13	4.928	310	313	315	rBV4	1138	1492	0.13%	0.013%
14	4.975	319	321	325	rVV4	1540	1362	0.12%	0.012%
15	5.187	355	357	360	rVV3	1382	1272	0.11%	0.011%
16	5.510	411	412	414	rBV2	1516	1326	0.12%	0.012%
17	5.710	442	446	448	rBV4	1565	2197	0.19%	0.019%
18	5.787	456	459	462	rVB4	1251	1539	0.13%	0.013%
19	5.816	462	464	467	rBV3	1350	1576	0.14%	0.014%
20	6.069	505	507	510	rVB4	1490	1430	0.13%	0.012%
21	6.128	514	517	520	rVB3	1424	1750	0.15%	0.015%
22	6.251	535	538	540	rVB4	1530	1552	0.14%	0.014%
23	6.281	540	543	547	rBV6	1935	2218	0.19%	0.019%
24	6.587	593	595	599	rVV4	1771	1506	0.13%	0.013%
25	6.628	599	602	605	rVB4	1675	2021	0.18%	0.018%
26	6.757	618	624	637	rBV	183384	334683	29.27%	2.924%
27	6.934	648	654	669	rBV	168862	271527	23.75%	2.372%
28	7.110	677	684	697	rBV	206870	356134	31.15%	3.112%
29	7.357	724	726	730	rVB5	1253	1645	0.14%	0.014%
30	7.410	730	735	736	rBV3	1429	1725	0.15%	0.015%
31	7.575	756	763	775	rBV	194454	318457	27.86%	2.782%
32	7.881	813	815	818	rVB2	1547	1324	0.12%	0.012%
33	7.910	818	820	823	rBV3	1456	1561	0.14%	0.014%
34	8.069	843	847	850	rVB4	1093	1637	0.14%	0.014%
35	8.287	878	884	899	rBV	223545	398157	34.83%	3.479%
36	8.451	909	912	913	rVB3	2039	1233	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045312.D
Acq On : 17 Apr 2024 12:10
Operator : MA/JU
Sample : PB160236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	8.475	913	916	918	rVV2	1244	1212	0.11%	0.011%
38	8.551	926	929	930	rBV2	1335	1401	0.12%	0.012%
39	8.645	943	945	950	rVB4	1208	1985	0.17%	0.017%
40	8.739	954	961	968	rBV	178622	313745	27.44%	2.741%
41	9.122	1024	1026	1028	rVV3	1161	1437	0.13%	0.013%
42	9.186	1036	1037	1040	rVB3	1575	1349	0.12%	0.012%
43	9.222	1040	1043	1044	rBV3	1406	1208	0.11%	0.011%
44	9.257	1047	1049	1052	rVB3	1645	1496	0.13%	0.013%
45	9.451	1074	1082	1093	rBV	152003	269069	23.54%	2.351%
46	9.557	1097	1100	1103	rBV3	875	1221	0.11%	0.011%
47	9.981	1166	1172	1180	rBV	193969	354094	30.97%	3.094%
48	10.345	1225	1234	1242	rBV	246233	412771	36.11%	3.607%
49	10.510	1254	1262	1281	rBV	151902	387726	33.91%	3.388%
50	10.698	1292	1294	1297	rVB3	1122	1350	0.12%	0.012%
51	10.810	1310	1313	1317	rBV5	1184	2177	0.19%	0.019%
52	11.051	1351	1354	1358	rVB3	1369	1692	0.15%	0.015%
53	11.116	1361	1365	1366	rVV4	1148	1270	0.11%	0.011%
54	11.163	1366	1373	1376	rVB4	736	1309	0.11%	0.011%
55	11.339	1401	1403	1405	rVB3	1236	1251	0.11%	0.011%
56	11.386	1407	1411	1414	rVB4	917	1307	0.11%	0.011%
57	11.880	1493	1495	1500	rVB4	1443	1758	0.15%	0.015%
58	11.986	1508	1513	1519	rBV4	2158	5286	0.46%	0.046%
59	12.304	1562	1567	1568	rBV3	997	1559	0.14%	0.014%
60	12.763	1641	1645	1647	rBV3	1275	1483	0.13%	0.013%
61	13.110	1700	1704	1705	rBV3	1532	1570	0.14%	0.014%
62	13.169	1712	1714	1718	rVB4	1202	1382	0.12%	0.012%
63	13.657	1791	1797	1808	rBV	354346	527542	46.14%	4.609%
64	13.916	1832	1841	1852	rBV2	454927	671047	58.70%	5.863%
65	13.998	1852	1855	1858	rVB4	1487	1205	0.11%	0.011%
66	14.227	1887	1894	1902	rVV	348497	501684	43.88%	4.383%
67	14.474	1931	1936	1954	rBV2	54818	174066	15.23%	1.521%
68	14.680	1969	1971	1975	rVB3	1834	1747	0.15%	0.015%
69	14.910	2008	2010	2014	rVB4	1002	1276	0.11%	0.011%
70	15.233	2058	2065	2073	rBV	528079	807795	70.66%	7.058%
71	15.380	2085	2090	2101	rBV	113610	188279	16.47%	1.645%
72	16.021	2193	2199	2203	rBV5	2063	2718	0.24%	0.024%
73	16.986	2357	2363	2369	rBV	412511	542274	47.43%	4.738%
74	17.086	2374	2380	2397	rVV	549535	837414	73.25%	7.317%
75	17.433	2434	2439	2441	rVV4	955	1343	0.12%	0.012%
76	17.480	2443	2447	2449	rVV3	1006	1357	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045312.D
 Acq On : 17 Apr 2024 12:10
 Operator : MA/JU
 Sample : PB160236BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.521	2452	2454	2458	rBV3	1306	1660	0.15%	0.015%
78	17.621	2467	2471	2473	rVB3	1603	2034	0.18%	0.018%
79	17.645	2473	2475	2477	rBV2	1233	1238	0.11%	0.011%
80	17.745	2490	2492	2495	rVB2	1614	1292	0.11%	0.011%
81	17.921	2520	2522	2525	rVB2	1606	1524	0.13%	0.013%
82	17.962	2527	2529	2531	rVB2	1368	1237	0.11%	0.011%
83	18.151	2554	2561	2562	rBV6	1675	2802	0.25%	0.024%
84	18.227	2569	2574	2575	rBV5	1133	1733	0.15%	0.015%
85	18.292	2583	2585	2587	rBV2	1290	1477	0.13%	0.013%
86	18.404	2602	2604	2607	rBV4	1121	1550	0.14%	0.014%
87	18.509	2618	2622	2624	rBV4	1261	1389	0.12%	0.012%
88	18.762	2663	2665	2668	rBV3	1072	1523	0.13%	0.013%
89	18.827	2673	2676	2680	rBV5	1202	2152	0.19%	0.019%
90	18.874	2681	2684	2686	rBV3	878	1203	0.11%	0.011%
91	18.915	2689	2691	2694	rBV4	1029	1247	0.11%	0.011%
92	18.956	2695	2698	2703	rVV5	4190	5425	0.47%	0.047%
93	19.039	2707	2712	2714	rBV5	4579	6818	0.60%	0.060%
94	19.398	2767	2773	2788	rBV	607468	915987	80.12%	8.003%
95	19.786	2837	2839	2840	rBV2	2269	1258	0.11%	0.011%
96	19.933	2862	2864	2868	rBV5	1888	2021	0.18%	0.018%
97	20.074	2886	2888	2890	rBV2	2344	1786	0.16%	0.016%
98	21.203	3075	3080	3089	rBV	394410	581783	50.89%	5.083%
99	23.256	3423	3429	3438	rBV	627278	1143240	100.00%	9.989%
100	23.397	3447	3453	3467	rBV	358344	719556	62.94%	6.287%

Sum of corrected areas: 11444997




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045312.D
Acq On : 17 Apr 2024 12:10
Operator : MA/JU
Sample : PB160236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

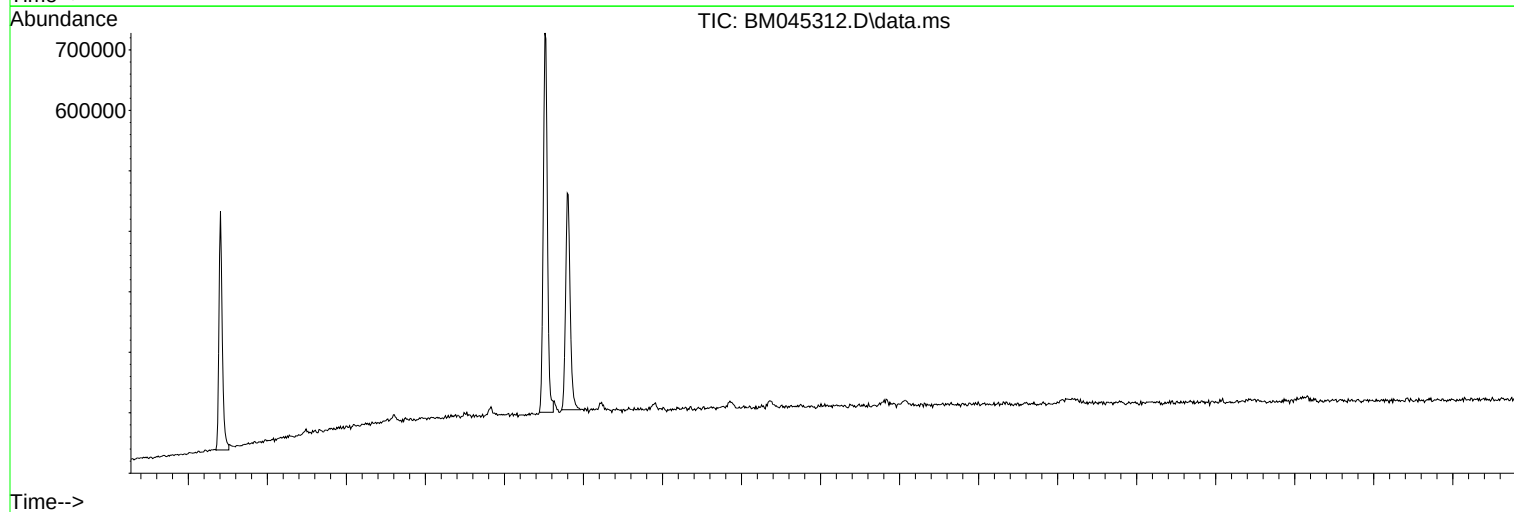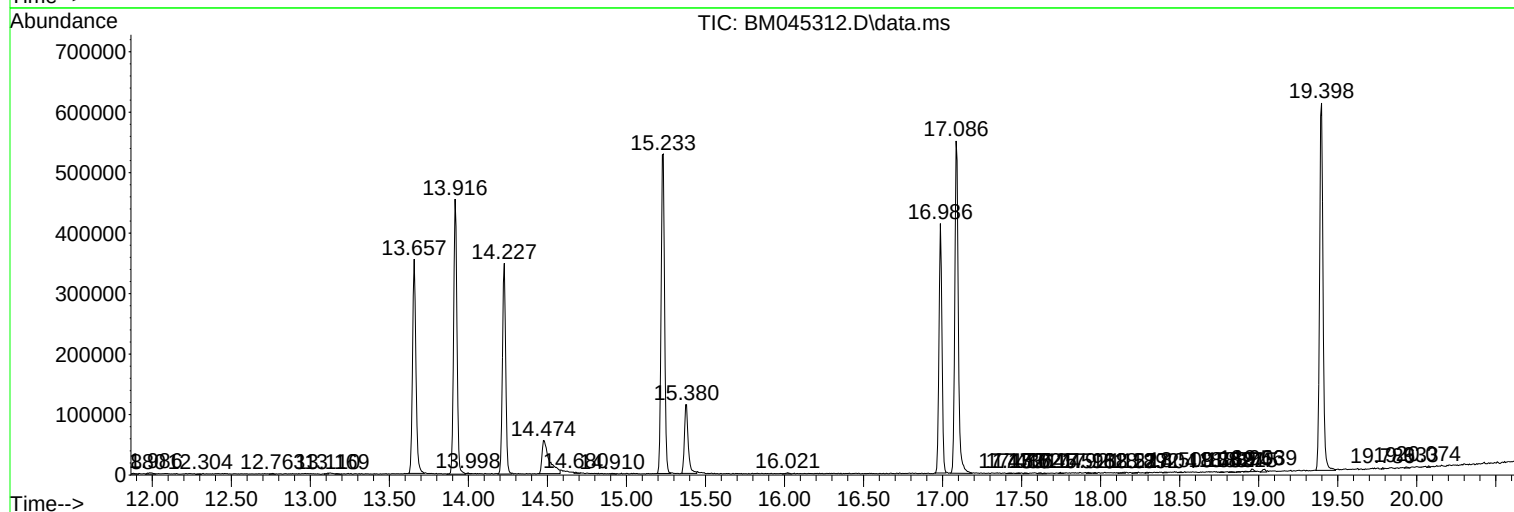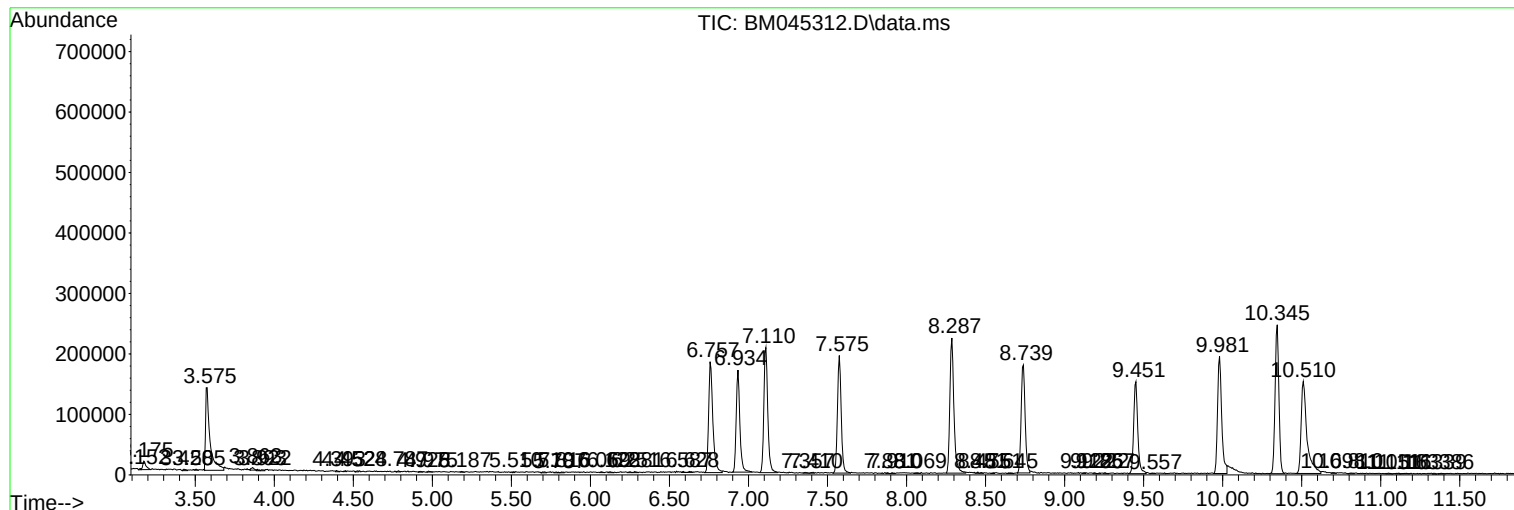

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045312.D
Acq On : 17 Apr 2024 12:10
Operator : MA/JU
Sample : PB160236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045312.D
Acq On : 17 Apr 2024 12:10
Operator : MA/JU
Sample : PB160236BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK236

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
