

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045313.D
 Acq On : 17 Apr 2024 12:46
 Operator : MA/JU
 Sample : PB160233BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	22	rVB2	12909	19732	1.68%	0.159%
2	3.222	22	23	27	rVB4	1623	1452	0.12%	0.012%
3	3.446	60	61	64	rVB3	2463	1498	0.13%	0.012%
4	3.569	79	82	97	rBV	138278	255887	21.75%	2.068%
5	3.858	126	131	135	rBV5	3528	5942	0.51%	0.048%
6	3.946	145	146	148	rBV2	2104	1503	0.13%	0.012%
7	4.240	195	196	200	rBV2	1304	1538	0.13%	0.012%
8	4.305	203	207	208	rBV3	1531	1463	0.12%	0.012%
9	4.369	215	218	221	rVB5	1721	1732	0.15%	0.014%
10	4.405	221	224	226	rBV3	1522	1817	0.15%	0.015%
11	4.557	247	250	253	rBV4	1679	2406	0.20%	0.019%
12	4.587	253	255	258	rBV3	1905	2257	0.19%	0.018%
13	4.669	267	269	272	rVB2	1512	1526	0.13%	0.012%
14	4.810	290	293	294	rBV2	1309	1446	0.12%	0.012%
15	5.046	331	333	335	rBV2	1520	1430	0.12%	0.012%
16	5.269	369	371	374	rVB3	1642	1262	0.11%	0.010%
17	5.316	376	379	381	rBV4	943	1225	0.10%	0.010%
18	5.416	393	396	399	rVB4	1189	1415	0.12%	0.011%
19	5.640	432	434	436	rBV3	1419	1461	0.12%	0.012%
20	5.716	444	447	450	rBV3	1108	1284	0.11%	0.010%
21	5.852	468	470	473	rVB3	1267	1507	0.13%	0.012%
22	5.893	475	477	480	rVB3	2048	1789	0.15%	0.014%
23	5.922	480	482	485	rBV3	2015	2251	0.19%	0.018%
24	6.240	532	536	537	rBV4	1241	1432	0.12%	0.012%
25	6.640	600	604	607	rBV5	833	1449	0.12%	0.012%
26	6.669	607	609	613	rVB4	1312	1677	0.14%	0.014%
27	6.757	618	624	634	rBV	178212	327965	27.88%	2.650%
28	6.934	648	654	665	rBV	167982	272336	23.15%	2.201%
29	7.046	670	673	676	rVV4	1495	2045	0.17%	0.017%
30	7.110	678	684	694	rVV	215570	356033	30.27%	2.877%
31	7.198	698	699	703	rVV2	1497	1391	0.12%	0.011%
32	7.428	736	738	741	rBV4	1690	1351	0.11%	0.011%
33	7.575	757	763	775	rVV	242556	396563	33.71%	3.204%
34	7.687	779	782	784	rVB3	1519	1387	0.12%	0.011%
35	7.963	826	829	832	rVB4	997	1537	0.13%	0.012%
36	7.993	832	834	836	rBV3	1222	1304	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045313.D
Acq On : 17 Apr 2024 12:46
Operator : MA/JU
Sample : PB160233BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	8.110	850	854	855	rBV2	1008	1260	0.11%	0.010%
38	8.287	877	884	899	rBV	217706	398179	33.85%	3.218%
39	8.740	954	961	970	rBV	177482	314036	26.70%	2.538%
40	9.340	1061	1063	1067	rVB3	896	1329	0.11%	0.011%

41	9.398	1070	1073	1074	rBV2	1329	1188	0.10%	0.010%
42	9.451	1074	1082	1092	rVV	148722	261028	22.19%	2.109%
43	9.516	1092	1093	1095	rVV2	1912	1452	0.12%	0.012%
44	9.687	1121	1122	1125	rBV	1675	1592	0.14%	0.013%
45	9.763	1133	1135	1139	rVB3	1655	1933	0.16%	0.016%

46	9.981	1165	1172	1183	rBV	198384	363004	30.86%	2.933%
47	10.128	1195	1197	1199	rVB2	1996	2029	0.17%	0.016%
48	10.345	1227	1234	1247	rBV	311881	516469	43.91%	4.173%
49	10.434	1247	1249	1252	rVB3	1608	1439	0.12%	0.012%
50	10.510	1255	1262	1286	rBV	154902	391183	33.26%	3.161%

51	10.916	1328	1331	1334	rVV3	1067	1670	0.14%	0.013%
52	10.963	1334	1339	1344	rVB4	989	2101	0.18%	0.017%
53	11.234	1382	1385	1388	rBV3	939	1305	0.11%	0.011%
54	11.992	1508	1514	1518	rBV5	1792	3729	0.32%	0.030%
55	12.369	1573	1578	1581	rBV4	689	1436	0.12%	0.012%

56	13.133	1702	1708	1712	rBV5	2010	4165	0.35%	0.034%
57	13.169	1712	1714	1717	rVB3	1277	1499	0.13%	0.012%
58	13.416	1752	1756	1757	rBV2	1398	1604	0.14%	0.013%
59	13.604	1785	1788	1791	rBV4	1463	1553	0.13%	0.013%
60	13.657	1791	1797	1808	rVV	349340	519240	44.14%	4.196%

61	13.916	1835	1841	1852	rBV2	443978	653934	55.60%	5.284%
62	14.227	1887	1894	1902	rBV	438135	628895	53.47%	5.082%
63	14.398	1916	1923	1926	rBV3	1270	2769	0.24%	0.022%
64	14.474	1929	1936	1952	rBV2	58928	180622	15.36%	1.460%
65	14.651	1964	1966	1969	rVB4	1762	2102	0.18%	0.017%

66	14.686	1969	1972	1976	rVB3	1426	1504	0.13%	0.012%
67	15.227	2058	2064	2076	rBV	535910	801018	68.10%	6.473%
68	15.380	2083	2090	2099	rBV	116088	191874	16.31%	1.550%
69	15.474	2104	2106	2109	rVV3	2115	2532	0.22%	0.020%
70	15.957	2187	2188	2193	rBV2	869	1208	0.10%	0.010%

71	16.021	2193	2199	2203	rVV5	1390	1661	0.14%	0.013%
72	16.774	2325	2327	2330	rBV3	1184	1218	0.10%	0.010%
73	16.898	2345	2348	2351	rVB4	1051	1310	0.11%	0.011%
74	16.986	2357	2363	2371	rVV	516068	705552	59.98%	5.701%
75	17.086	2374	2380	2393	rVV2	545746	837340	71.19%	6.766%

76	17.198	2396	2399	2403	rVB4	970	1178	0.10%	0.010%
----	--------	------	------	------	------	-----	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045313.D
 Acq On : 17 Apr 2024 12:46
 Operator : MA/JU
 Sample : PB160233BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.415	2432	2436	2439	rBV3	614	1205	0.10%	0.010%
78	17.715	2485	2487	2489	rBV2	1262	1247	0.11%	0.010%
79	18.151	2559	2561	2564	rBV3	1096	1341	0.11%	0.011%
80	18.327	2587	2591	2592	rBV2	1715	2113	0.18%	0.017%
81	18.586	2632	2635	2636	rBV2	1987	1453	0.12%	0.012%
82	18.639	2641	2644	2647	rBV4	1153	1640	0.14%	0.013%
83	18.810	2671	2673	2677	rBV2	1301	1618	0.14%	0.013%
84	18.957	2695	2698	2704	rVB5	5148	7542	0.64%	0.061%
85	19.033	2707	2711	2714	rBV3	3557	4352	0.37%	0.035%
86	19.174	2732	2735	2738	rBV4	1755	2364	0.20%	0.019%
87	19.245	2746	2747	2750	rBV3	1418	1271	0.11%	0.010%
88	19.398	2767	2773	2784	rBV	657823	941519	80.04%	7.608%
89	19.568	2800	2802	2803	rBV2	1258	1181	0.10%	0.010%
90	20.151	2899	2901	2902	rBV2	2222	1185	0.10%	0.010%
91	20.745	3000	3002	3003	rBV2	3985	2573	0.22%	0.021%
92	21.203	3075	3080	3090	rBV	527407	758926	64.52%	6.133%
93	23.262	3423	3430	3436	rBV	669017	1176241	100.00%	9.505%
94	23.403	3447	3454	3464	rBV	507125	978211	83.16%	7.904%



Sum of corrected areas: 12375415

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045313.D
Acq On : 17 Apr 2024 12:46
Operator : MA/JU
Sample : PB160233BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

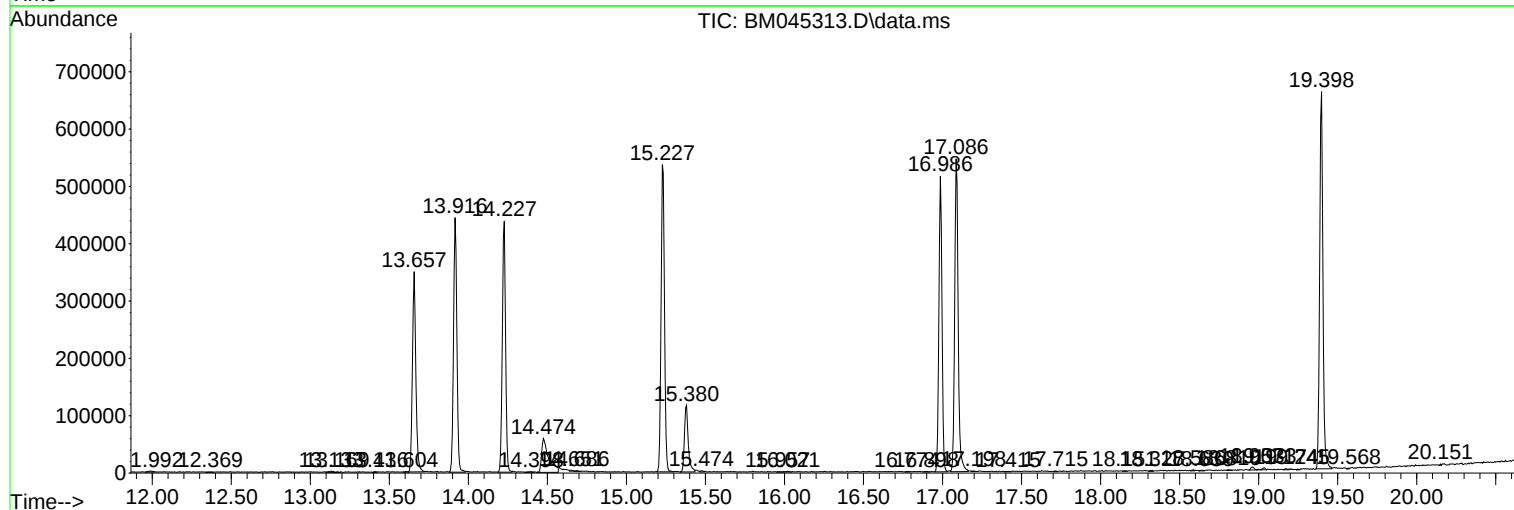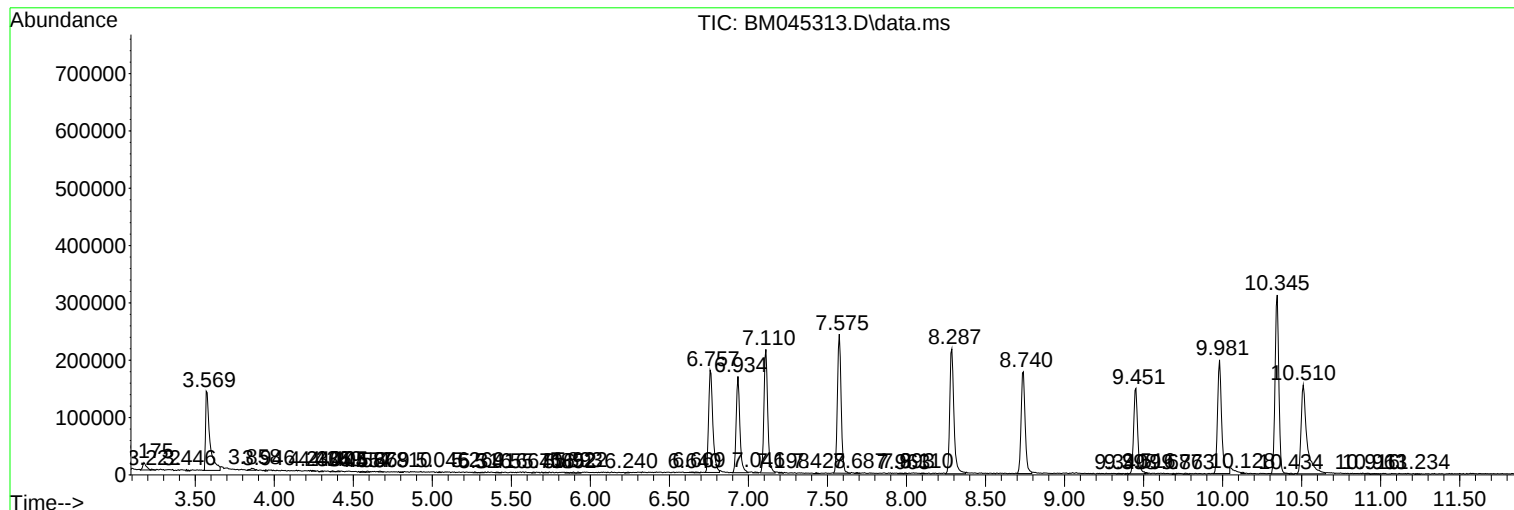

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045313.D
Acq On : 17 Apr 2024 12:46
Operator : MA/JU
Sample : PB160233BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045313.D
Acq On : 17 Apr 2024 12:46
Operator : MA/JU
Sample : PB160233BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
