

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045314.D
 Acq On : 17 Apr 2024 13:23
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	24	rVB	13926	19478	1.77%	0.180%
2	3.287	32	34	37	rBV2	1421	1750	0.16%	0.016%
3	3.475	64	66	67	rBV2	1835	1346	0.12%	0.012%
4	3.546	75	78	80	rBV2	1856	2380	0.22%	0.022%
5	3.569	80	82	108	rVV	134412	267571	24.32%	2.471%
6	3.763	113	115	116	rVV2	3420	2230	0.20%	0.021%
7	3.781	116	118	120	rVV3	2140	2605	0.24%	0.024%
8	3.863	129	132	135	rVV5	4334	4714	0.43%	0.044%
9	3.999	153	155	157	rVB3	1957	1118	0.10%	0.010%
10	4.616	258	260	263	rVB4	1531	1440	0.13%	0.013%
11	4.687	271	272	275	rVB3	2337	1448	0.13%	0.013%
12	4.716	275	277	278	rBV2	1536	1160	0.11%	0.011%
13	4.916	309	311	314	rVB5	1529	1355	0.12%	0.013%
14	4.940	314	315	317	rBV2	2236	1439	0.13%	0.013%
15	4.969	317	320	321	rVV3	1445	1237	0.11%	0.011%
16	5.051	331	334	337	rBV5	1367	1836	0.17%	0.017%
17	5.110	343	344	347	rBV3	1208	1147	0.10%	0.011%
18	5.163	350	353	356	rBV4	1020	1394	0.13%	0.013%
19	5.275	370	372	374	rVB3	1855	1421	0.13%	0.013%
20	5.457	400	403	406	rBV4	1379	1837	0.17%	0.017%
21	5.646	432	435	438	rVB5	1611	1791	0.16%	0.017%
22	5.669	438	439	442	rBV3	1485	1717	0.16%	0.016%
23	5.869	470	473	474	rBV3	1015	1185	0.11%	0.011%
24	6.287	543	544	546	rBV2	1546	1439	0.13%	0.013%
25	6.345	551	554	556	rBV4	1524	1891	0.17%	0.017%
26	6.704	612	615	616	rVB2	1600	1481	0.13%	0.014%
27	6.763	617	625	636	rBV	174223	325946	29.63%	3.011%
28	6.934	648	654	663	rBV	162172	260198	23.65%	2.403%
29	7.110	678	684	694	rBV	210515	343297	31.21%	3.171%
30	7.245	706	707	713	rVB4	1648	2094	0.19%	0.019%
31	7.575	756	763	773	rVV	188705	310875	28.26%	2.871%
32	7.881	811	815	818	rBV4	881	1248	0.11%	0.012%
33	7.963	827	829	832	rBV3	1501	1567	0.14%	0.014%
34	8.039	839	842	845	rVB3	1211	1679	0.15%	0.016%
35	8.287	878	884	896	rBV	214895	379252	34.48%	3.503%
36	8.592	932	936	938	rBV3	1409	1529	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045314.D
 Acq On : 17 Apr 2024 13:23
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	8.657	944	947	948	rBV3	1416	1114	0.10%	0.010%
38	8.739	951	961	969	rBV	169397	304693	27.70%	2.814%
39	8.804	971	972	974	rVB2	2373	1218	0.11%	0.011%
40	9.057	1013	1015	1018	rVV2	904	1239	0.11%	0.011%
41	9.451	1076	1082	1095	rBV	141575	256284	23.30%	2.367%
42	9.539	1095	1097	1100	rVB2	1703	1610	0.15%	0.015%
43	9.686	1119	1122	1126	rVB3	1132	1434	0.13%	0.013%
44	9.857	1149	1151	1155	rVB2	1245	1158	0.11%	0.011%
45	9.981	1166	1172	1192	rBV	184759	366267	33.30%	3.383%
46	10.345	1227	1234	1242	rBV	240599	387467	35.22%	3.579%
47	10.510	1254	1262	1285	rBV	146854	372390	33.85%	3.440%
48	11.075	1357	1358	1362	rVB3	1132	1205	0.11%	0.011%
49	11.427	1414	1418	1420	rVB3	846	1169	0.11%	0.011%
50	11.710	1465	1466	1469	rVB	1515	1322	0.12%	0.012%
51	11.775	1474	1477	1480	rBV3	1261	1801	0.16%	0.017%
52	11.880	1490	1495	1498	rVB	1334	1815	0.17%	0.017%
53	11.986	1508	1513	1520	rVB4	2226	4265	0.39%	0.039%
54	12.222	1549	1553	1555	rVB2	1372	1786	0.16%	0.016%
55	12.339	1569	1573	1575	rBV2	1055	1305	0.12%	0.012%
56	12.569	1609	1612	1616	rBV3	1445	1707	0.16%	0.016%
57	12.969	1677	1680	1684	rVV2	790	1414	0.13%	0.013%
58	13.127	1703	1707	1714	rVB4	2456	4763	0.43%	0.044%
59	13.298	1734	1736	1741	rVB4	1083	1303	0.12%	0.012%
60	13.657	1791	1797	1809	rBV	320613	482995	43.91%	4.461%
61	13.851	1827	1830	1835	rBV3	1177	1680	0.15%	0.016%
62	13.916	1835	1841	1852	rBV2	422936	622978	56.63%	5.754%
63	14.227	1886	1894	1903	rBV	315570	463853	42.17%	4.284%
64	14.480	1931	1937	1954	rBV2	48612	157771	14.34%	1.457%
65	14.698	1971	1974	1976	rVB3	1668	2020	0.18%	0.019%
66	14.721	1976	1978	1982	rBV2	1410	1840	0.17%	0.017%
67	15.080	2037	2039	2042	rVB3	1166	1134	0.10%	0.010%
68	15.233	2058	2065	2078	rBV	487904	743902	67.63%	6.871%
69	15.374	2084	2089	2104	rBV	100178	175168	15.92%	1.618%
70	15.474	2104	2106	2110	rVV3	2752	3382	0.31%	0.031%
71	15.639	2129	2134	2135	rBV2	1218	1569	0.14%	0.014%
72	15.774	2152	2157	2159	rVB3	1146	1478	0.13%	0.014%
73	15.898	2174	2178	2180	rBV3	1012	1417	0.13%	0.013%
74	16.027	2195	2200	2202	rVB4	1294	1436	0.13%	0.013%
75	16.068	2204	2207	2211	rBV2	1222	1482	0.13%	0.014%
76	16.651	2301	2306	2309	rBV4	890	1799	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045314.D
 Acq On : 17 Apr 2024 13:23
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	16.786	2325	2329	2331	rVB2	1216	1232	0.11%	0.011%
78	16.874	2341	2344	2348	rBV3	1044	1438	0.13%	0.013%
79	16.986	2356	2363	2374	rBV	350357	499580	45.42%	4.614%
80	17.086	2374	2380	2399	rVV	497658	759346	69.03%	7.014%
81	17.245	2403	2407	2410	rVB6	1018	1323	0.12%	0.012%
82	17.598	2463	2467	2469	rBV4	1035	1315	0.12%	0.012%
83	17.627	2469	2472	2474	rVV4	1566	1353	0.12%	0.012%
84	17.645	2474	2475	2480	rVB3	1508	1855	0.17%	0.017%
85	17.733	2489	2490	2493	rVV3	1531	1129	0.10%	0.010%
86	17.874	2510	2514	2516	rVB4	1491	1703	0.15%	0.016%
87	17.892	2516	2517	2519	rBV	1407	1231	0.11%	0.011%
88	18.204	2566	2570	2571	rBV2	1300	1618	0.15%	0.015%
89	18.333	2590	2592	2596	rBV3	1260	1590	0.14%	0.015%
90	18.745	2659	2662	2665	rVB4	933	1246	0.11%	0.012%
91	18.962	2696	2699	2701	rBV3	4279	5567	0.51%	0.051%
92	19.039	2708	2712	2715	rBV3	4330	5038	0.46%	0.047%
93	19.351	2761	2765	2766	rBV4	1631	1731	0.16%	0.016%
94	19.398	2767	2773	2786	rVV	571446	845668	76.88%	7.811%
95	19.533	2794	2796	2797	rBV2	1818	1161	0.11%	0.011%
96	20.098	2890	2892	2897	rBV4	3124	2892	0.26%	0.027%
97	20.474	2954	2956	2958	rBV3	2834	2986	0.27%	0.028%
98	21.203	3075	3080	3093	rBV	356398	548956	49.91%	5.070%
99	23.256	3423	3429	3445	rBV2	598933	1099994	100.00%	10.160%
100	23.397	3447	3453	3465	rVB	340682	695874	63.26%	6.427%




Sum of corrected areas: 10826554

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045314.D
Acq On : 17 Apr 2024 13:23
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

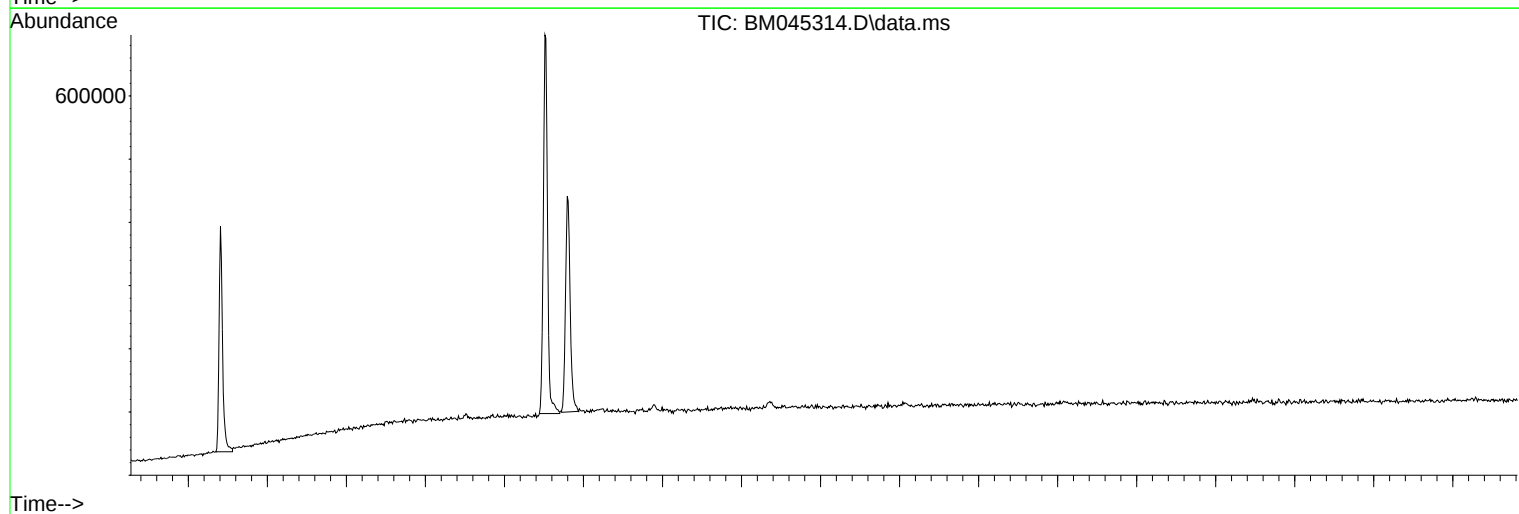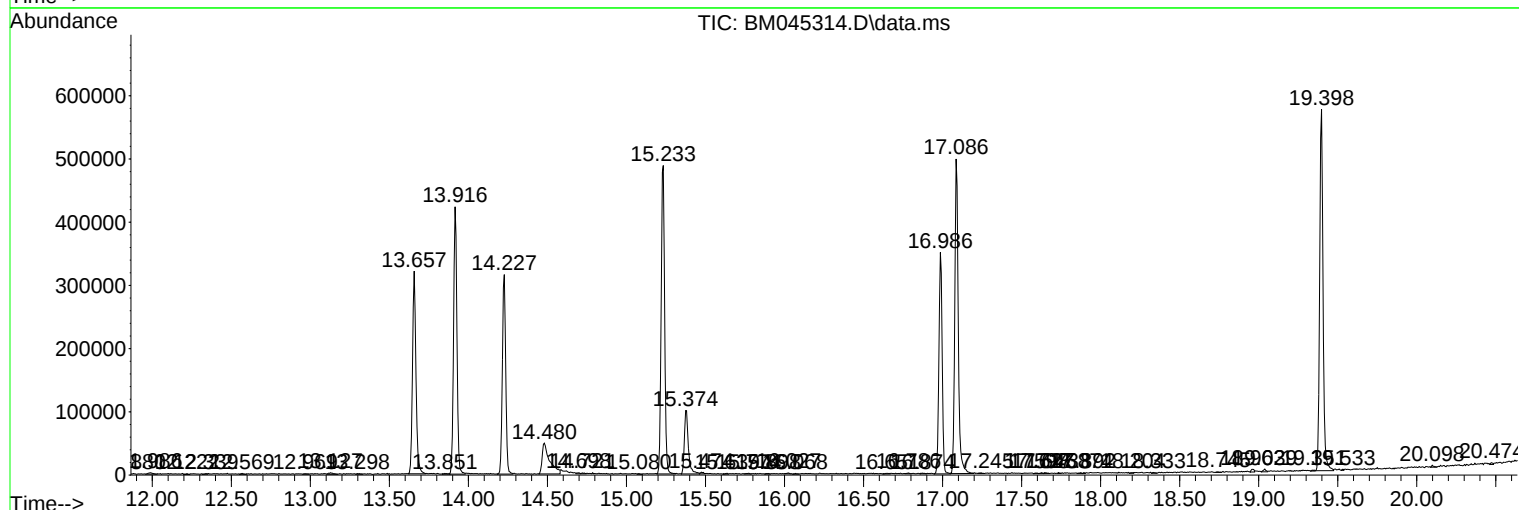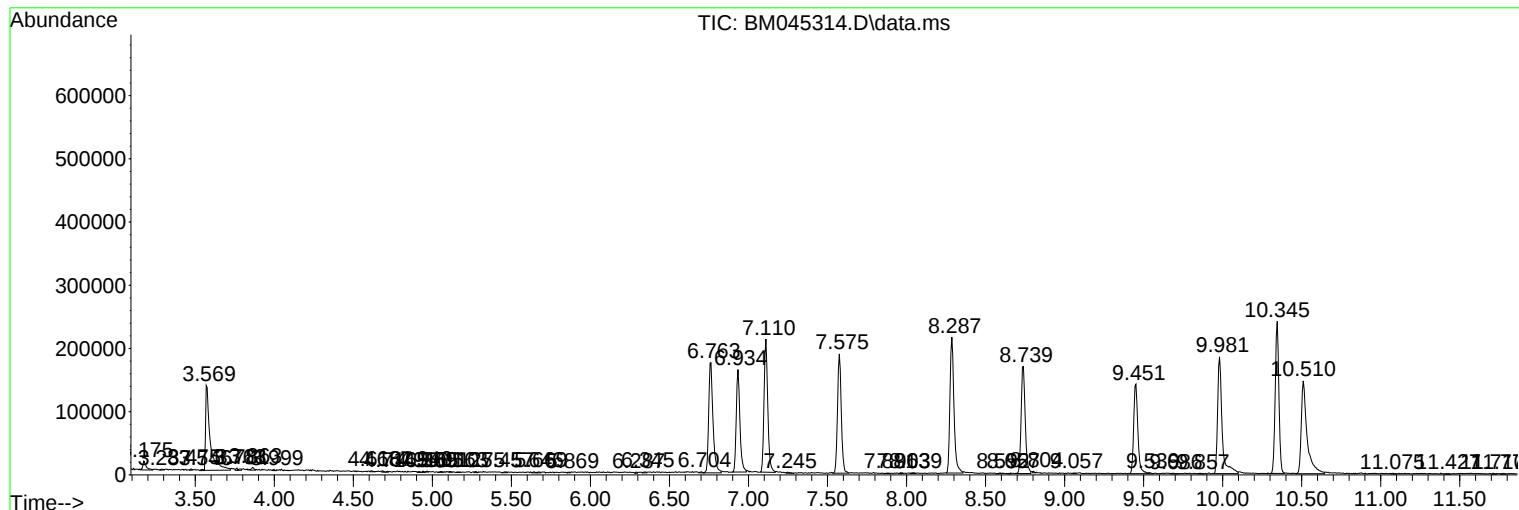

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045314.D
Acq On : 17 Apr 2024 13:23
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045314.D
Acq On : 17 Apr 2024 13:23
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------