

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045324.D
 Acq On : 17 Apr 2024 19:30
 Operator : MA/JU
 Sample : P2032-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	22	rBV	14825	21363	1.40%	0.163%
2	3.340	42	43	47	rVB4	2380	2131	0.14%	0.016%
3	3.581	81	84	95	rBV	43142	88715	5.80%	0.676%
4	3.658	95	97	99	rVV3	5320	5553	0.36%	0.042%
5	3.693	101	103	107	rVB4	2131	2666	0.17%	0.020%
6	3.775	113	117	126	rVB9	3594	6132	0.40%	0.047%
7	3.863	129	132	137	rVB5	4395	5762	0.38%	0.044%
8	4.022	155	159	160	rBV4	1842	1703	0.11%	0.013%
9	4.087	167	170	174	rVB5	1890	2442	0.16%	0.019%
10	4.163	181	183	186	rBV3	1449	2172	0.14%	0.017%
11	4.922	308	312	314	rBV5	1231	1838	0.12%	0.014%
12	5.063	333	336	342	rBV5	2032	3146	0.21%	0.024%
13	5.187	354	357	361	rBV6	1370	2429	0.16%	0.019%
14	5.634	431	433	437	rBV3	1240	1616	0.11%	0.012%
15	5.775	454	457	460	rBV3	1317	1599	0.10%	0.012%
16	6.504	576	581	582	rBV4	1228	1578	0.10%	0.012%
17	6.769	620	626	633	rBV	39779	79271	5.18%	0.604%
18	6.934	648	654	670	rBV	201454	349173	22.81%	2.662%
19	7.110	677	684	693	rBV	199577	346526	22.64%	2.642%
20	7.222	701	703	708	rVB4	1336	2205	0.14%	0.017%
21	7.298	714	716	719	rBV3	1585	1713	0.11%	0.013%
22	7.575	756	763	773	rBV	226021	384322	25.11%	2.930%
23	8.287	878	884	894	rBV2	131860	238196	15.56%	1.816%
24	8.734	954	960	968	rBV	244476	414019	27.05%	3.157%
25	9.004	1004	1006	1008	rBV2	1729	1634	0.11%	0.012%
26	9.445	1071	1081	1091	rVV	199393	346795	22.66%	2.644%
27	9.510	1091	1092	1097	rVB4	2343	2689	0.18%	0.021%
28	9.975	1165	1171	1191	rBV	230341	465505	30.41%	3.549%
29	10.345	1225	1234	1245	rVV	292629	509442	33.29%	3.884%
30	10.510	1254	1262	1286	rBV	178123	450590	29.44%	3.435%
31	11.392	1410	1412	1417	rVB4	988	1546	0.10%	0.012%
32	11.981	1507	1512	1516	rBV5	2491	5364	0.35%	0.041%
33	13.122	1701	1706	1709	rBV4	1847	3288	0.21%	0.025%
34	13.651	1789	1796	1810	rBV	422750	655848	42.85%	5.000%
35	13.916	1835	1841	1851	rBV2	564169	832845	54.42%	6.350%
36	14.227	1887	1894	1902	rVV	390931	596059	38.94%	4.545%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045324.D
 Acq On : 17 Apr 2024 19:30
 Operator : MA/JU
 Sample : P2032-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.416	1923	1926	1929	rBV3	1318	1905	0.12%	0.015%
38	14.533	1938	1946	1959	rBV7	6303	26255	1.72%	0.200%
39	14.798	1987	1991	1994	rBV5	1508	2198	0.14%	0.017%
40	14.839	1996	1998	2002	rVV4	1515	1879	0.12%	0.014%
41	15.227	2058	2064	2074	rBV	659840	992397	64.84%	7.566%
42	15.374	2082	2089	2103	rBV	165485	265799	17.37%	2.027%
43	15.474	2105	2106	2111	rVB3	3280	3225	0.21%	0.025%
44	15.939	2182	2185	2188	rBV2	1187	1689	0.11%	0.013%
45	16.692	2311	2313	2319	rVB3	1351	2058	0.13%	0.016%
46	16.986	2353	2363	2372	rBV	459836	628860	41.09%	4.795%
47	17.086	2374	2380	2391	rBV2	700496	1028722	67.21%	7.843%
48	17.339	2420	2423	2427	rVB4	1359	1970	0.13%	0.015%
49	17.568	2459	2462	2464	rBV2	1344	1768	0.12%	0.013%
50	17.774	2495	2497	2502	rVB4	1470	1708	0.11%	0.013%
51	17.904	2516	2519	2525	rBV4	8989	11846	0.77%	0.090%
52	18.145	2558	2560	2561	rBV2	1883	1538	0.10%	0.012%
53	18.957	2695	2698	2702	rVB3	8320	11069	0.72%	0.084%
54	18.986	2702	2703	2707	rBV4	2189	3074	0.20%	0.023%
55	19.033	2707	2711	2714	rVV4	5780	8057	0.53%	0.061%
56	19.080	2717	2719	2723	rVB5	1883	2038	0.13%	0.016%
57	19.198	2735	2739	2744	rBV5	7284	10957	0.72%	0.084%
58	19.392	2766	2772	2781	rBV	818186	1138171	74.36%	8.678%
59	19.733	2828	2830	2832	rBV3	2935	2175	0.14%	0.017%
60	20.056	2883	2885	2888	rBV4	3053	3548	0.23%	0.027%
61	20.156	2900	2902	2904	rBV3	2768	2921	0.19%	0.022%
62	20.621	2979	2981	2982	rBV	4381	2899	0.19%	0.022%
63	21.203	3075	3080	3090	rBV	483549	677736	44.28%	5.167%
64	23.256	3423	3429	3444	rVB2	824113	1530532	100.00%	11.669%
65	23.397	3447	3453	3468	rVB	455346	911041	59.52%	6.946%

Sum of corrected areas: 13115910




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045324.D
Acq On : 17 Apr 2024 19:30
Operator : MA/JU
Sample : P2032-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

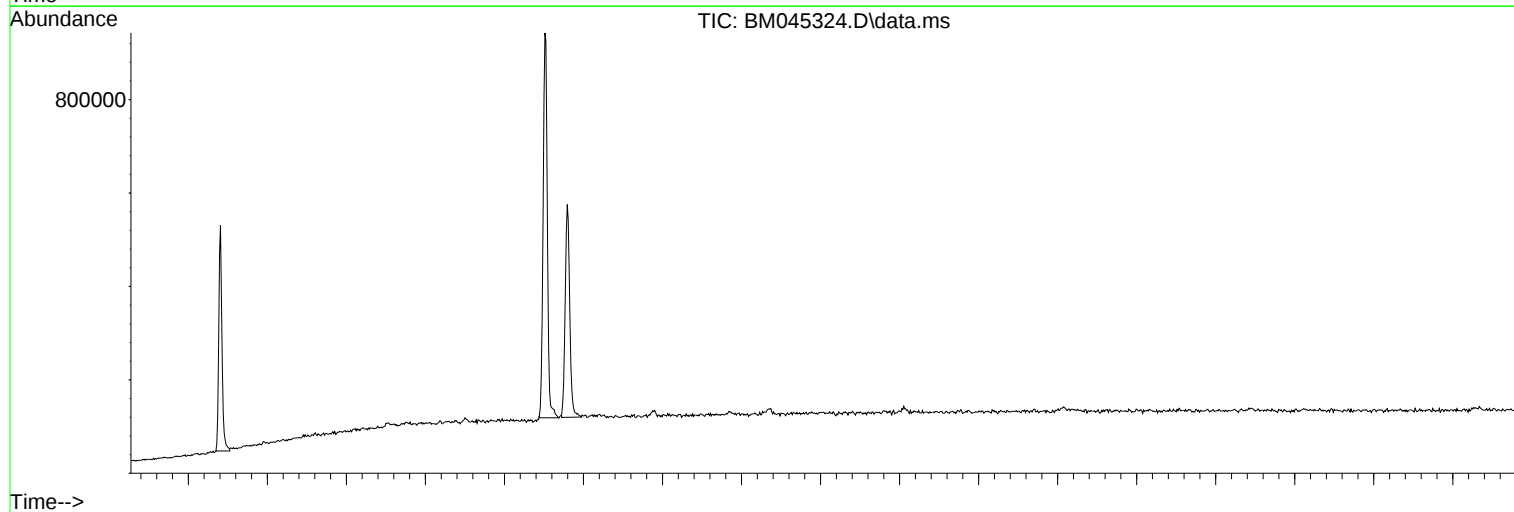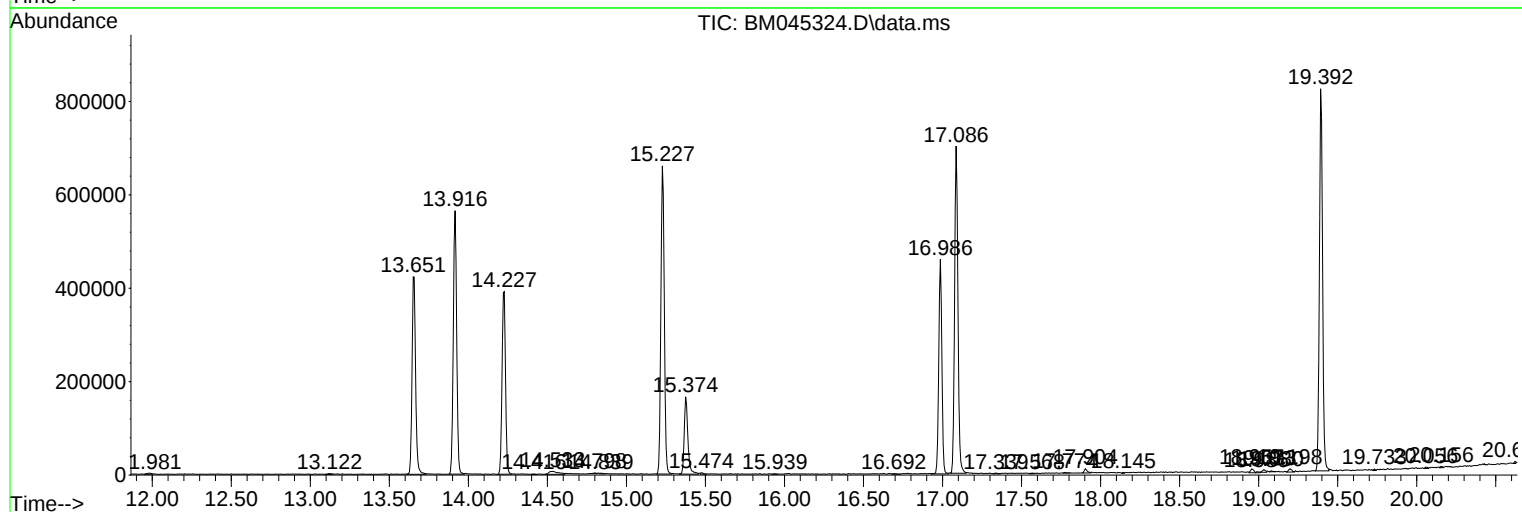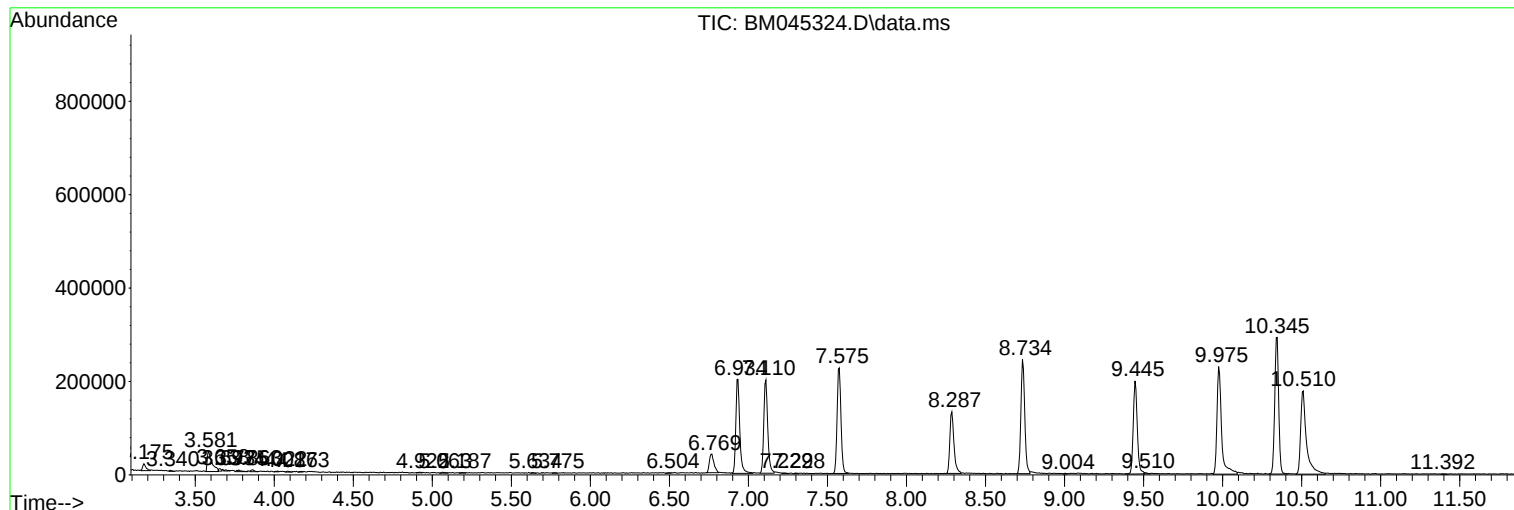

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045324.D
Acq On : 17 Apr 2024 19:30
Operator : MA/JU
Sample : P2032-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045324.D
Acq On : 17 Apr 2024 19:30
Operator : MA/JU
Sample : P2032-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------