

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045326.D
 Acq On : 17 Apr 2024 20:43
 Operator : MA/JU
 Sample : P2032-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	21	rBV2	12071	16556	1.00%	0.123%
2	3.269	27	31	32	rBV4	1260	1676	0.10%	0.012%
3	3.481	65	67	72	rVB6	1806	2315	0.14%	0.017%
4	3.581	80	84	93	rBV	54545	104723	6.34%	0.776%
5	3.869	129	133	135	rVB2	4034	5764	0.35%	0.043%
6	4.481	233	237	240	rBV6	1132	1717	0.10%	0.013%
7	4.746	279	282	284	rBV5	1864	2143	0.13%	0.016%
8	4.793	286	290	293	rBV3	1813	2748	0.17%	0.020%
9	5.546	415	418	421	rBV4	1755	1705	0.10%	0.013%
10	6.328	548	551	556	rBV6	1428	2943	0.18%	0.022%
11	6.763	618	625	635	rBV2	49654	98698	5.98%	0.731%
12	6.934	647	654	664	rBV	204349	340799	20.64%	2.524%
13	7.004	664	666	668	rVV2	2578	2076	0.13%	0.015%
14	7.110	678	684	693	rVV	202566	353688	21.42%	2.619%
15	7.175	693	695	698	rVB3	2034	2147	0.13%	0.016%
16	7.422	730	737	738	rBV3	1237	2039	0.12%	0.015%
17	7.575	756	763	774	rBV	237653	396227	24.00%	2.934%
18	7.887	815	816	823	rBV6	1101	1777	0.11%	0.013%
19	8.287	878	884	896	rBV2	143441	259658	15.73%	1.923%
20	8.734	953	960	972	rBV	237181	409021	24.78%	3.029%
21	8.846	977	979	983	rVB4	1515	1773	0.11%	0.013%
22	9.445	1074	1081	1093	rBV	194093	332938	20.17%	2.466%
23	9.975	1164	1171	1192	rBV	241670	466296	28.24%	3.453%
24	10.110	1192	1194	1199	rVV4	2445	3899	0.24%	0.029%
25	10.340	1224	1233	1244	rBV	304531	512353	31.03%	3.794%
26	10.504	1254	1261	1286	rBV	171741	422183	25.57%	3.126%
27	11.975	1505	1511	1520	rBV5	2634	6704	0.41%	0.050%
28	12.563	1604	1611	1612	rBV3	851	1680	0.10%	0.012%
29	13.122	1700	1706	1710	rBV3	2857	4831	0.29%	0.036%
30	13.563	1778	1781	1785	rBV3	1106	1794	0.11%	0.013%
31	13.651	1791	1796	1808	rVV	439046	660835	40.03%	4.894%
32	13.916	1834	1841	1854	rBV	549147	827876	50.15%	6.131%
33	14.222	1885	1893	1904	rBV	412735	601222	36.42%	4.452%
34	14.516	1938	1943	1944	rBV3	7320	7806	0.47%	0.058%
35	14.722	1975	1978	1982	rVB2	1427	1897	0.11%	0.014%
36	15.227	2058	2064	2075	rBV	673323	997752	60.44%	7.389%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045326.D
 Acq On : 17 Apr 2024 20:43
 Operator : MA/JU
 Sample : P2032-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.375	2084	2089	2103	rBV	175872	270512	16.39%	2.003%
38	15.475	2103	2106	2114	rVB3	3189	5823	0.35%	0.043%
39	16.022	2195	2199	2204	rVB4	1722	2265	0.14%	0.017%
40	16.439	2268	2270	2275	rBV3	1742	2375	0.14%	0.018%
41	16.986	2356	2363	2374	rBV	470212	650340	39.39%	4.816%
42	17.086	2374	2380	2395	rVB2	695684	1061756	64.31%	7.863%
43	17.904	2513	2519	2525	rBV3	6471	10873	0.66%	0.081%
44	18.145	2557	2560	2562	rBV2	1536	1757	0.11%	0.013%
45	18.339	2589	2593	2597	rVB3	2435	3211	0.19%	0.024%
46	18.404	2602	2604	2606	rBV3	1657	1958	0.12%	0.014%
47	18.810	2672	2673	2677	rBV4	1485	1833	0.11%	0.014%
48	18.874	2683	2684	2687	rBV3	1409	1781	0.11%	0.013%
49	18.957	2694	2698	2702	rBV6	6218	9694	0.59%	0.072%
50	19.027	2706	2710	2717	rBV5	5946	12755	0.77%	0.094%
51	19.192	2736	2738	2743	rVV5	7383	10645	0.64%	0.079%
52	19.274	2749	2752	2754	rBV4	1641	1977	0.12%	0.015%
53	19.392	2766	2772	2783	rVV	917970	1242536	75.26%	9.201%
54	19.639	2811	2814	2816	rBV4	2458	2962	0.18%	0.022%
55	19.674	2818	2820	2824	rVV5	1647	2369	0.14%	0.018%
56	19.762	2834	2835	2838	rBV3	1868	2034	0.12%	0.015%
57	19.904	2857	2859	2860	rBV2	3155	1870	0.11%	0.014%
58	20.974	3039	3041	3042	rBV2	5989	3917	0.24%	0.029%
59	21.198	3074	3079	3092	rBV	522370	734589	44.50%	5.440%
60	23.256	3422	3429	3436	rBV2	883808	1650932	100.00%	12.226%
61	23.398	3446	3453	3463	rVB	493938	952652	57.70%	7.055%

Sum of corrected areas: 13503675




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045326.D
Acq On : 17 Apr 2024 20:43
Operator : MA/JU
Sample : P2032-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

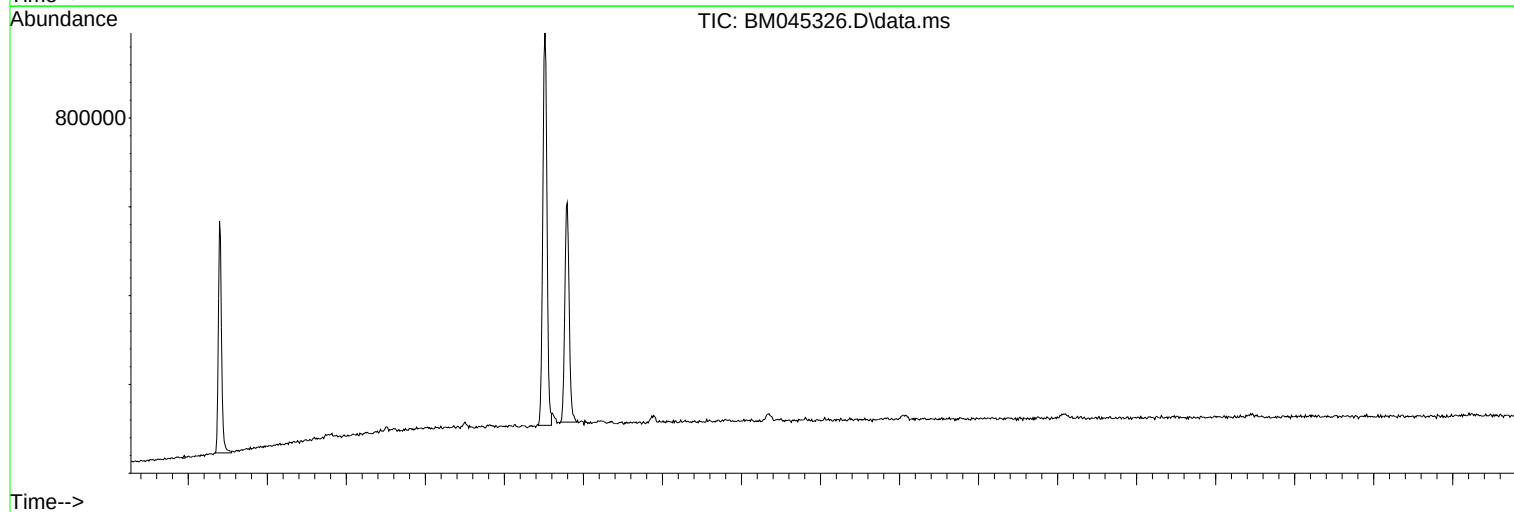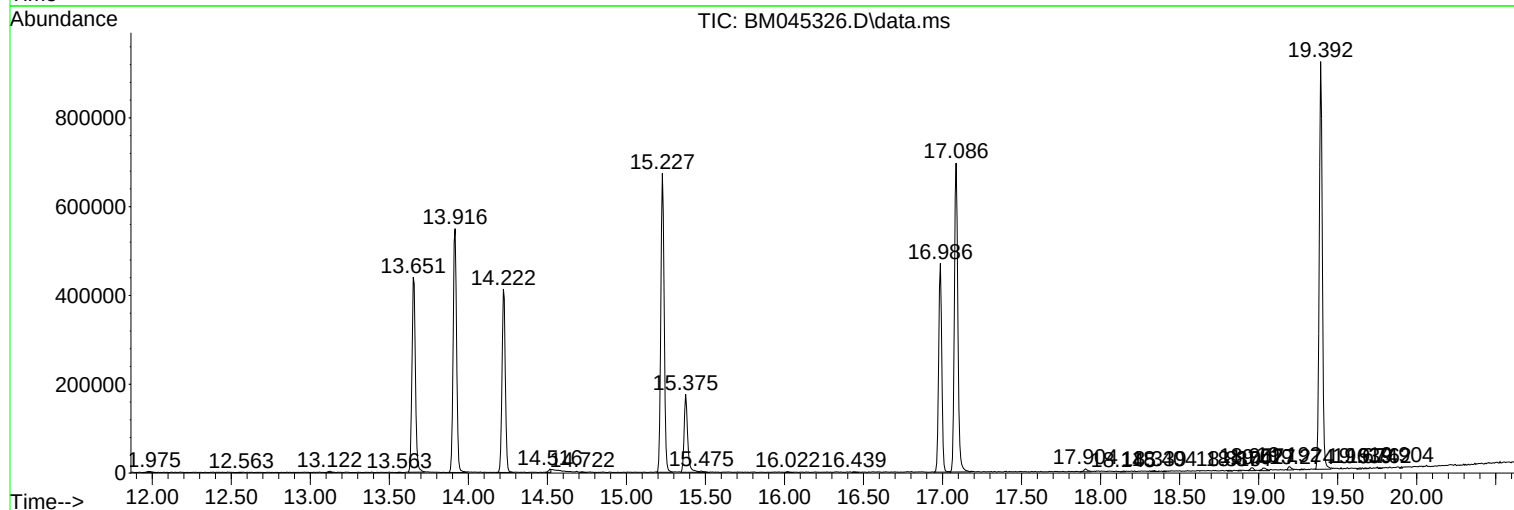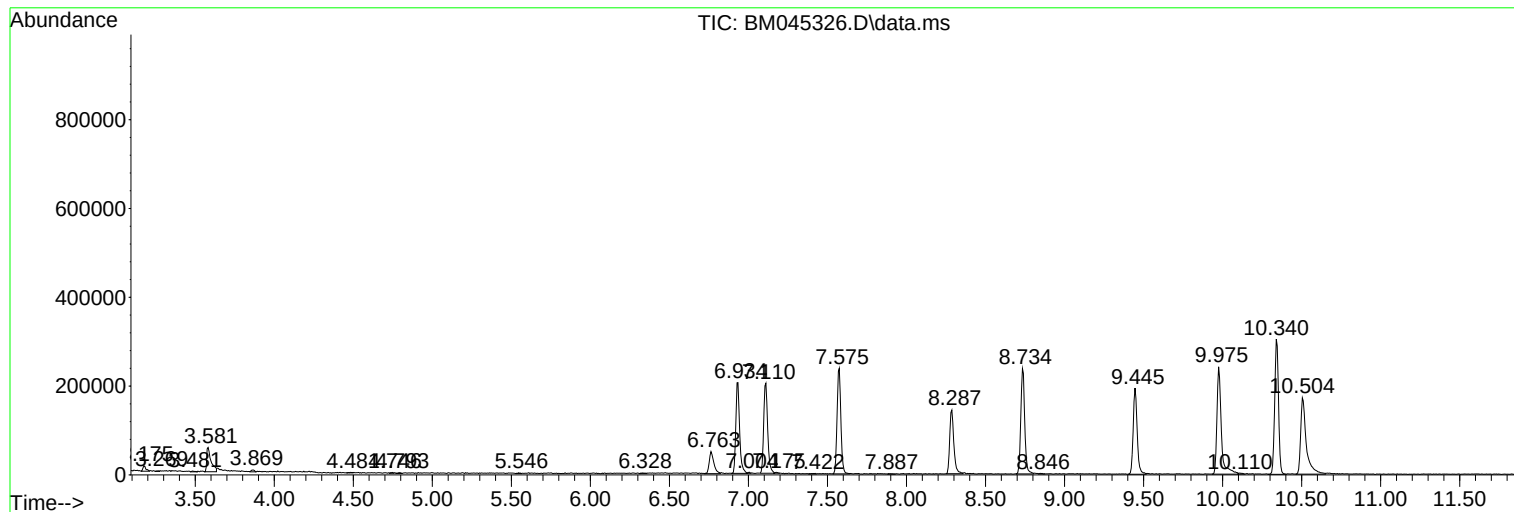

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045326.D
Acq On : 17 Apr 2024 20:43
Operator : MA/JU
Sample : P2032-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045326.D
Acq On : 17 Apr 2024 20:43
Operator : MA/JU
Sample : P2032-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------