

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045329.D
 Acq On : 17 Apr 2024 23:09
 Operator : MA/JU
 Sample : PB160307BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045329.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	21	rVB	11333	15453	1.59%	0.174%
2	3.575	80	83	97	rBV	109239	203909	20.99%	2.302%
3	4.163	181	183	186	rBV4	1906	1704	0.18%	0.019%
4	5.334	380	382	383	rBV2	1497	1296	0.13%	0.015%
5	6.145	518	520	522	rBV3	1424	1591	0.16%	0.018%
6	6.645	602	605	606	rVB3	1644	1298	0.13%	0.015%
7	6.757	618	624	639	rBV	145081	274126	28.21%	3.094%
8	6.934	648	654	665	rBV	126241	215053	22.13%	2.427%
9	7.104	676	683	693	rBV	167986	288399	29.68%	3.255%
10	7.304	715	717	719	rBV2	1140	1351	0.14%	0.015%
11	7.498	748	750	754	rBV5	1330	1646	0.17%	0.019%
12	7.575	756	763	770	rBV	145202	254682	26.21%	2.875%
13	7.981	831	832	837	rVB4	1414	1693	0.17%	0.019%
14	8.287	878	884	898	rBV	166778	313363	32.25%	3.537%
15	8.575	929	933	937	rVB4	1271	1493	0.15%	0.017%
16	8.681	948	951	953	rVB3	1756	1886	0.19%	0.021%
17	8.734	953	960	969	rBV	139808	258657	26.62%	2.920%
18	8.916	989	991	996	rBV4	1092	1543	0.16%	0.017%
19	9.104	1022	1023	1027	rBV2	885	1246	0.13%	0.014%
20	9.239	1044	1046	1050	rBV4	1763	2258	0.23%	0.025%
21	9.445	1075	1081	1092	rBV	114027	205409	21.14%	2.319%
22	9.551	1097	1099	1102	rBV4	1809	1649	0.17%	0.019%
23	9.757	1130	1134	1135	rVB2	1543	1365	0.14%	0.015%
24	9.781	1135	1138	1141	rBV4	1428	1478	0.15%	0.017%
25	9.981	1165	1172	1186	rBV	140384	292845	30.14%	3.305%
26	10.339	1227	1233	1244	rVB	188205	319120	32.84%	3.602%
27	10.451	1250	1252	1254	rVB2	1900	1428	0.15%	0.016%
28	10.510	1254	1262	1282	rBV	110195	307019	31.60%	3.465%
29	10.680	1289	1291	1294	rVB3	1266	1576	0.16%	0.018%
30	10.757	1300	1304	1306	rBV4	1075	1624	0.17%	0.018%
31	10.892	1326	1327	1331	rVB3	1567	1254	0.13%	0.014%
32	10.928	1331	1333	1336	rBV3	1322	1285	0.13%	0.015%
33	10.969	1337	1340	1343	rBV3	1240	1432	0.15%	0.016%
34	11.116	1362	1365	1368	rBV3	1015	1300	0.13%	0.015%
35	11.245	1383	1387	1391	rVB4	1218	1807	0.19%	0.020%
36	11.745	1470	1472	1475	rVB3	1471	1339	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045329.D
 Acq On : 17 Apr 2024 23:09
 Operator : MA/JU
 Sample : PB160307BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	11.922	1500	1502	1505	rBV4	1412	1492	0.15%	0.017%
38	11.980	1508	1512	1514	rVV3	1664	2282	0.23%	0.026%
39	12.004	1514	1516	1521	rVB4	1537	2182	0.22%	0.025%
40	12.516	1602	1603	1606	rBV2	1562	1353	0.14%	0.015%
41	12.951	1674	1677	1681	rBV4	976	1583	0.16%	0.018%
42	13.480	1764	1767	1771	rBV3	1603	2273	0.23%	0.026%
43	13.657	1791	1797	1809	rVB	248643	390751	40.22%	4.411%
44	13.916	1834	1841	1853	rBV	340179	494703	50.91%	5.584%
45	14.221	1887	1893	1905	rBV	250950	369571	38.04%	4.171%
46	14.386	1919	1921	1923	rBV2	1358	1351	0.14%	0.015%
47	14.486	1932	1938	1951	rBV4	35164	116619	12.00%	1.316%
48	14.780	1987	1988	1991	rVB2	1695	1407	0.14%	0.016%
49	14.857	1999	2001	2004	rVB2	1504	1231	0.13%	0.014%
50	14.904	2004	2009	2012	rBV3	972	1868	0.19%	0.021%
51	15.227	2056	2064	2073	rBV	389359	601110	61.87%	6.785%
52	15.374	2084	2089	2100	rBV	78913	135665	13.96%	1.531%
53	15.727	2144	2149	2153	rBV4	803	1717	0.18%	0.019%
54	16.021	2194	2199	2205	rBV6	1528	2743	0.28%	0.031%
55	16.445	2268	2271	2274	rBV3	1303	1805	0.19%	0.020%
56	16.480	2276	2277	2281	rVB4	1201	1421	0.15%	0.016%
57	16.986	2357	2363	2370	rBV	281372	391747	40.32%	4.422%
58	17.086	2374	2380	2395	rVB	407454	631201	64.96%	7.125%
59	17.927	2520	2523	2526	rBV3	1305	1788	0.18%	0.020%
60	18.309	2586	2588	2590	rBV2	1576	1313	0.14%	0.015%
61	18.892	2685	2687	2689	rBV	1398	1270	0.13%	0.014%
62	18.956	2694	2698	2703	rBV5	4451	7833	0.81%	0.088%
63	19.033	2709	2711	2718	rVB4	4062	5013	0.52%	0.057%
64	19.221	2741	2743	2744	rBV2	2121	1607	0.17%	0.018%
65	19.262	2748	2750	2751	rBV3	2407	1812	0.19%	0.020%
66	19.392	2766	2772	2785	rBV	500469	718384	73.94%	8.109%
67	21.203	3075	3080	3090	rBV	278755	440228	45.31%	4.969%
68	23.256	3423	3429	3444	rVB	542377	971640	100.00%	10.967%
69	23.397	3447	3453	3466	rVB	271891	567936	58.45%	6.410%




Sum of corrected areas: 8859476

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045329.D
Acq On : 17 Apr 2024 23:09
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

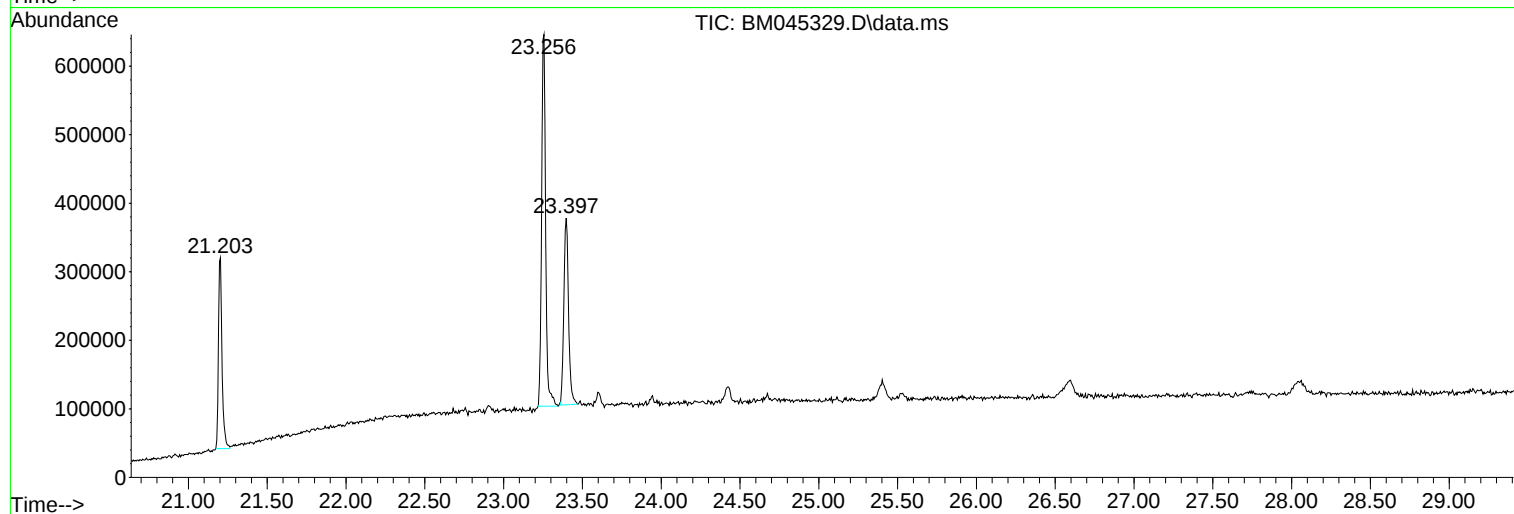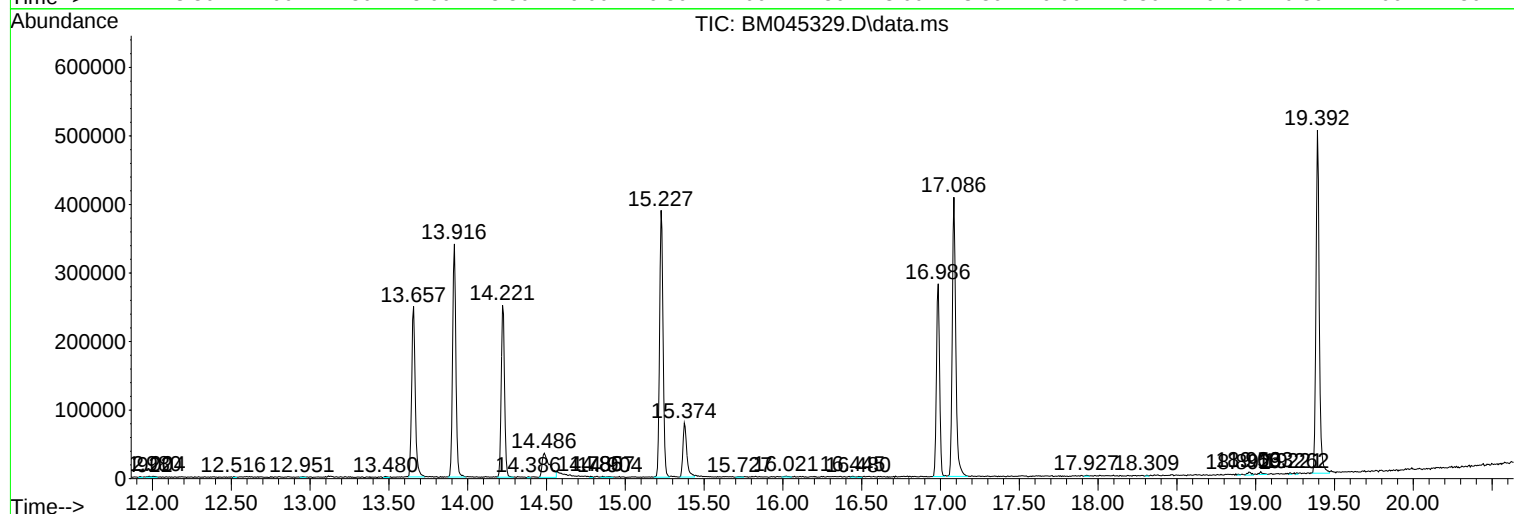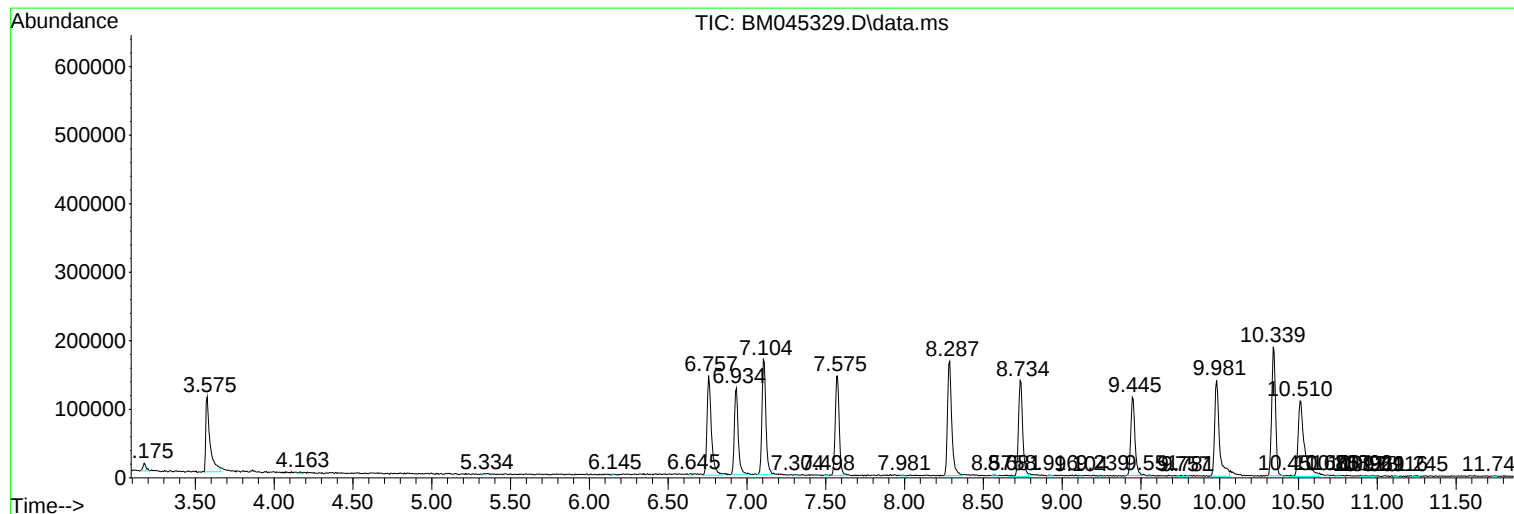

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045329.D
Acq On : 17 Apr 2024 23:09
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045329.D
Acq On : 17 Apr 2024 23:09
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------