

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045345.D
 Acq On : 18 Apr 2024 08:50
 Operator : MA/JU
 Sample : PB160316BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	20	rBV	12289	17802	1.44%	0.153%
2	3.352	44	45	47	rBV2	2596	1663	0.13%	0.014%
3	3.493	66	69	72	rBV3	2193	2340	0.19%	0.020%
4	3.569	79	82	97	rBV	153195	260917	21.04%	2.247%
5	3.822	123	125	126	rBV2	1725	1586	0.13%	0.014%
6	3.863	129	132	135	rVB3	3809	3787	0.31%	0.033%
7	3.928	141	143	145	rBV3	1429	1513	0.12%	0.013%
8	4.005	154	156	159	rVB3	2484	2346	0.19%	0.020%
9	4.105	169	173	176	rBV5	1037	1474	0.12%	0.013%
10	4.516	241	243	247	rVB3	1785	1950	0.16%	0.017%
11	4.728	277	279	283	rVB4	1231	1272	0.10%	0.011%
12	4.781	287	288	291	rBV2	1392	1330	0.11%	0.011%
13	5.034	330	331	336	rBV4	1452	1906	0.15%	0.016%
14	5.093	340	341	347	rVB6	1320	1521	0.12%	0.013%
15	5.199	356	359	362	rBV3	1408	1622	0.13%	0.014%
16	5.304	374	377	379	rBV3	1603	1803	0.15%	0.016%
17	5.363	385	387	390	rVB2	1971	1818	0.15%	0.016%
18	5.393	390	392	395	rVB3	1544	1720	0.14%	0.015%
19	5.510	409	412	414	rBV3	1227	1395	0.11%	0.012%
20	5.593	422	426	429	rBV6	962	1374	0.11%	0.012%
21	5.851	468	470	472	rBV3	1524	1321	0.11%	0.011%
22	5.904	472	479	481	rVV5	1353	2576	0.21%	0.022%
23	6.204	528	530	533	rVB4	1462	1799	0.15%	0.015%
24	6.322	547	550	552	rBV3	2066	2527	0.20%	0.022%
25	6.463	570	574	575	rBV3	987	1386	0.11%	0.012%
26	6.587	592	595	599	rBV3	991	1324	0.11%	0.011%
27	6.757	617	624	638	rBV	186806	340258	27.44%	2.931%
28	6.928	646	653	666	rBV	166455	267695	21.59%	2.306%
29	7.104	676	683	695	rBV	215804	354940	28.63%	3.057%
30	7.228	702	704	707	rBV4	1345	1415	0.11%	0.012%
31	7.257	707	709	712	rVB3	1858	2145	0.17%	0.018%
32	7.569	755	762	772	rBV	178188	282237	22.76%	2.431%
33	8.057	843	845	850	rVV4	1019	1350	0.11%	0.012%
34	8.281	876	883	900	rBV	223746	398878	32.17%	3.436%
35	8.592	933	936	938	rVB3	1220	1294	0.10%	0.011%
36	8.728	952	959	971	rBV	184748	322723	26.03%	2.780%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045345.D
 Acq On : 18 Apr 2024 08:50
 Operator : MA/JU
 Sample : PB160316BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	9.151	1028	1031	1034	rVB3	1463	1908	0.15%	0.016%
38	9.187	1034	1037	1040	rBV2	1214	1749	0.14%	0.015%
39	9.439	1074	1080	1095	rBV	155327	279413	22.54%	2.407%
40	9.975	1163	1171	1190	rBV	198924	403129	32.52%	3.472%
41	10.339	1226	1233	1242	rVB	210956	370037	29.85%	3.187%
42	10.422	1242	1247	1251	rVB5	1396	2818	0.23%	0.024%
43	10.504	1254	1261	1285	rBV	163315	397739	32.08%	3.426%
44	11.116	1364	1365	1368	rBV2	1188	1287	0.10%	0.011%
45	11.451	1421	1422	1427	rBV3	882	1335	0.11%	0.011%
46	11.592	1444	1446	1449	rVB4	1116	1287	0.10%	0.011%
47	11.628	1449	1452	1455	rBV4	1051	1555	0.13%	0.013%
48	11.698	1461	1464	1467	rBV3	1105	1313	0.11%	0.011%
49	11.975	1509	1511	1514	rVB4	1455	1671	0.13%	0.014%
50	12.063	1523	1526	1531	rVB3	1241	2285	0.18%	0.020%
51	12.598	1615	1617	1620	rVB2	1355	1382	0.11%	0.012%
52	12.622	1620	1621	1626	rBV4	979	1442	0.12%	0.012%
53	13.116	1702	1705	1708	rBV2	2248	2788	0.22%	0.024%
54	13.651	1790	1796	1809	rVV	356383	539776	43.54%	4.649%
55	13.910	1834	1840	1848	rBV2	449535	677274	54.63%	5.833%
56	14.004	1855	1856	1861	rVB4	1093	1307	0.11%	0.011%
57	14.222	1887	1893	1899	rBV	312950	460948	37.18%	3.970%
58	14.345	1910	1914	1915	rBV3	1162	1256	0.10%	0.011%
59	14.469	1928	1935	1946	rBV2	68804	184538	14.88%	1.589%
60	15.227	2054	2064	2072	rBV	521239	804320	64.87%	6.928%
61	15.374	2083	2089	2100	rVV	135951	225866	18.22%	1.945%
62	15.474	2103	2106	2112	rVB5	1764	2590	0.21%	0.022%
63	15.674	2137	2140	2142	rBV2	1234	1620	0.13%	0.014%
64	15.986	2189	2193	2196	rBV3	1254	2194	0.18%	0.019%
65	16.092	2208	2211	2213	rVB4	1291	1554	0.13%	0.013%
66	16.363	2254	2257	2259	rBV3	1067	1561	0.13%	0.013%
67	16.515	2280	2283	2287	rBV2	1000	1254	0.10%	0.011%
68	16.727	2317	2319	2324	rVB5	1406	1865	0.15%	0.016%
69	16.980	2357	2362	2369	rVV	369464	519330	41.89%	4.473%
70	17.027	2369	2370	2373	rVV2	1615	1504	0.12%	0.013%
71	17.080	2373	2379	2395	rVB2	545889	852249	68.74%	7.341%
72	17.545	2456	2458	2461	rBV3	952	1272	0.10%	0.011%
73	17.904	2515	2519	2524	rVB7	3070	4513	0.36%	0.039%
74	18.080	2546	2549	2551	rVV3	1464	1558	0.13%	0.013%
75	18.115	2554	2555	2558	rBV3	1511	1368	0.11%	0.012%
76	18.298	2584	2586	2588	rBV3	1173	1472	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045345.D
 Acq On : 18 Apr 2024 08:50
 Operator : MA/JU
 Sample : PB160316BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	18.657	2645	2647	2650	rBV3	1528	1356	0.11%	0.012%
78	18.698	2651	2654	2656	rVB3	1381	1489	0.12%	0.013%
79	18.957	2693	2698	2701	rBV2	6456	8201	0.66%	0.071%
80	19.027	2705	2710	2713	rBV4	3943	6332	0.51%	0.055%
81	19.115	2724	2725	2727	rVB	2353	1255	0.10%	0.011%
82	19.351	2763	2765	2766	rBV2	1272	1283	0.10%	0.011%
83	19.392	2766	2772	2788	rVV2	686790	975567	78.69%	8.403%
84	19.615	2808	2810	2812	rBV3	1774	1839	0.15%	0.016%
85	19.668	2818	2819	2821	rBV2	1754	1434	0.12%	0.012%
86	19.792	2838	2840	2842	rBV3	1825	1759	0.14%	0.015%
87	19.992	2870	2874	2877	rBV4	3146	4498	0.36%	0.039%
88	20.615	2978	2980	2981	rBV2	3876	2232	0.18%	0.019%
89	21.198	3074	3079	3087	rBV	398998	573640	46.27%	4.941%
90	23.256	3422	3429	3435	rBV2	686078	1239815	100.00%	10.679%
91	23.392	3446	3452	3466	rVB	368927	730130	58.89%	6.289%




Sum of corrected areas: 11610164

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045345.D
Acq On : 18 Apr 2024 08:50
Operator : MA/JU
Sample : PB160316BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

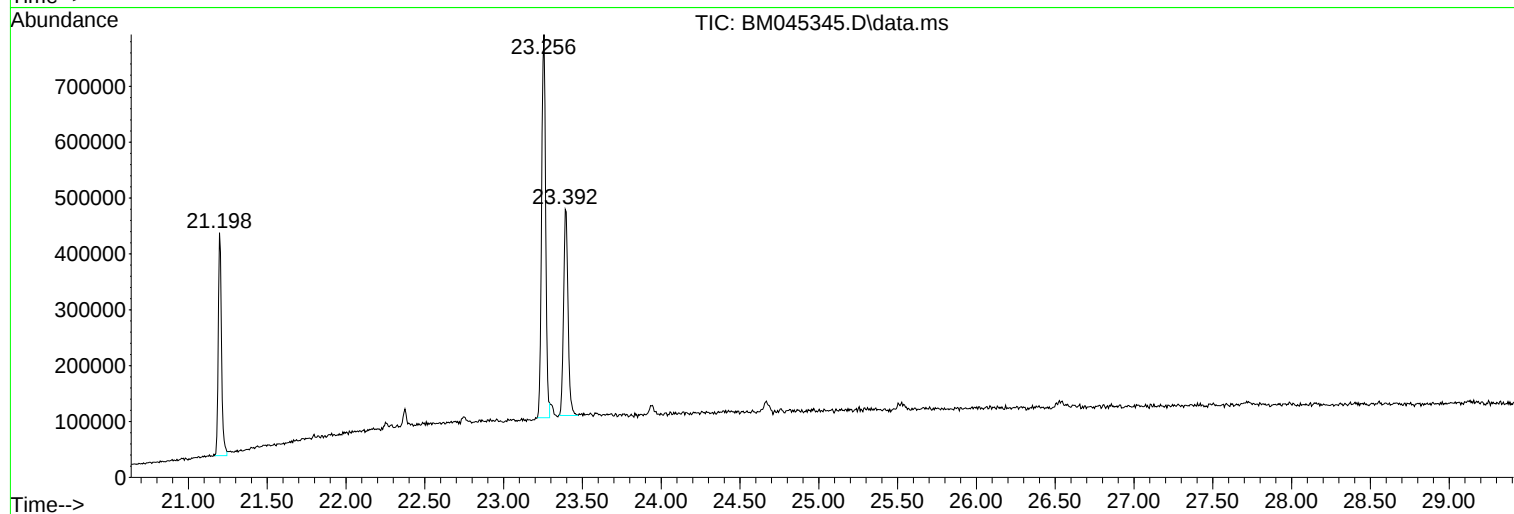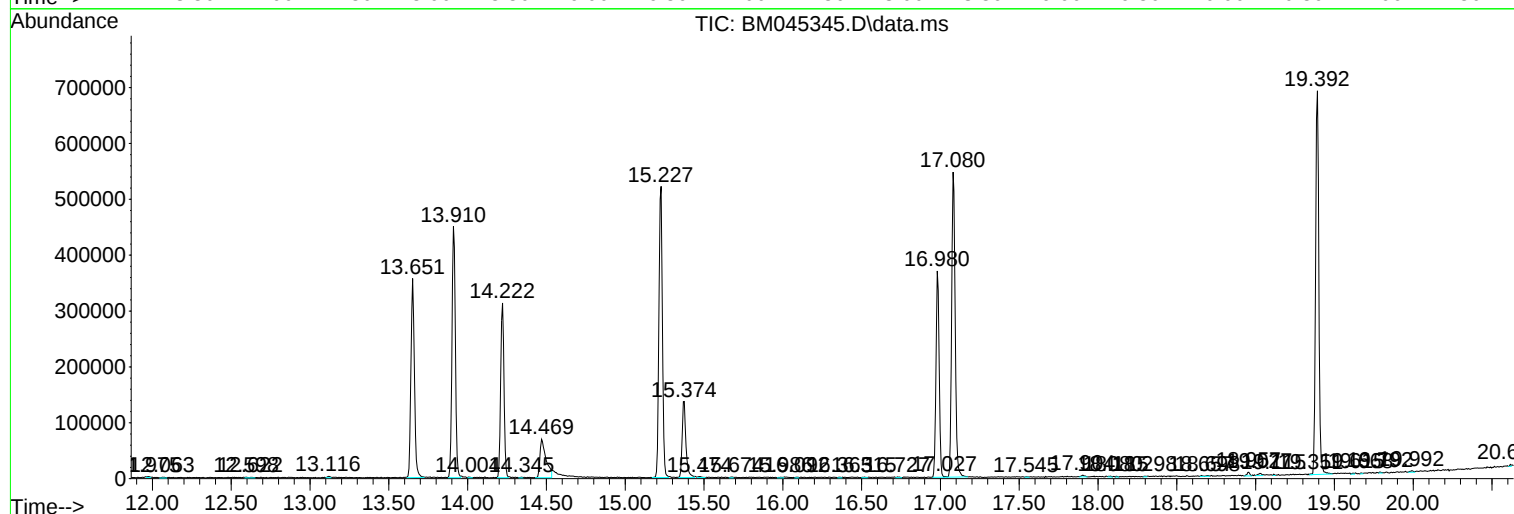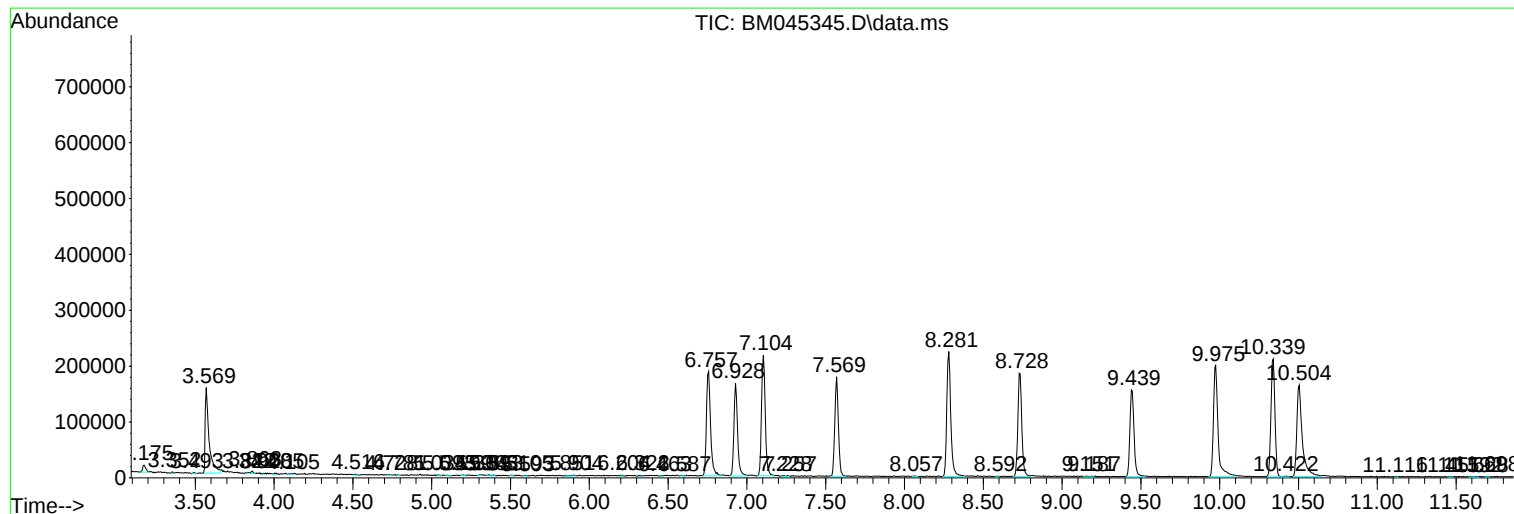

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045345.D
Acq On : 18 Apr 2024 08:50
Operator : MA/JU
Sample : PB160316BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045345.D
Acq On : 18 Apr 2024 08:50
Operator : MA/JU
Sample : PB160316BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------