

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045346.D
 Acq On : 18 Apr 2024 09:26
 Operator : MA/JU
 Sample : PB160307BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	12	15	20	rVB	12909	15656	1.28%	0.130%
2	3.281	31	33	34	rBV	1859	1327	0.11%	0.011%
3	3.393	50	52	55	rBV3	1479	1359	0.11%	0.011%
4	3.569	79	82	100	rBV	142306	248456	20.39%	2.067%
5	3.858	127	131	135	rBV4	4034	6350	0.52%	0.053%
6	3.928	142	143	146	rBV3	1741	1426	0.12%	0.012%
7	4.075	166	168	170	rBV3	2101	1869	0.15%	0.016%
8	4.340	211	213	216	rVB3	1571	1270	0.10%	0.011%
9	4.452	230	232	234	rBV3	1348	1335	0.11%	0.011%
10	4.699	270	274	275	rVB3	1217	1418	0.12%	0.012%
11	4.746	279	282	286	rBV4	1273	2392	0.20%	0.020%
12	4.775	286	287	291	rVV3	1820	1835	0.15%	0.015%
13	4.840	293	298	299	rBV4	1736	2294	0.19%	0.019%
14	4.940	312	315	318	rVB3	1578	1885	0.15%	0.016%
15	5.163	350	353	358	rVB4	1062	1337	0.11%	0.011%
16	5.275	369	372	375	rBV6	1394	1507	0.12%	0.013%
17	5.322	377	380	381	rBV3	1482	1440	0.12%	0.012%
18	5.428	396	398	399	rBV2	1498	1307	0.11%	0.011%
19	6.016	494	498	499	rBV3	1357	1844	0.15%	0.015%
20	6.081	507	509	514	rVB4	1392	1863	0.15%	0.015%
21	6.175	522	525	526	rVB3	1505	1294	0.11%	0.011%
22	6.275	540	542	543	rBV	1404	1288	0.11%	0.011%
23	6.534	583	586	587	rBV2	1368	1285	0.11%	0.011%
24	6.751	618	623	636	rBV	177815	327032	26.84%	2.720%
25	6.928	647	653	669	rVB	158563	269116	22.09%	2.239%
26	7.104	677	683	692	rBV	211772	351441	28.84%	2.923%
27	7.304	715	717	719	rVB3	1467	1313	0.11%	0.011%
28	7.410	732	735	737	rVB4	1094	1266	0.10%	0.011%
29	7.569	755	762	772	rBV	220949	362834	29.78%	3.018%
30	7.675	777	780	782	rVV3	1338	1699	0.14%	0.014%
31	8.040	840	842	845	rVB3	1088	1268	0.10%	0.011%
32	8.281	877	883	900	rBV	218577	391639	32.14%	3.258%
33	8.493	916	919	922	rVV4	1098	1531	0.13%	0.013%
34	8.581	932	934	937	rVV3	1159	1283	0.11%	0.011%
35	8.734	953	960	972	rVV	176254	319162	26.19%	2.655%
36	8.898	985	988	989	rBV3	1432	1299	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045346.D
 Acq On : 18 Apr 2024 09:26
 Operator : MA/JU
 Sample : PB160307BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	9.045	1011	1013	1016	rVB4	1809	1570	0.13%	0.013%
38	9.075	1016	1018	1021	rBV4	1124	1773	0.15%	0.015%
39	9.169	1033	1034	1037	rBV2	1469	1289	0.11%	0.011%
40	9.445	1073	1081	1093	rBV	151384	274959	22.57%	2.287%

41	9.540	1096	1097	1100	rVB4	1911	1658	0.14%	0.014%
42	9.563	1100	1101	1104	rBV2	1360	1488	0.12%	0.012%
43	9.657	1115	1117	1120	rVB3	1134	1235	0.10%	0.010%
44	9.975	1164	1171	1187	rBV	193166	393464	32.29%	3.273%
45	10.339	1225	1233	1242	rBV	272294	462633	37.97%	3.848%

46	10.504	1253	1261	1280	rBV	157253	387113	31.77%	3.220%
47	10.751	1300	1303	1305	rVV3	1278	1715	0.14%	0.014%
48	10.810	1309	1313	1314	rVV2	1336	1515	0.12%	0.013%
49	10.857	1318	1321	1327	rVV5	1472	2626	0.22%	0.022%
50	10.904	1327	1329	1333	rVV4	1043	1374	0.11%	0.011%

51	10.998	1342	1345	1347	rBV3	1247	1241	0.10%	0.010%
52	11.581	1442	1444	1451	rVV4	1183	1939	0.16%	0.016%
53	11.828	1482	1486	1489	rBV4	1091	1688	0.14%	0.014%
54	11.975	1507	1511	1514	rVB3	1755	2639	0.22%	0.022%
55	12.651	1624	1626	1632	rBV3	740	1276	0.10%	0.011%

56	12.763	1639	1645	1647	rBV5	1254	2030	0.17%	0.017%
57	13.045	1687	1693	1696	rBV3	1138	2676	0.22%	0.022%
58	13.080	1696	1699	1701	rVV3	1455	1674	0.14%	0.014%
59	13.116	1701	1705	1710	rVV5	2853	6071	0.50%	0.051%
60	13.175	1714	1715	1718	rVB2	1277	1244	0.10%	0.010%

61	13.651	1790	1796	1810	rVV	347571	525332	43.11%	4.370%
62	13.910	1833	1840	1851	rBV2	431591	654226	53.69%	5.442%
63	14.222	1887	1893	1901	rBV	382863	559106	45.89%	4.651%
64	14.474	1929	1936	1957	rBV2	61108	198677	16.31%	1.653%
65	14.722	1976	1978	1981	rVB3	1139	1289	0.11%	0.011%

66	14.780	1987	1988	1992	rVB	1772	1587	0.13%	0.013%
67	14.810	1992	1993	1996	rBV3	1724	1502	0.12%	0.012%
68	15.086	2037	2040	2045	rBV2	1434	1648	0.14%	0.014%
69	15.227	2057	2064	2072	rBV	515961	778341	63.88%	6.475%
70	15.280	2072	2073	2078	rVB2	1250	1416	0.12%	0.012%

71	15.369	2083	2088	2096	rBV	134745	206358	16.94%	1.717%
72	15.474	2103	2106	2107	rVB3	1602	1587	0.13%	0.013%
73	15.527	2113	2115	2121	rVB3	1139	1450	0.12%	0.012%
74	15.716	2144	2147	2152	rBV5	1157	1440	0.12%	0.012%
75	16.192	2227	2228	2231	rBV2	1689	1367	0.11%	0.011%

76	16.980	2356	2362	2369	rBV	438506	612193	50.24%	5.093%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045346.D
 Acq On : 18 Apr 2024 09:26
 Operator : MA/JU
 Sample : PB160307BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

77	17.080	2373	2379	2394	rVV2	530712	824380	67.66%	6.858%
78	17.510	2451	2452	2458	rVV3	1129	1631	0.13%	0.014%
79	17.610	2463	2469	2470	rVB5	1144	1260	0.10%	0.010%
80	17.951	2525	2527	2530	rVB2	1367	1395	0.11%	0.012%
81	17.980	2530	2532	2536	rBV4	1251	1523	0.12%	0.013%
82	18.015	2536	2538	2540	rBV3	1262	1237	0.10%	0.010%
83	18.486	2612	2618	2621	rBV5	1395	2806	0.23%	0.023%
84	18.551	2628	2629	2632	rBV3	1239	1580	0.13%	0.013%
85	18.721	2656	2658	2661	rVB5	1474	1304	0.11%	0.011%
86	18.951	2693	2697	2701	rVB4	4923	6666	0.55%	0.055%
87	19.027	2707	2710	2716	rVB6	3744	5521	0.45%	0.046%
88	19.098	2719	2722	2726	rBV4	2405	3359	0.28%	0.028%
89	19.221	2741	2743	2746	rBV3	1159	1562	0.13%	0.013%
90	19.345	2762	2764	2766	rBV3	1990	1745	0.14%	0.015%
91	19.392	2766	2772	2783	rVV	693597	936234	76.84%	7.788%
92	19.574	2801	2803	2804	rVB2	2053	1317	0.11%	0.011%
93	19.598	2804	2807	2808	rBV3	2229	2162	0.18%	0.018%
94	19.651	2814	2816	2818	rBV2	1760	1387	0.11%	0.012%
95	19.674	2818	2820	2821	rBV2	1698	1647	0.14%	0.014%
96	19.833	2845	2847	2849	rVB3	2556	1934	0.16%	0.016%
97	20.815	3013	3014	3015	rBV	3778	1568	0.13%	0.013%
98	21.198	3074	3079	3089	rBV	488658	673481	55.27%	5.602%
99	23.250	3422	3428	3435	rBV2	667525	1218486	100.00%	10.136%
100	23.392	3445	3452	3463	rBV	457090	889788	73.02%	7.402%




Sum of corrected areas: 12021302

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045346.D
Acq On : 18 Apr 2024 09:26
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

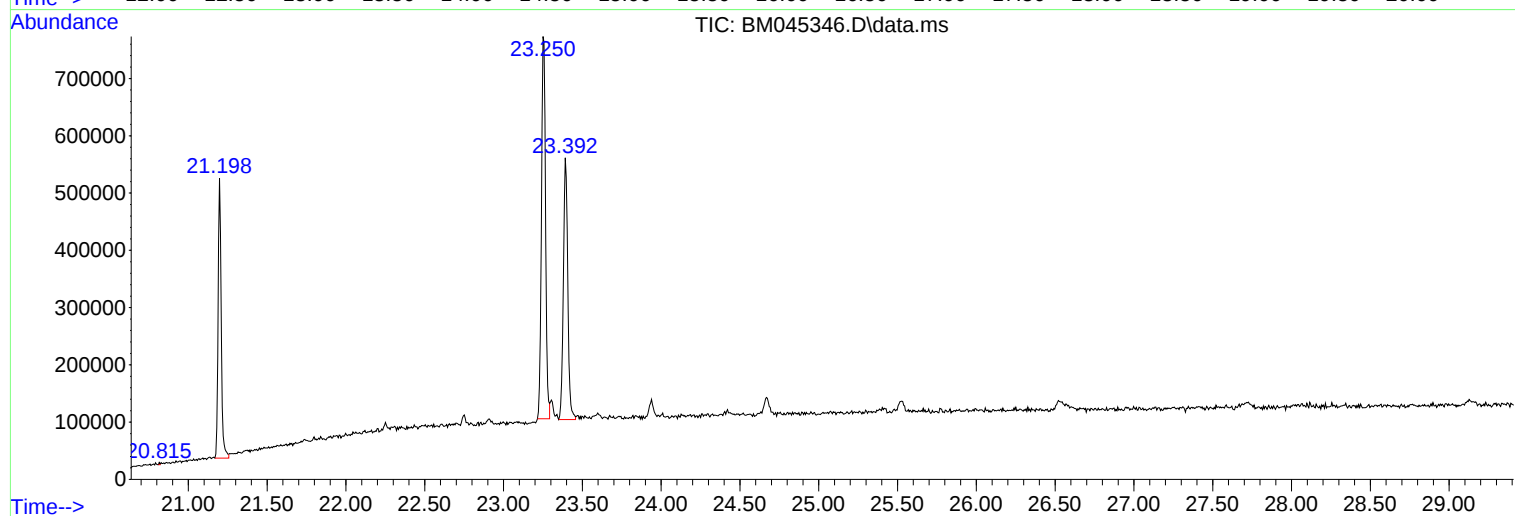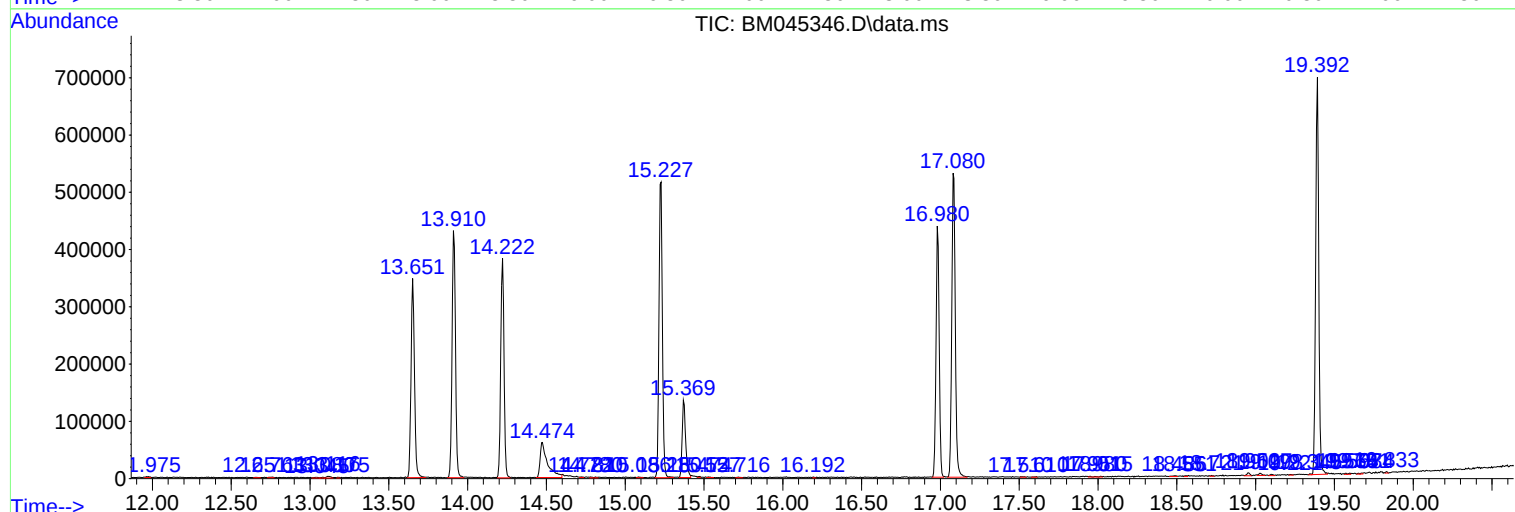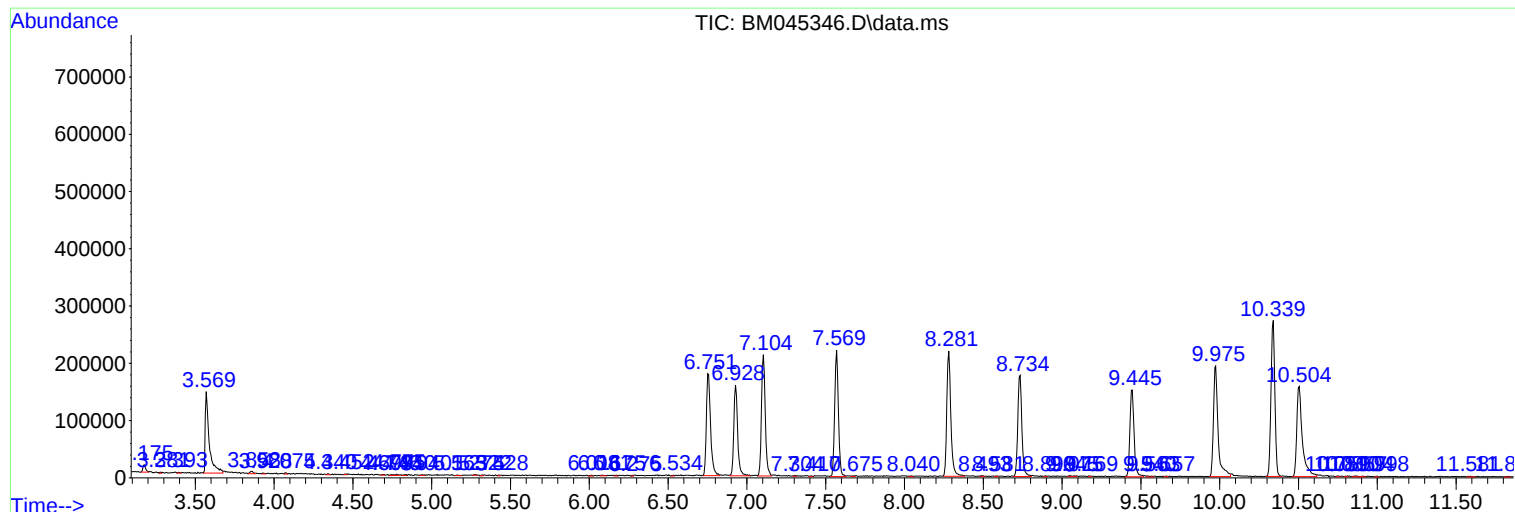

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045346.D
Acq On : 18 Apr 2024 09:26
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045346.D
Acq On : 18 Apr 2024 09:26
Operator : MA/JU
Sample : PB160307BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK307

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------