

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045357.D
 Acq On : 18 Apr 2024 16:05
 Operator : MA/JU
 Sample : P2145-14
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E07Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	5	7	12	rVB6	3828	4403	0.28%	0.035%
2	3.169	12	14	18	rBV	9298	11347	0.71%	0.091%
3	3.257	26	29	33	rBV5	3593	4646	0.29%	0.037%
4	3.334	41	42	45	rVB2	3127	2833	0.18%	0.023%
5	3.493	67	69	71	rBV3	1973	2294	0.14%	0.018%
6	3.581	81	84	94	rBV	29543	58203	3.65%	0.465%
7	3.793	118	120	123	rVB3	1757	1802	0.11%	0.014%
8	3.857	127	131	137	rVB4	7327	12512	0.78%	0.100%
9	3.975	148	151	155	rVV6	3132	4601	0.29%	0.037%
10	4.228	189	194	196	rBV5	2841	4346	0.27%	0.035%
11	4.251	196	198	200	rVB2	2715	2314	0.15%	0.019%
12	4.287	200	204	206	rBV4	1693	2743	0.17%	0.022%
13	4.322	206	210	215	rBV4	2051	3647	0.23%	0.029%
14	4.457	231	233	237	rBV5	1865	2564	0.16%	0.020%
15	4.646	264	265	270	rBV5	1202	1833	0.11%	0.015%
16	4.875	301	304	310	rVV7	1914	2780	0.17%	0.022%
17	5.081	336	339	342	rBV5	1857	2101	0.13%	0.017%
18	5.175	351	355	359	rVB6	1455	2418	0.15%	0.019%
19	6.757	618	624	633	rBV2	49690	100486	6.30%	0.803%
20	6.857	638	641	646	rVB5	1816	3315	0.21%	0.027%
21	6.928	646	653	664	rBV	191890	319414	20.03%	2.554%
22	7.104	677	683	692	rBV	197232	319269	20.02%	2.553%
23	7.169	692	694	697	rVB3	2357	2344	0.15%	0.019%
24	7.569	754	762	771	rBV	180845	305140	19.14%	2.440%
25	8.281	877	883	900	rBV2	128705	233579	14.65%	1.867%
26	8.457	908	913	919	rVB4	3400	5035	0.32%	0.040%
27	8.728	952	959	973	rBV	228180	387626	24.31%	3.099%
28	8.898	985	988	991	rBV5	1874	2317	0.15%	0.019%
29	9.439	1072	1080	1094	rBV	179711	312485	19.60%	2.498%
30	9.904	1157	1159	1164	rBV5	1287	2086	0.13%	0.017%
31	9.969	1164	1170	1190	rVV	214130	423821	26.58%	3.388%
32	10.333	1226	1232	1242	rVB	234427	398065	24.96%	3.183%
33	10.504	1253	1261	1278	rBV	155409	373922	23.45%	2.990%
34	11.963	1503	1509	1514	rVB6	2693	5099	0.32%	0.041%
35	12.104	1530	1533	1538	rVB3	1145	1703	0.11%	0.014%
36	12.304	1565	1567	1571	rBV2	1071	1630	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
 Data File : BM045357.D
 Acq On : 18 Apr 2024 16:05
 Operator : MA/JU
 Sample : P2145-14
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E07Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.116	1699	1705	1711	rVB4	2796	5127	0.32%	0.041%
38	13.651	1789	1796	1808	rBV	420910	638731	40.06%	5.107%
39	13.910	1833	1840	1851	rBV	538642	809375	50.76%	6.471%
40	14.221	1885	1893	1903	rVB	329915	502385	31.51%	4.017%
41	14.521	1938	1944	1946	rBV4	6512	11629	0.73%	0.093%
42	14.921	2008	2012	2018	rBV4	2111	3723	0.23%	0.030%
43	15.221	2057	2063	2078	rBV	630370	964426	60.48%	7.711%
44	15.374	2083	2089	2102	rVV	159709	262453	16.46%	2.098%
45	15.468	2102	2105	2110	rVB4	3012	3595	0.23%	0.029%
46	15.621	2128	2131	2135	rVB3	1319	2043	0.13%	0.016%
47	16.021	2193	2199	2202	rBV6	1808	3756	0.24%	0.030%
48	16.980	2356	2362	2369	rBV	406777	568704	35.67%	4.547%
49	17.080	2373	2379	2394	rVV2	682908	1044777	65.52%	8.353%
50	17.321	2418	2420	2424	rBV3	1412	2175	0.14%	0.017%
51	17.439	2438	2440	2446	rVB4	1361	2526	0.16%	0.020%
52	17.492	2446	2449	2451	rBV2	1621	2162	0.14%	0.017%
53	17.615	2465	2470	2475	rBV4	1557	3561	0.22%	0.028%
54	17.833	2503	2507	2509	rBV4	1898	2185	0.14%	0.017%
55	17.892	2512	2517	2528	rVB3	20722	34217	2.15%	0.274%
56	17.980	2528	2532	2534	rBV4	1411	2041	0.13%	0.016%
57	18.145	2555	2560	2564	rVB5	1683	2476	0.16%	0.020%
58	18.209	2569	2571	2574	rVB3	1485	1600	0.10%	0.013%
59	18.562	2630	2631	2636	rBV4	1126	1850	0.12%	0.015%
60	18.951	2694	2697	2701	rVB3	7673	10161	0.64%	0.081%
61	19.027	2706	2710	2715	rVB2	6146	7998	0.50%	0.064%
62	19.192	2733	2738	2743	rBV4	20085	28961	1.82%	0.232%
63	19.392	2765	2772	2781	rBV	808284	1189191	74.58%	9.508%
64	19.680	2819	2821	2823	rBV3	1742	1668	0.10%	0.013%
65	19.715	2826	2827	2829	rBV2	2430	1680	0.11%	0.013%
66	19.756	2833	2834	2837	rBV3	2320	2160	0.14%	0.017%
67	19.974	2869	2871	2873	rBV3	2652	2135	0.13%	0.017%
68	21.197	3074	3079	3090	rBV	471317	650247	40.78%	5.199%
69	23.250	3422	3428	3435	rBV2	837776	1594550	100.00%	12.748%
70	23.391	3446	3452	3462	rVB	417615	818773	51.35%	6.546%


Sum of corrected areas: 12507764

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045357.D
Acq On : 18 Apr 2024 16:05
Operator : MA/JU
Sample : P2145-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

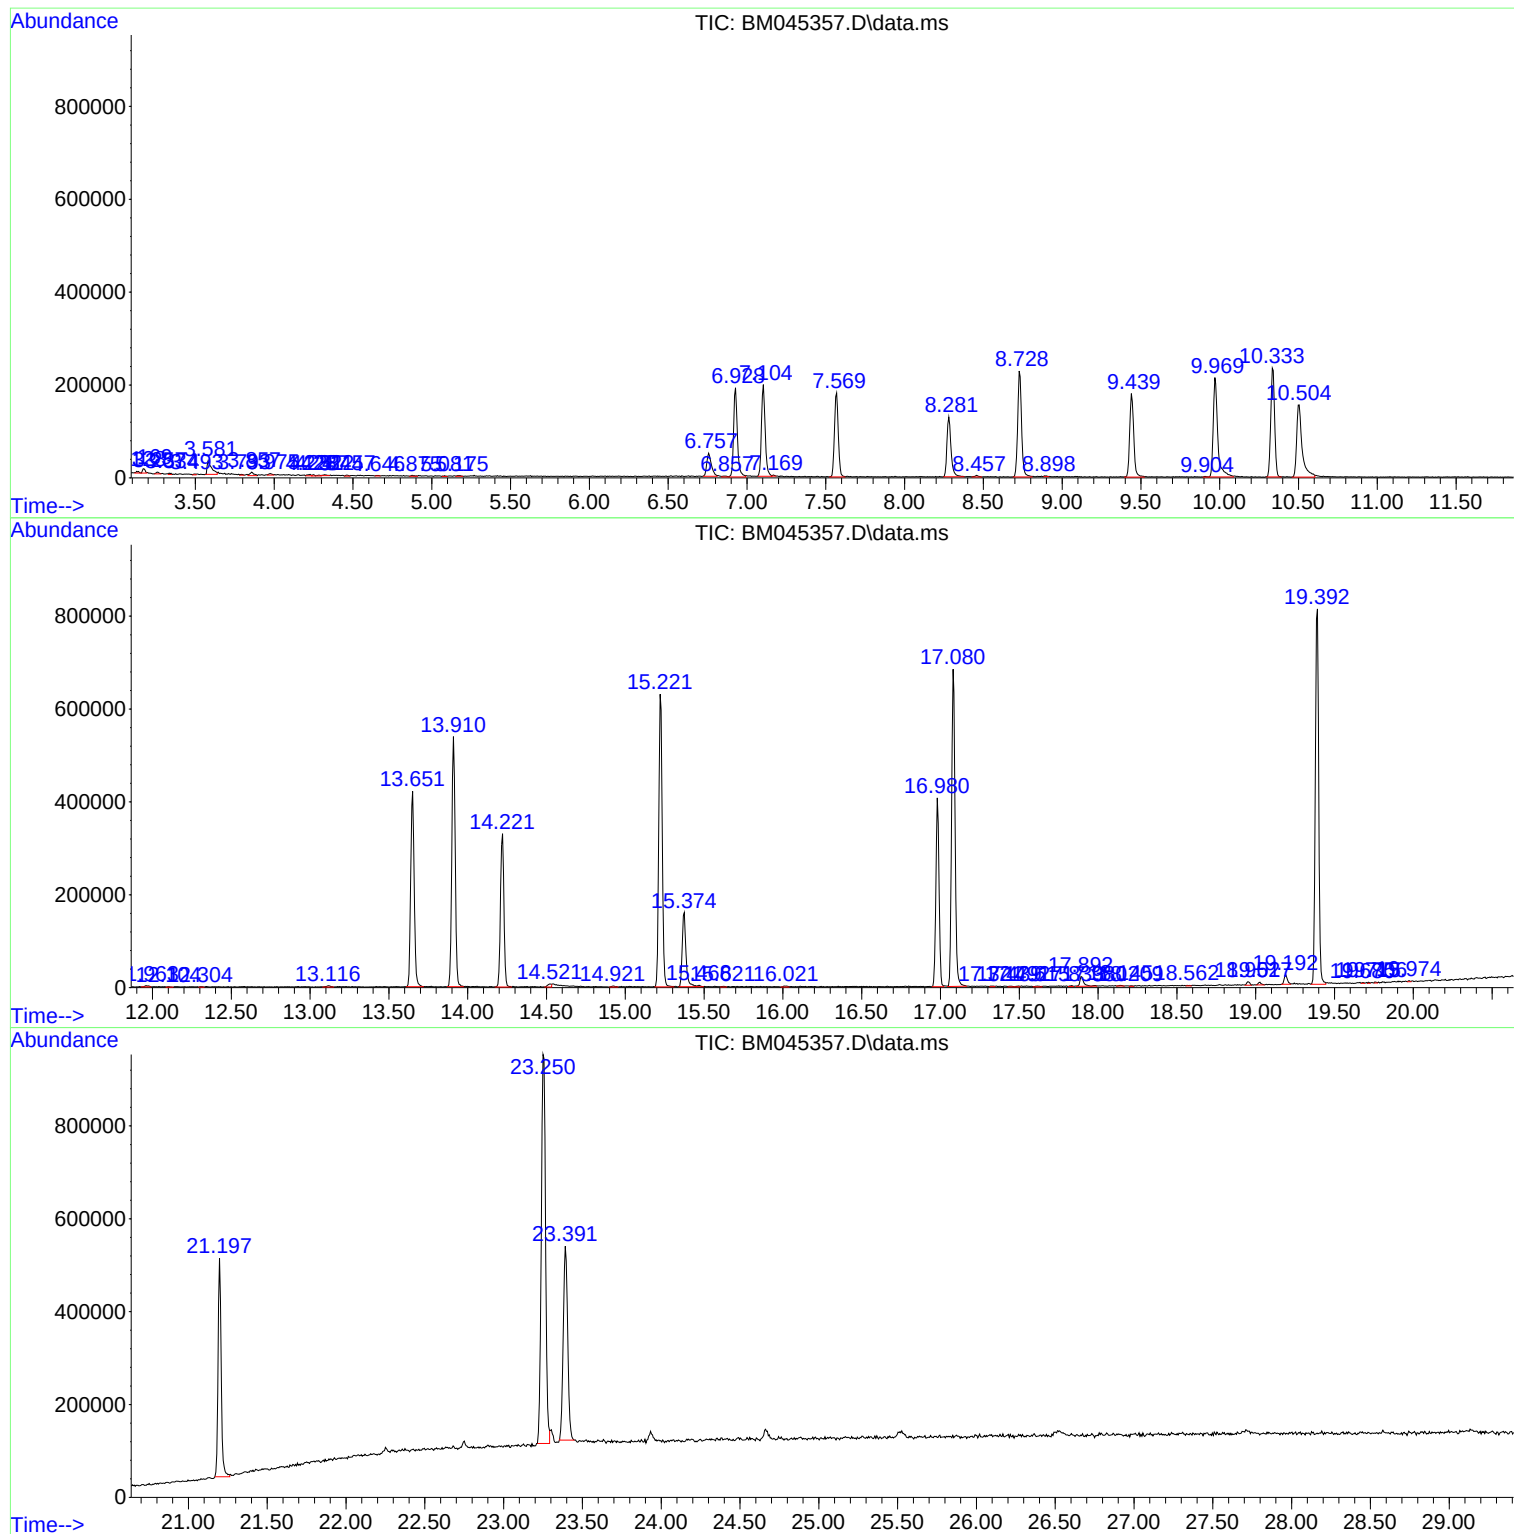

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045357.D
Acq On : 18 Apr 2024 16:05
Operator : MA/JU
Sample : P2145-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041724\
Data File : BM045357.D
Acq On : 18 Apr 2024 16:05
Operator : MA/JU
Sample : P2145-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E07Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc