


Data Path : Z:\HPCHEM1\BNA M\DATA\BM041815\
 Data File : BM001040.D
 Acq On : 17 Apr 2015 21:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM041815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 10 16:15:17 2015

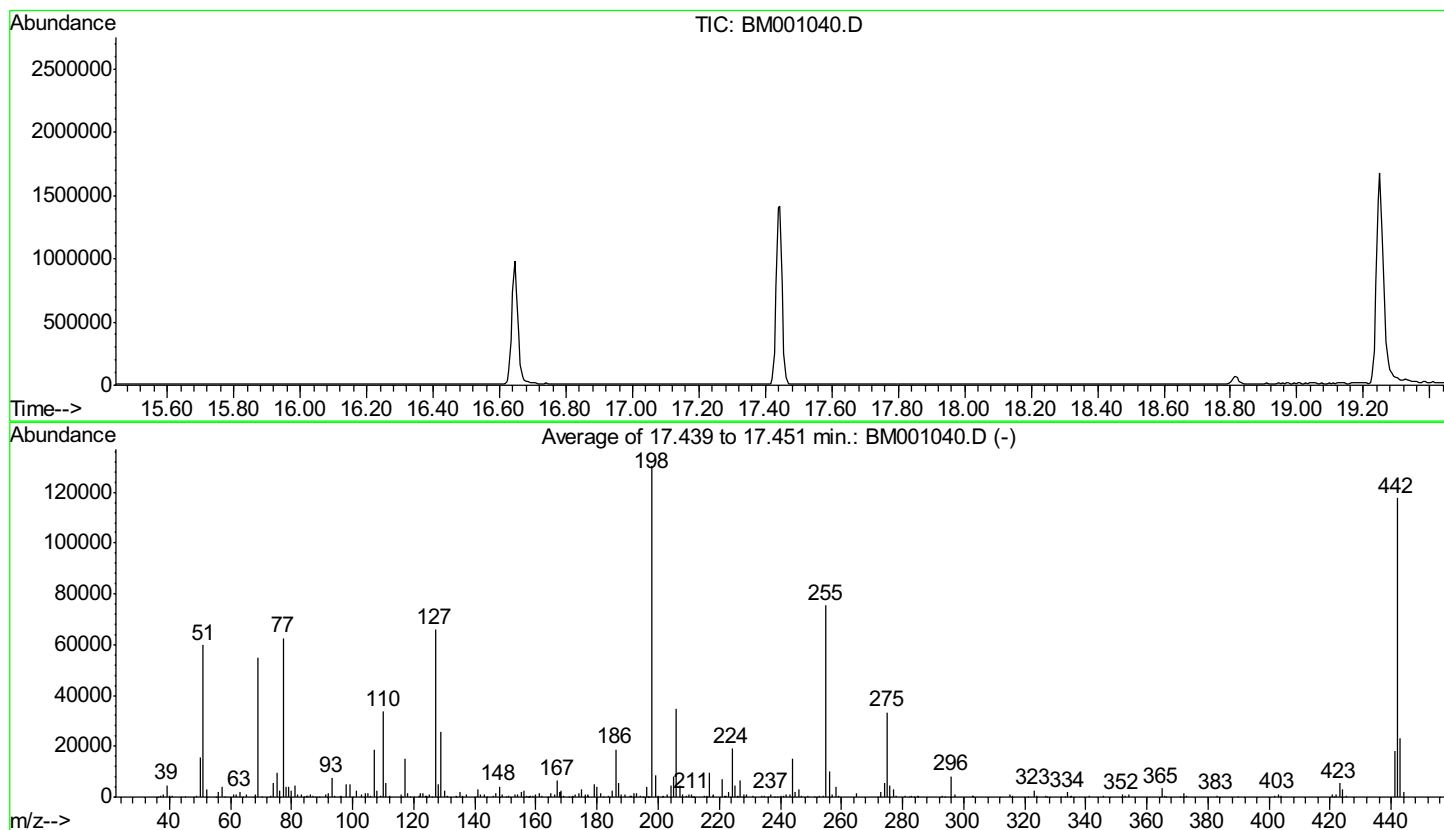

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.9	59856	PASS
68	69	0.00	2	1.7	934	PASS
69	198	0.00	100	42.3	55112	PASS
70	69	0.00	2	0.3	187	PASS
127	198	10	80	50.5	65800	PASS
197	198	0.00	2	0.2	258	PASS
198	198	100	100	100.0	130421	PASS
199	198	5	9	6.6	8612	PASS
275	198	10	60	25.7	33480	PASS
365	198	1	100	2.7	3491	PASS
441	442	0.01	24	15.4	18138	PASS
442	198	50	100	90.2	117658	PASS
443	442	15	24	19.8	23269	PASS