

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041816\
 Data File : BM004987.D
 Acq On : 18 Apr 2016 23:47
 Operator : UM/SJ
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD0.460

Quant Time: Apr 19 08:29:27 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM041816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 19 08:25:48 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	1119	0.40	ng/ul	0.00
4) Naphthalene-d8	10.61	136	4549	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.45	164	2229	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.19	188	4477	0.40	ng/ul	0.00
18) Chrysene-d12	21.38	240	3766	0.40	ng/ul	-0.01
22) Perylene-d12	23.67	264	2914	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.31	96	1152	2.13	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.21	152	2085	0.38	ng/ul	0.01
16) Fluoranthene-d10	19.23	212	3752	0.41	ng/ul	0.00
Target Compounds				Ovalue		
3) 1,4-Dioxane	3.34	88	1399	2.10	ng/ul#	23
5) Naphthalene	10.66	128	4372	0.41	ng/ul#	94
7) 2-Methylnaphthalene	12.28	142	2740	0.38	ng/ul	97
9) Acenaphthylene	14.16	152	3511	0.39	ng/ul#	97
10) Acenaphthene	14.50	153	2991	0.40	ng/ul#	84
11) Fluorene	15.51	166	3117	0.39	ng/ul#	97
13) Pentachlorophenol	16.87	266	204	0.39	ng/ul	95
14) Phenanthrene	17.23	178	4771	0.39	ng/ul#	91
15) Anthracene	17.33	178	3890	0.37	ng/ul	94
17) Fluoranthene	19.25	202	5162	0.41	ng/ul	93
19) Pyrene	19.62	202	5329	0.35	ng/ul	98
20) Benzo(a)anthracene	21.37	228	3760	0.38	ng/ul	95
21) Chrysene	21.42	228	5062	0.42	ng/ul	97
23) Benzo(b)fluoranthene	22.97	252	4013	0.38	ng/ul	91
24) Benzo(k)fluoranthene	23.01	252	4470	0.44	ng/ul#	92
25) Benzo(a)pyrene	23.57	252	3717	0.41	ng/ul#	88
26) Indeno(1,2,3-cd)pyrene	25.98	276	3761	0.41	ng/ul#	79
27) Dibenzo(a,h)anthracene	26.01	278	2911	0.41	ng/ul#	81
28) Benzo(g,h,i)perylene	26.68	276	3472	0.41	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041816\
Data File : BM004987.D
Acq On : 18 Apr 2016 23:47
Operator : UM/SJ
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
SSTD0.460

Quant Time: Apr 19 08:29:27 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM041816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 19 08:25:48 2016
Response via : Initial Calibration

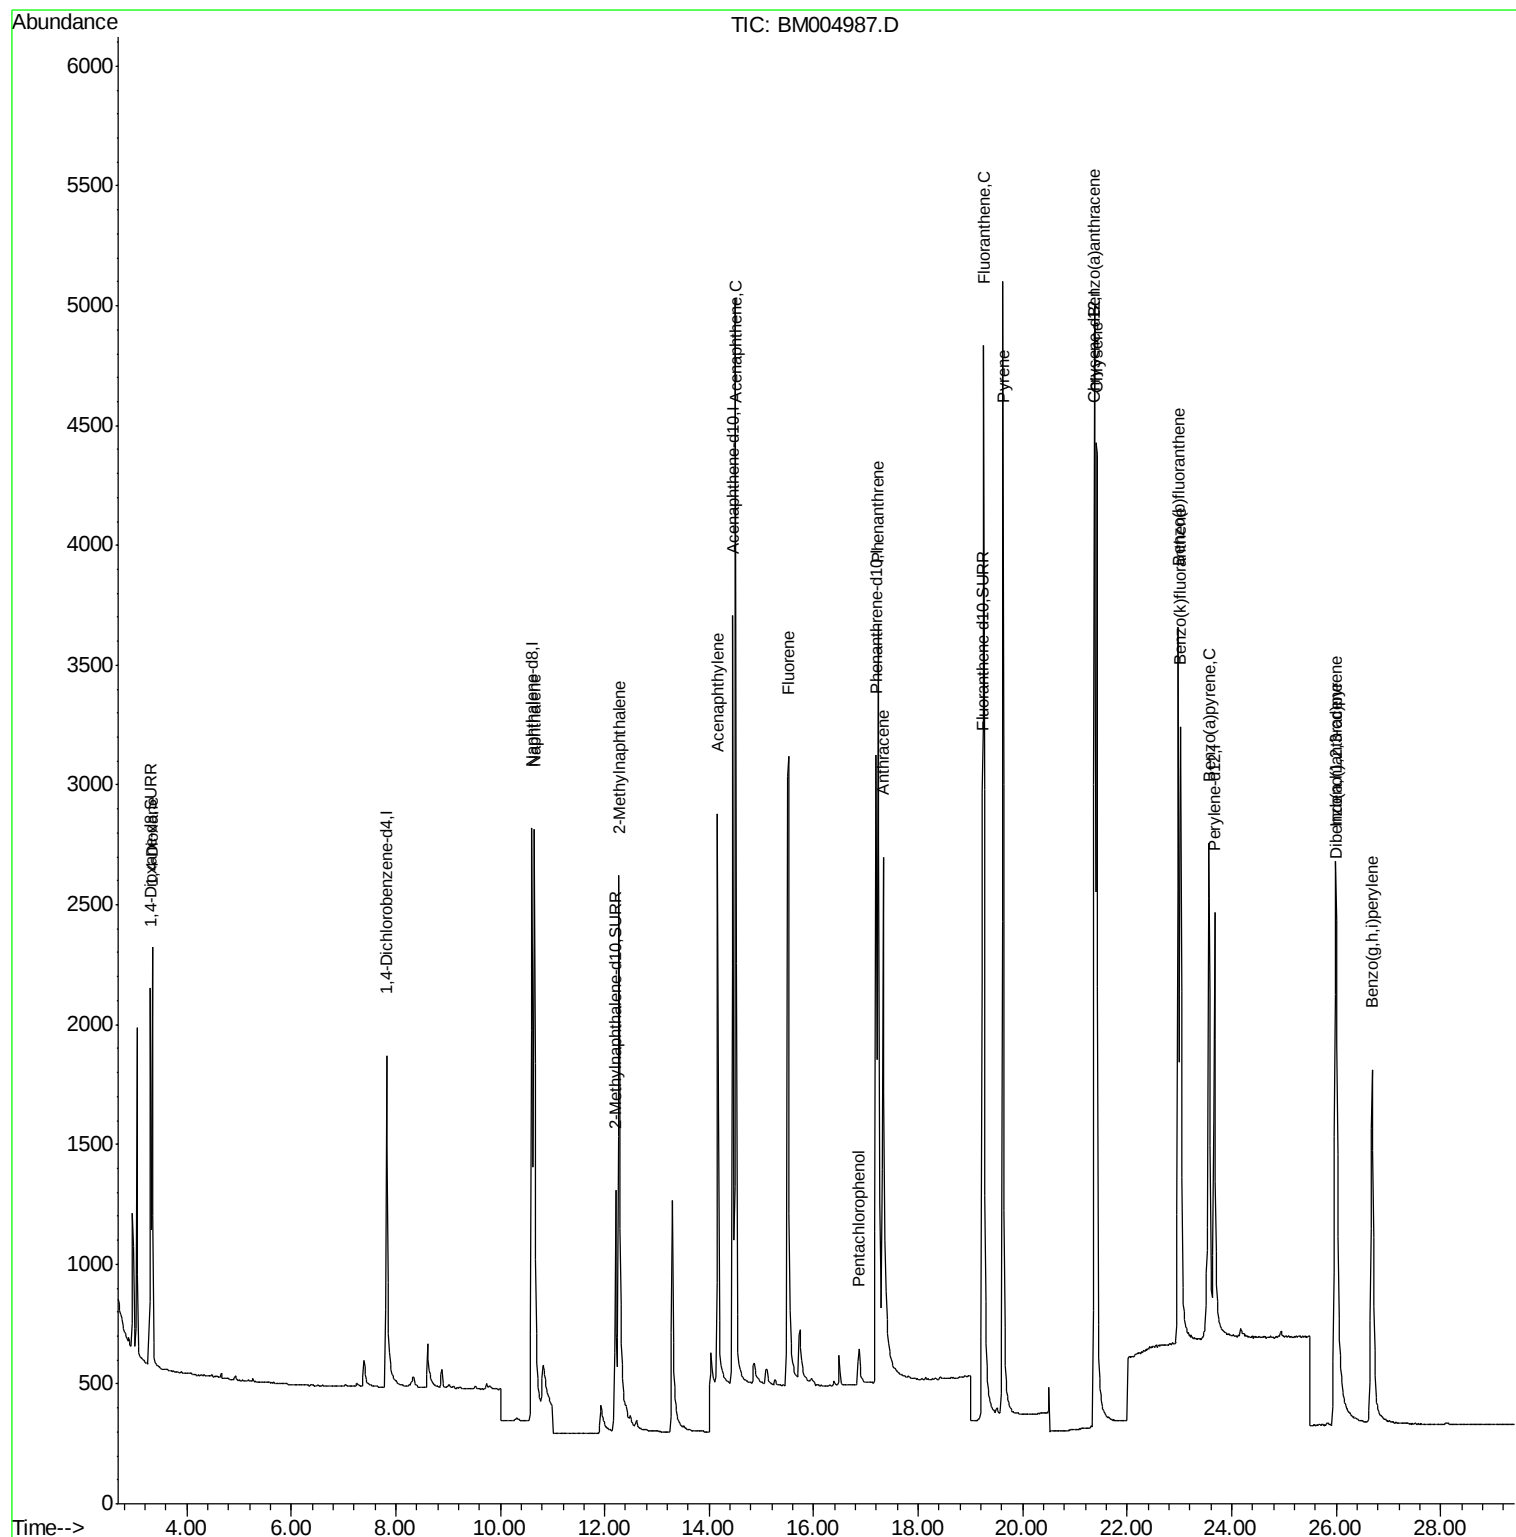

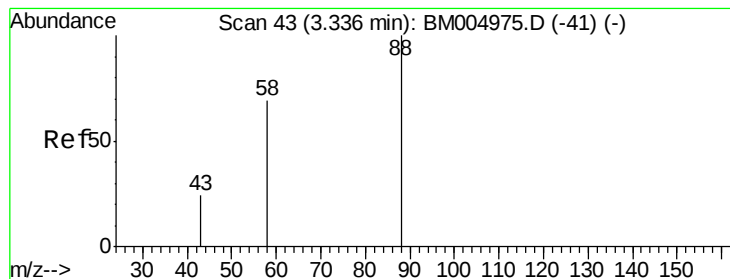

#3

1,4-Dioxane

Concen: 2.10 ng/ul

RT: 3.34 min Scan# 43

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion: 88 Resp: 1399

Ion Ratio Lower Upper

88 100

58 57.4 8.0 12.0#




43 19.4 8.0 12.0#

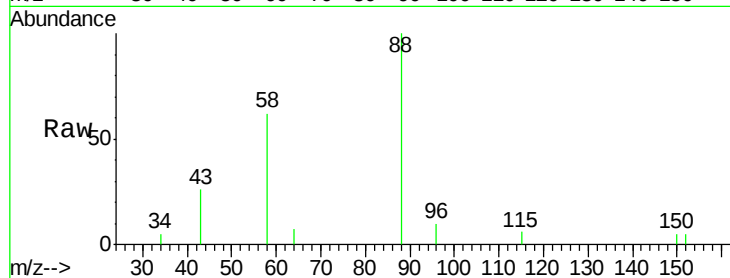

Abundance Ion 88.00 (87.70 to 88.70): BM004987.D (-41) (-)

Ion 58.00 (57.70 to 58.70): BM004987.D (-41) (-)

Ion 43.00 (42.70 to 43.70): BM004987.D (-41) (-)

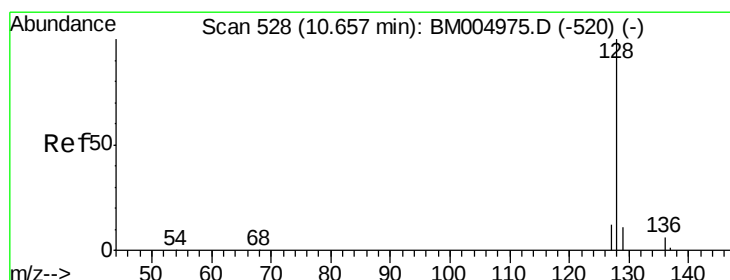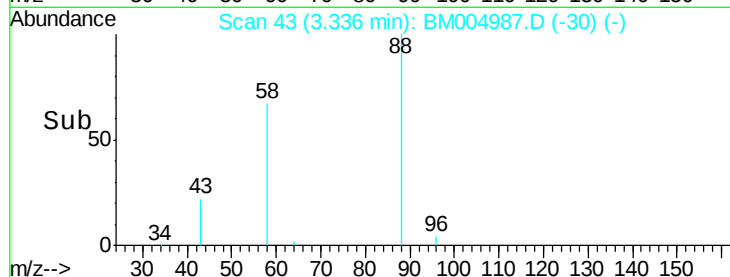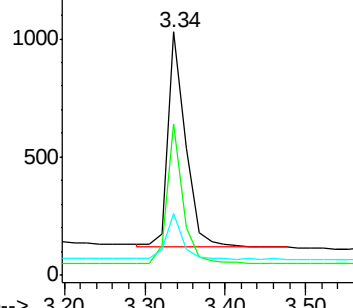

#5

Naphthalene

Concen: 0.41 ng/ul

RT: 10.66 min Scan# 528

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion: 128 Resp: 4372

Ion Ratio Lower Upper

128 100

129 13.3 9.0 13.6



127 14.6 9.6 14.4#

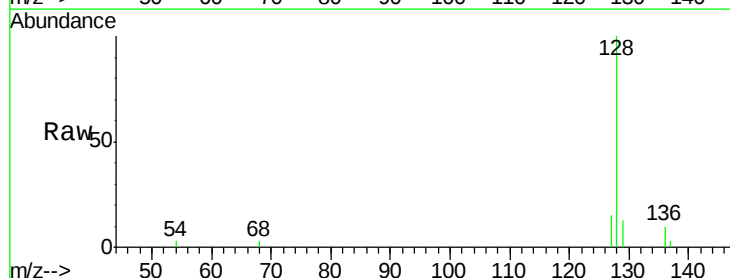


Abundance Ion 128.00 (127.70 to 128.70): BM004987.D (-511) (-)

Ion 129.00 (128.70 to 129.70): BM004987.D (-511) (-)

Ion 127.00 (126.70 to 127.70): BM004987.D (-511) (-)

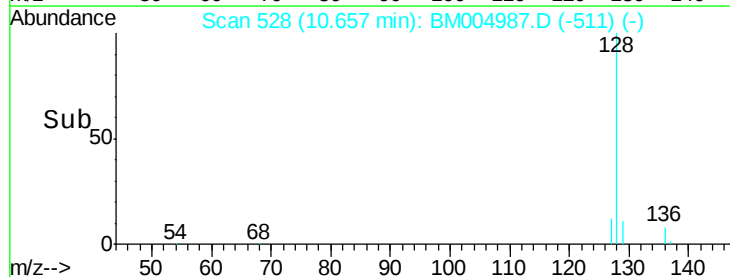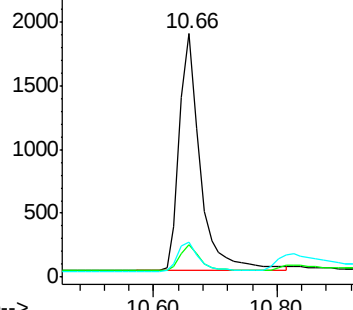

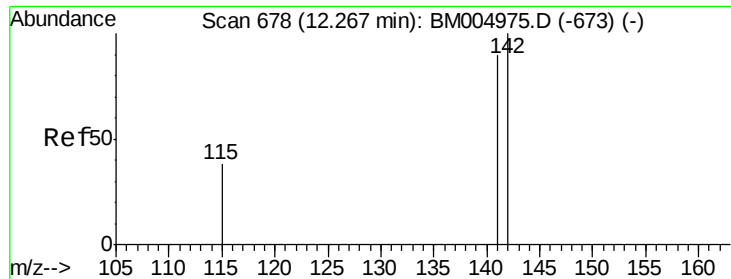

#7

2-Methylnaphthalene

Concen: 0.38 ng/ul

RT: 12.28 min Scan# 679

Delta R.T. 0.01 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :


SSTD0.460

Tot Ion:142 Resp: 2740

Ion Ratio Lower Upper

142 100

141 90.3 70.3 105.5

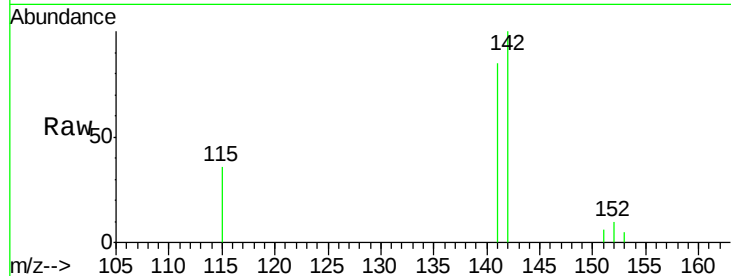

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

1200

1000

800

600



400

200

0

Time--> 12.20 12.30 12.40

12.28

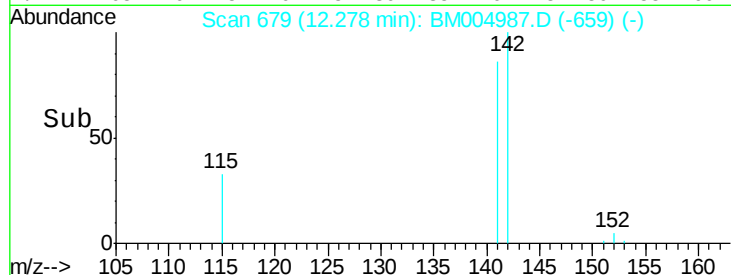

#9

Acenaphthylene

Concen: 0.39 ng/ul

RT: 14.16 min Scan# 854

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:152 Resp: 3511

Ion Ratio Lower Upper

152 100

151 22.1 17.6 26.4

153 14.7 9.7 14.5#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

2500

2000

1500


1000


500

0

Time--> 14.00 14.10 14.20 14.30

14.16





#10

Acenaphthene

Concen: 0.40 ng/ul

RT: 14.50 min Scan# 874

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:153 Resp: 2991

Ion Ratio Lower Upper

153 100

152 51.2 33.9 50.9#




154 84.2 80.6 121.0



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

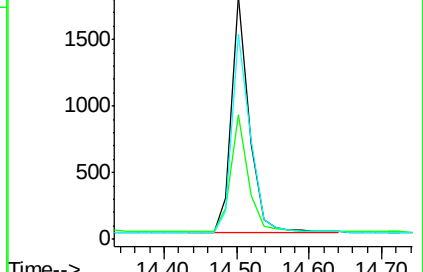

#11

Fluorene

Concen: 0.39 ng/ul

RT: 15.51 min Scan# 933

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:166 Resp: 3117

Ion Ratio Lower Upper

166 100

165 89.6 69.6 104.4



167 17.9 11.9 17.9#




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

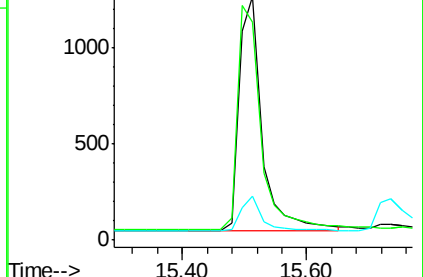


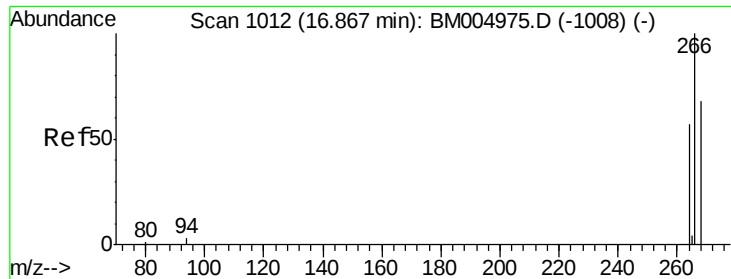


#13
 Pentachlorophenol
 Concen: 0.39 ng/ul
 RT: 16.87 min Scan# 1012
 Delta R.T. 0.00 min
 Lab File: BM004987.D
 Acq: 18 Apr 2016 23:47

Instrument :
 BNA_M
 ClientSampleId :
 SST0.460



Tot Ion:266 Resp: 204
 Ion Ratio Lower Upper
 266 100
 264 65.7 51.8 77.8
 268 64.7 46.8 70.2



Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

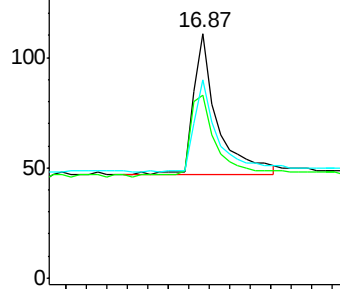


Time--> 16.60 16.80 17.00

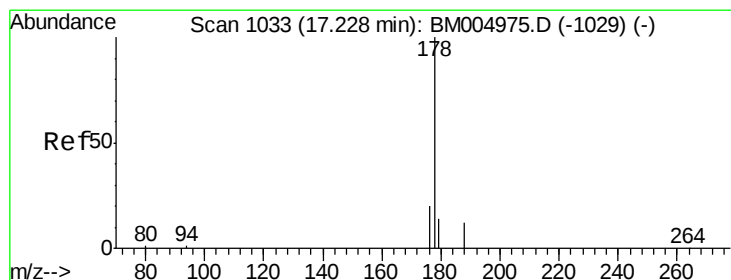


#14
 Phenanthrene
 Concen: 0.39 ng/ul
 RT: 17.23 min Scan# 1033
 Delta R.T. 0.00 min
 Lab File: BM004987.D
 Acq: 18 Apr 2016 23:47


Tgt Ion:178 Resp: 4771
 Ion Ratio Lower Upper
 178 100
 176 22.4 13.0 19.4#
 179 16.1 14.2 21.2




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

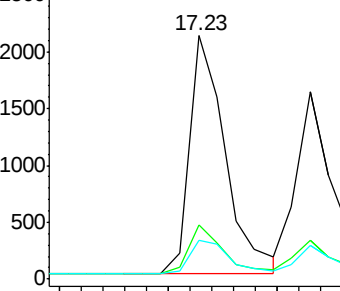

Time--> 17.10 17.20 17.30

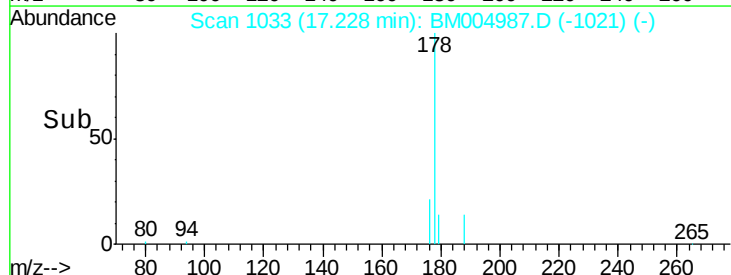

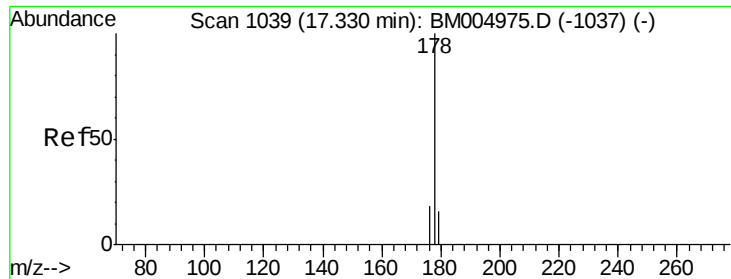

#15

Anthracene

Concen: 0.37 ng/ul

RT: 17.33 min Scan# 1039

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:178 Resp: 3890

Ion Ratio Lower Upper

178 100

176 20.8 14.0 21.0




179 17.8 12.9 19.3



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

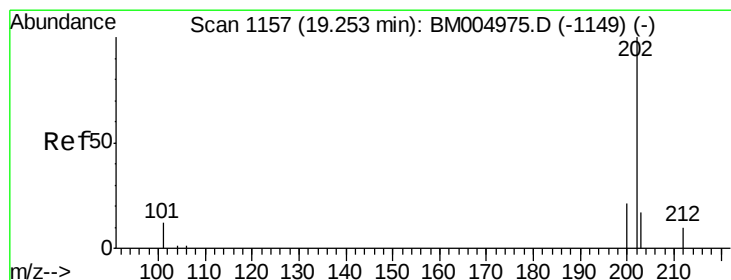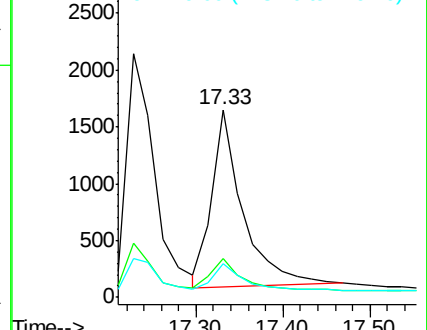

#17

Fluoranthene

Concen: 0.41 ng/ul

RT: 19.25 min Scan# 1157

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:202 Resp: 5162

Ion Ratio Lower Upper

202 100

101 13.4 0.0 29.6



203 18.5 0.0 36.3




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

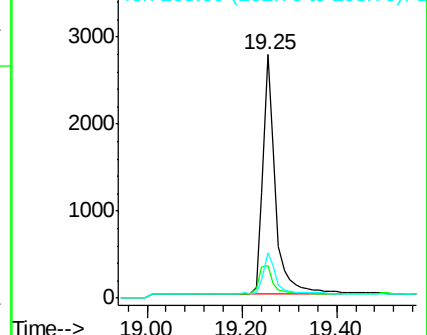



#19

Pvrene

Concen: 0.35 ng/ul

RT: 19.62 min Scan# 1187

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:202 Resp: 5329

Ion Ratio Lower Upper

202 100

200 22.2 17.8 26.8




203 18.0 12.8 19.2

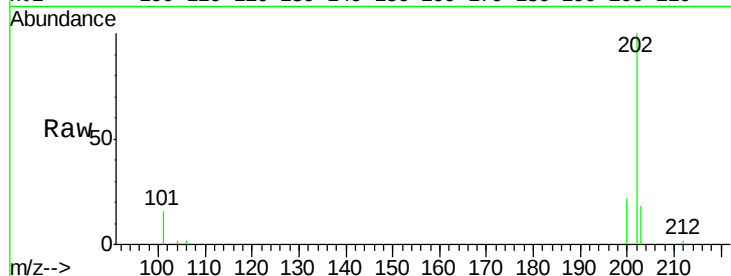

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

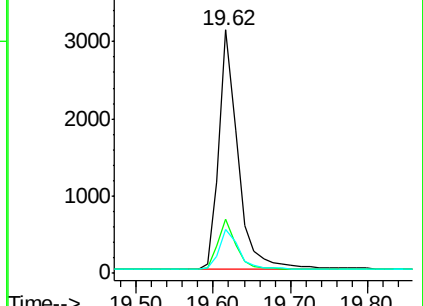

#20

Benzo(a)anthracene

Concen: 0.38 ng/ul

RT: 21.37 min Scan# 1343

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:228 Resp: 3760

Ion Ratio Lower Upper

228 100

226 27.4 18.8 28.2



229 22.0 17.1 25.7




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

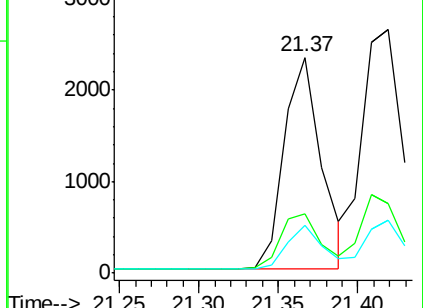



#21

Chrysene

Concen: 0.42 ng/ul

RT: 21.42 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:228 Resp: 5062

Ion Ratio Lower Upper

228 100

226 28.6 21.2 31.8




229 21.8 17.0 25.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

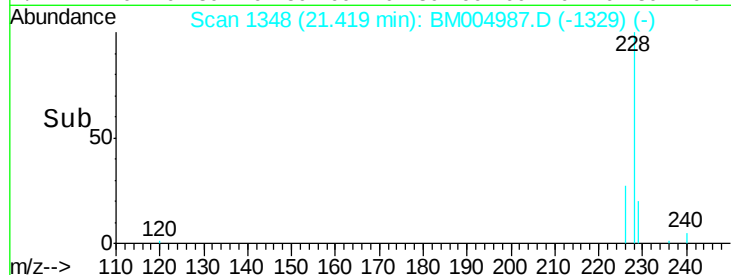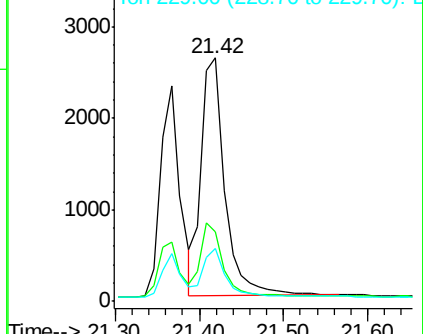

#23

Benzo(b)fluoranthene

Concen: 0.38 ng/ul

RT: 22.97 min Scan# 1497

Delta R.T. -0.01 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:252 Resp: 4013

Ion Ratio Lower Upper

252 100

253 26.4 0.0 45.4



125 19.0 0.0 28.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

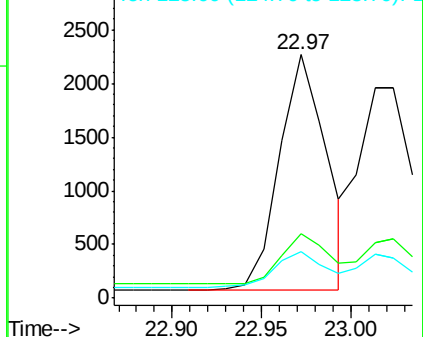

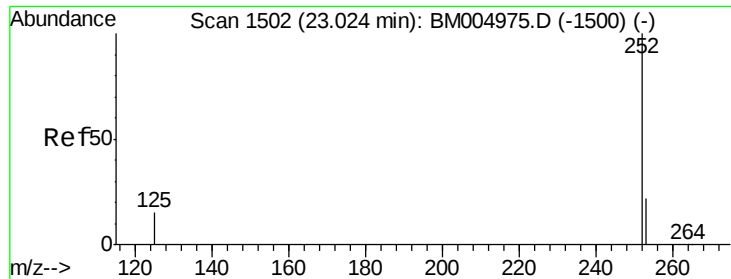

#24

Benzo(k)fluoranthene

Concen: 0.44 ng/ul

RT: 23.01 min Scan# 1501

Delta R.T. -0.01 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:252 Resp: 4470

Ion Ratio Lower Upper

252 100

253 26.2 19.8 29.8




125 20.6 10.4 15.6#

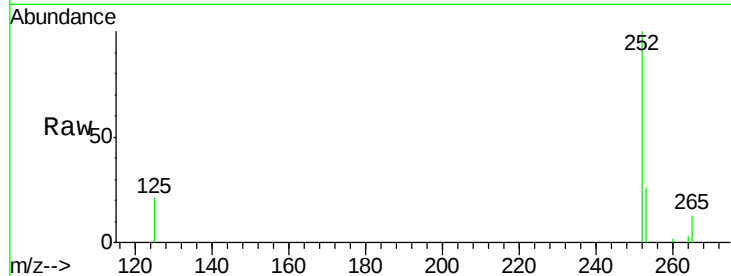

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

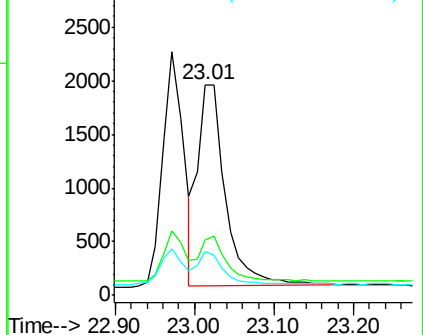

#25

Benzo(a)pyrene

Concen: 0.41 ng/ul

RT: 23.57 min Scan# 1554

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:252 Resp: 3717

Ion Ratio Lower Upper

252 100

253 29.5 19.4 29.2#



125 22.3 12.7 19.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

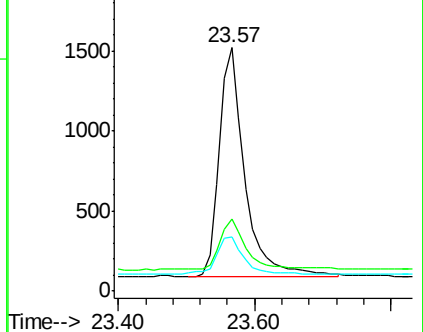

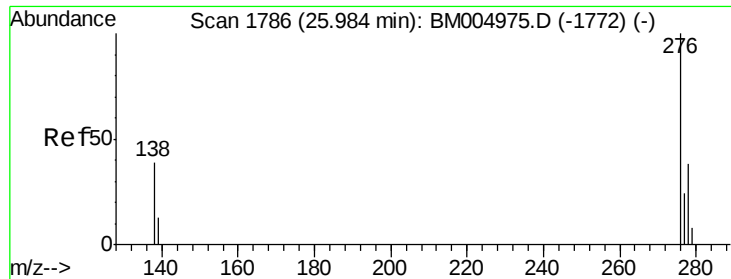

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.41 ng/ul

RT: 25.98 min Scan# 1786

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion:276 Resp: 3761

Ion Ratio Lower Upper

276 100

138 41.5 16.3 24.5#




277 24.7 19.8 29.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

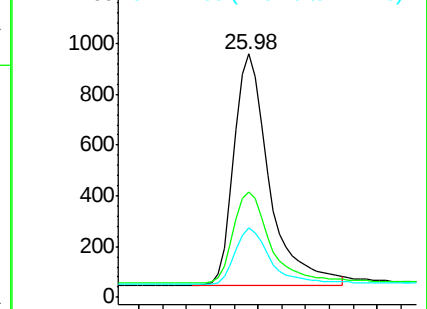

#27

Dibenzo(a,h)anthracene

Concen: 0.41 ng/ul

RT: 26.01 min Scan# 1788

Delta R.T. 0.00 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47


Tgt Ion:278 Resp: 2911

Ion Ratio Lower Upper

278 100

139 33.0 16.4 24.6#



279 31.1 20.2 30.2#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

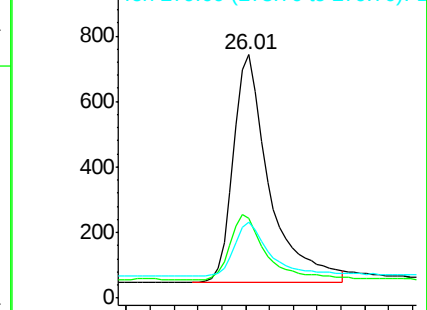



#28

Benzo(a,h,i)perylene

Concen: 0.41 ng/ul

RT: 26.68 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BM004987.D

Acq: 18 Apr 2016 23:47

Instrument :

BNA_M

ClientSampleId :

SSTD0.460


Tot Ion: 276 Resp: 3472

Ion Ratio Lower Upper

276 100

277 27.2 18.9 28.3



138 39.9 22.5 33.7



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

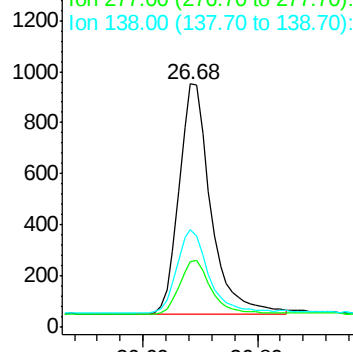

Time-->