

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041816\
 Data File : BM004980.D
 Acq On : 18 Apr 2016 19:31
 Operator : UM/SJ
 Sample : H2298-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T92

Manual Integrations
 APPROVED

Sohil
 4/19/2016 6:31:19 PM

Quant Time: Apr 27 13:01:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM041816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 19 08:25:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	1826	0.40	ng/ul	0.00
4) Naphthalene-d8	10.60	136	7587	0.40	ng/ul	-0.01
8) Acenaphthene-d10	14.45	164	3974	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.19	188	7410m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	6327	0.40	ng/ul	0.00
22) Perylene-d12	23.67	264	4109m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.31	96	3750	4.26	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.19	152	2634	0.29	ng/ul	0.00
16) Fluoranthene-d10	19.22	212	4841	0.32	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.65	128	658	0.04	ng/ul#	Qvalue 65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041816\
Data File : BM004980.D
Acq On : 18 Apr 2016 19:31
Operator : UM/SJ
Sample : H2298-09
Misc :
ALS Vial : 15 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
D9T92

Manual Integrations
APPROVED

Sohil
4/19/2016 6:31:19 PM

Quant Time: Apr 27 13:01:01 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM041816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 19 08:25:48 2016
Response via : Initial Calibration

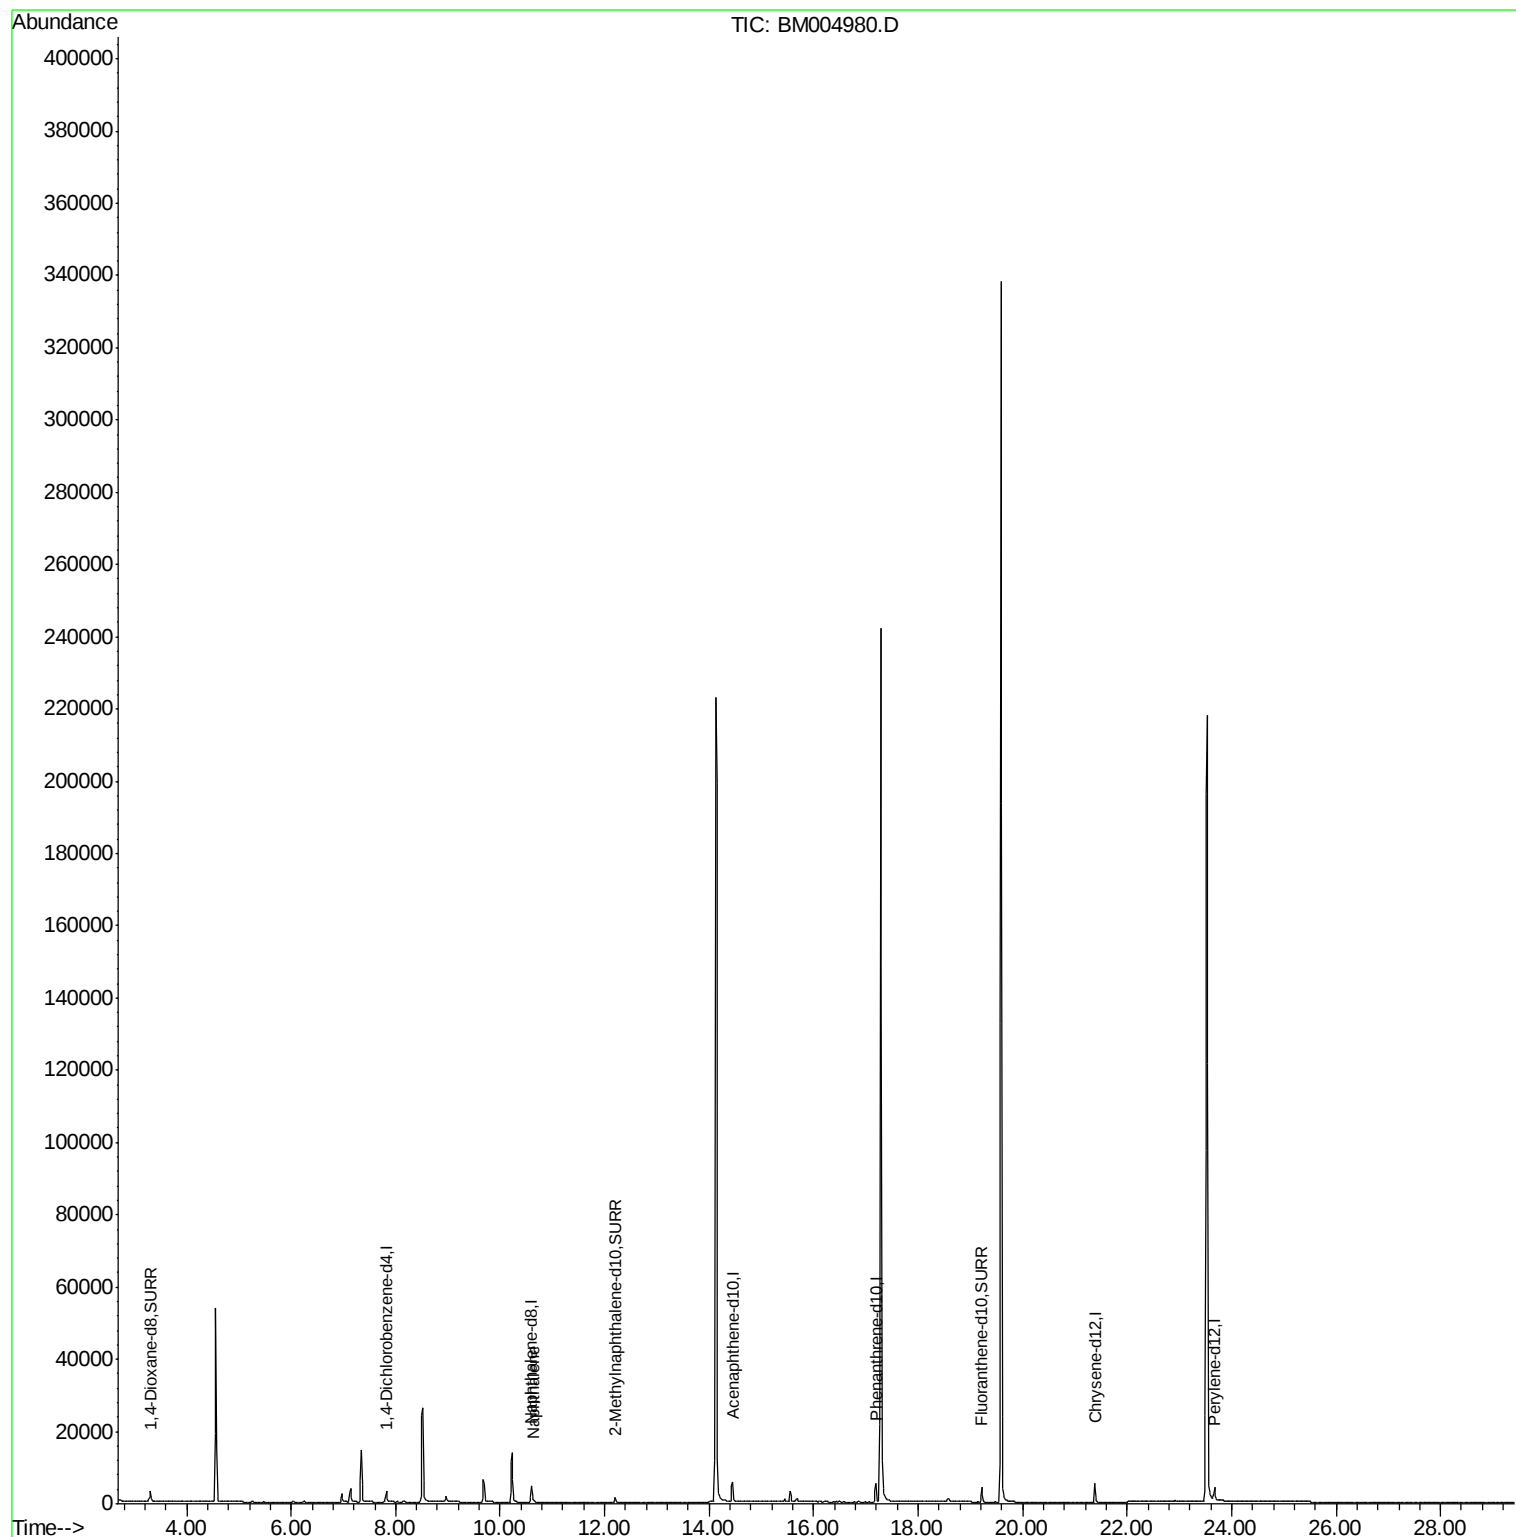

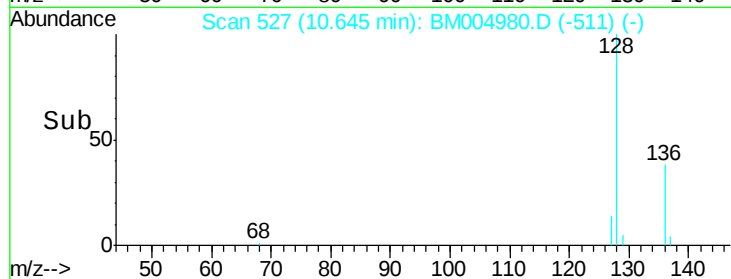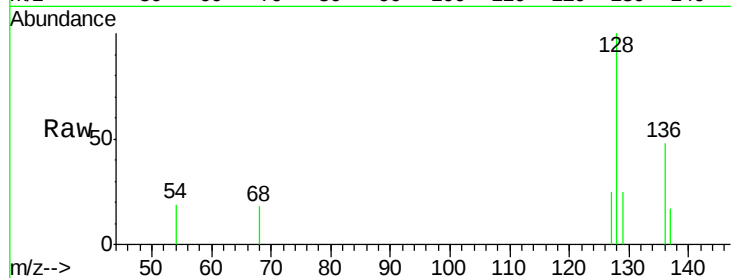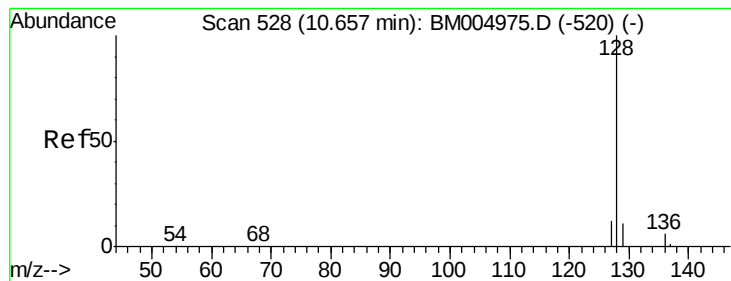

#5

Naphthalene

Concen: 0.04 ng/ul

RT: 10.65 min Scan# 527

Delta R.T. -0.01 min

Lab File: BM004980.D

Acq: 18 Apr 2016 19:31

Tgt Ion:	128	Resp:	658
Ion Ratio	Lower	Upper	
128	100		
129	25.4	9.0	13.6#
127	25.1	9.6	14.4#

Instrument :

BNA_M

ClientSampleId :

D9T92

Manual Integrations
APPROVED

Sohil
4/19/2016 6:31:19 PM

