


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041817\
 Data File : BM009657.D
 Acq On : 18 Apr 2017 15:38
 Operator : SJ/MA
 Sample : DFTPP02
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP02

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041717.M
 Title : SVOA CALIBRATION
 Last Update : Wed Apr 19 10:29:34 2017

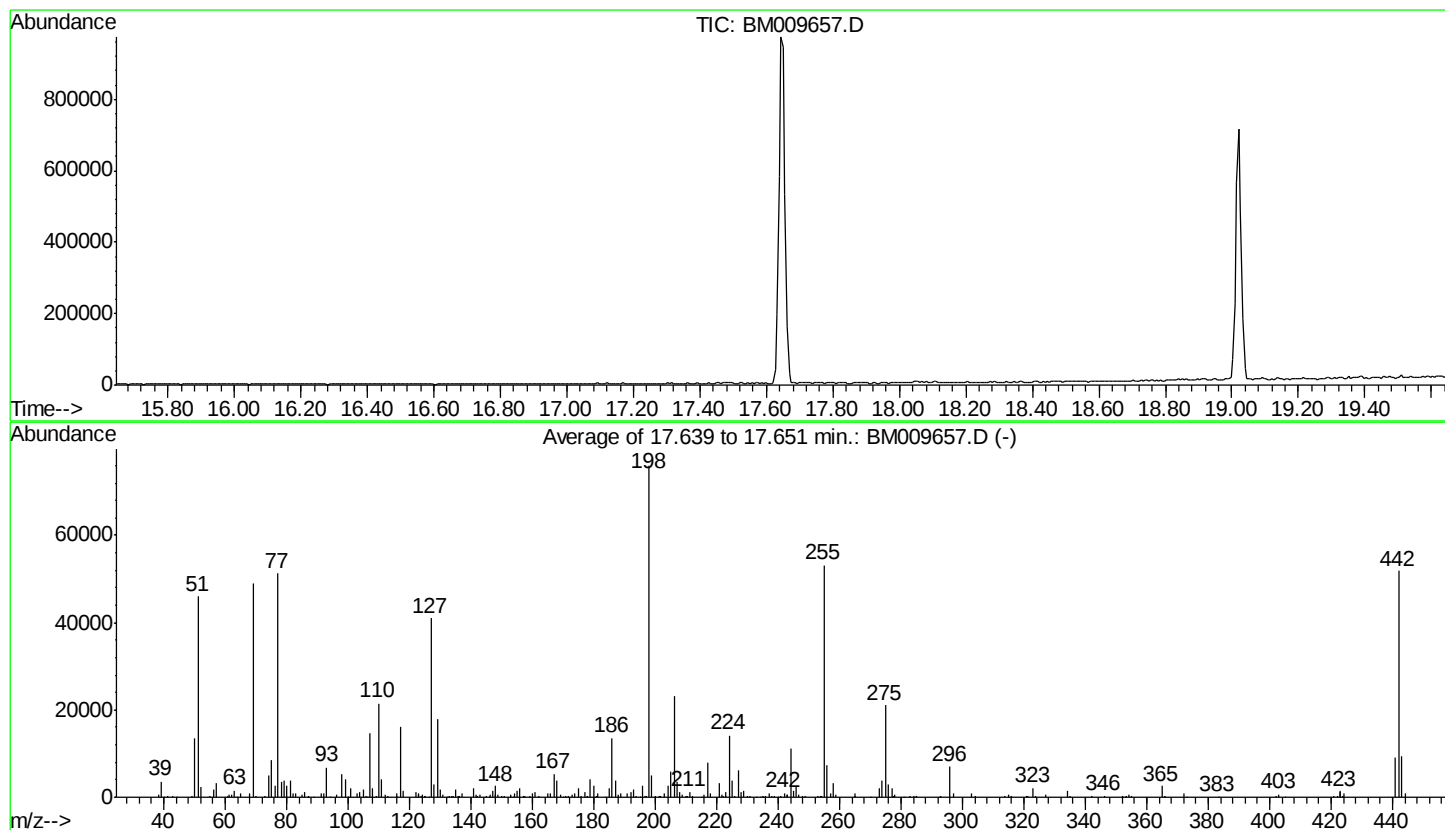

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	45949	PASS
68	69	0.00	2	1.8	888	PASS
69	198	0.00	100	64.6	49064	PASS
70	69	0.00	2	0.6	295	PASS
127	198	10	80	53.9	40957	PASS
197	198	0.00	2	0.4	304	PASS
198	198	100	100	100.0	75973	PASS
199	198	5	9	6.6	4997	PASS
275	198	10	60	27.7	21073	PASS
365	198	1	100	3.4	2587	PASS
441	443	0.01	100	96.6	9025	PASS
442	198	50	100	68.3	51909	PASS
443	442	15	24	18.0	9338	PASS

m/z	Abundance
38.10	547.0
39.00	2834.0
39.90	375.0
44.10	701.0
49.00	516.0
50.00	11013.0
51.10	38904.0
52.10	2415.0
56.00	2037.0
57.10	3022.0
61.10	880.0
62.00	512.0
63.10	1285.0
65.00	679.0
68.10	833.0
69.00	40232.0
73.20	996.0
74.00	3424.0
75.00	6744.0
76.10	1949.0
77.10	38712.0
78.20	2825.0
79.00	3189.0
79.90	1627.0
81.00	2996.0
82.10	954.0
83.10	744.0
84.90	625.0
85.90	927.0
86.90	335.0
91.10	1053.0
92.10	450.0
93.00	4854.0
98.00	4286.0
99.00	3323.0
101.00	1358.0
103.00	707.0
103.90	1413.0
104.90	1715.0
107.00	12071.0
108.00	1895.0
109.00	363.0
110.00	16968.0
111.00	2866.0
111.90	435.0
113.00	320.0
115.70	362.0
116.90	11382.0
117.90	1261.0
122.10	462.0
122.90	1265.0
123.90	469.0
124.80	393.0
127.00	30944.0
128.00	2294.0
129.00	14065.0
130.00	1368.0
131.00	302.0
132.90	345.0
134.00	335.0
135.00	1093.0
136.10	616.0
137.00	741.0
141.00	1759.0
141.90	347.0
143.00	585.0
146.20	396.0
147.00	1227.0
147.80	1906.0
149.10	389.0
150.00	453.0
150.90	384.0
152.80	628.0
153.70	462.0
154.10	412.0
155.00	971.0
156.00	1019.0
157.00	753.0
160.00	814.0
161.00	674.0
162.00	510.0
164.80	643.0
166.00	571.0
167.00	3969.0
168.00	3247.0
169.10	556.0
173.00	564.0
173.90	924.0
175.00	1968.0
176.90	747.0
177.50	302.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

179.00	3700.0
179.90	2121.0
180.80	670.0
185.00	1261.0
186.00	9105.0
187.00	2186.0
188.90	382.0
190.90	583.0
192.00	494.0
193.10	1064.0
195.90	1275.0
197.90	53360.0
198.90	4122.0
201.80	306.0
203.00	349.0
204.00	1756.0
205.00	4670.0
206.10	15420.0
207.00	3683.0
207.90	402.0
208.90	493.0
210.40	776.0
211.00	524.0
216.00	648.0
217.00	4261.0
217.90	454.0
221.00	2417.0
222.90	1284.0
224.00	8193.0
225.00	2984.0
226.10	374.0
227.00	4064.0
228.00	752.0
228.90	712.0
234.90	470.0
236.90	528.0
238.80	391.0
242.00	576.0
242.90	870.0
244.00	7416.0
245.10	1538.0
245.90	1645.0
253.90	515.0
255.00	34328.0
256.00	4475.0
257.00	819.0
258.00	2449.0
258.90	393.0
264.80	1160.0
272.90	1171.0
273.90	1621.0
275.00	14187.0
276.00	2380.0
276.90	1691.0
278.00	566.0
292.70	305.0
296.00	4150.0
296.90	432.0
303.00	414.0
322.90	1105.0
326.80	372.0
334.00	913.0
353.90	444.0
365.00	1764.0
372.00	875.0
403.00	375.0
423.00	883.0
423.90	651.0
441.00	4288.0
442.10	25208.0
443.10	4958.0
444.10	504.0

Instrument :

BNA_M

ClientSampleId :

DFTPP02

m/z	Abundance
38.10	762.0
39.00	4276.0
40.00	984.0
43.10	443.0
43.90	750.0
49.00	806.0
50.00	15885.0
51.10	54400.0
52.00	2168.0
54.90	456.0
56.10	2033.0
57.00	3196.0
61.00	553.0
62.10	563.0
63.10	1700.0
65.10	1404.0
68.00	1162.0
69.00	59744.0
70.20	552.0
73.10	1618.0
74.00	6678.0
75.00	10850.0
76.00	3237.0
77.10	59536.0
78.10	4330.0
79.00	5104.0
79.90	3714.0
81.10	4548.0
81.90	1051.0
83.10	898.0
85.00	581.0
86.00	1039.0
87.10	761.0
91.10	1043.0
92.10	857.0
93.00	8281.0
94.20	320.0
96.00	781.0
98.00	6151.0
99.00	4775.0
100.00	401.0
100.90	3451.0
102.90	1232.0
103.80	1025.0
105.00	1737.0
105.80	606.0
107.00	18024.0
108.00	3249.0
110.00	25056.0
111.00	5299.0
112.00	681.0
113.10	313.0
116.00	1615.0
117.00	19296.0
118.00	1846.0
122.00	1801.0
122.70	1481.0
124.10	958.0
124.80	723.0
126.20	462.0
127.00	48504.0
128.10	4067.0
129.00	20680.0
130.00	1987.0
131.00	480.0
132.70	434.0
134.10	589.0
134.90	2131.0
135.70	325.0
136.20	520.0
137.00	904.0
141.00	2566.0
141.80	725.0
142.20	613.0
143.00	541.0
146.10	786.0
146.90	1611.0
148.00	3749.0
149.00	1361.0
149.90	391.0
151.00	661.0
153.00	634.0
154.00	987.0
154.90	1738.0
155.90	2776.0
156.80	507.0
157.70	673.0
159.00	674.0
159.90	1386.0
161.10	1536.0
162.10	395.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

164.90	1527.0
165.80	1106.0
166.90	7052.0
168.00	3816.0
169.00	549.0
170.80	365.0
171.80	469.0
173.00	778.0
173.90	987.0
175.10	1891.0
176.00	671.0
177.00	1208.0
177.90	302.0
178.90	4224.0
180.00	2966.0
181.10	1223.0
183.80	341.0
185.00	1853.0
186.00	14383.0
186.90	4089.0
187.90	574.0
189.00	879.0
190.90	1016.0
191.90	1984.0
193.00	2383.0
193.90	323.0
194.90	392.0
196.00	3248.0
197.00	912.0
198.00	90192.0
198.90	4639.0
200.00	625.0
201.00	347.0
201.80	339.0
202.80	1367.0
203.90	3112.0
205.00	6579.0
206.00	27216.0
207.00	5309.0
207.90	1664.0
209.00	348.0
209.90	1009.0
211.10	1495.0
212.00	372.0
215.10	382.0
215.80	896.0
216.90	9684.0
217.90	985.0
220.90	3812.0
222.10	696.0
223.10	1603.0
224.00	16440.0
224.90	3649.0
225.90	433.0
227.00	6853.0
227.90	1353.0
228.90	1421.0
229.90	322.0
231.10	333.0
235.10	422.0
236.10	477.0
237.00	881.0
237.90	310.0
238.80	340.0
241.00	530.0
241.80	1120.0
243.10	766.0
244.10	12470.0
245.10	1572.0
245.90	2512.0
246.90	962.0
248.00	507.0
248.70	444.0
254.10	371.0
255.00	59336.0
256.00	8790.0
257.00	651.0
258.00	3433.0
259.00	797.0
265.00	1463.0
272.90	2020.0
274.00	4602.0
275.00	25536.0
276.00	3113.0
276.90	2082.0
277.70	618.0
280.90	387.0
283.00	577.0
284.00	444.0
284.90	510.0
296.00	8087.0
297.00	1222.0
303.00	1141.0
304.10	477.0
313.90	384.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

315.10	672.0
315.80	361.0
320.90	514.0
323.00	2726.0
326.90	662.0
334.00	1156.0
335.10	539.0
346.10	531.0
352.20	378.0
353.20	495.0
354.00	754.0
354.90	622.0
364.90	2507.0
365.80	466.0
371.90	668.0
372.90	368.0
383.20	444.0
402.00	467.0
403.00	671.0
422.00	320.0
422.90	3149.0
424.10	1027.0
441.00	9653.0
442.10	57464.0
443.00	10054.0
444.00	955.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
38.20	562.0
39.00	3463.0
40.00	610.0
41.10	468.0
43.10	382.0
44.00	779.0
50.10	13524.0
51.10	44544.0
52.00	2487.0
55.00	304.0
56.00	1249.0
57.00	3284.0
60.80	741.0
62.00	906.0
63.10	1610.0
63.90	317.0
65.00	1003.0
67.90	670.0
69.00	47216.0
70.20	333.0
73.00	1229.0
74.10	5002.0
75.00	7569.0
76.00	2858.0
77.10	56624.0
78.10	3576.0
79.00	3411.0
80.00	2962.0
81.00	4016.0
81.90	619.0
83.00	779.0
85.10	585.0
86.10	1208.0
88.90	415.0
91.00	560.0
91.90	1113.0
92.90	7138.0
96.10	773.0
98.00	5644.0
99.00	4392.0
100.20	370.0
100.90	1734.0
103.00	305.0
104.00	1205.0
104.90	1465.0
106.10	353.0
107.00	14169.0
108.00	1328.0
109.00	513.0
110.00	22496.0
110.90	4539.0
111.90	590.0
116.00	928.0
117.00	18128.0
118.10	1447.0
121.90	921.0
123.00	2126.0
124.00	862.0
125.00	620.0
127.00	43424.0
128.00	2410.0
129.00	19224.0
130.00	2027.0
130.90	624.0
132.00	328.0
133.80	615.0
134.90	1819.0
135.90	694.0
136.90	1018.0
140.90	2290.0
141.80	416.0
142.90	829.0
145.00	540.0
145.80	375.0
146.10	445.0
147.00	2563.0
148.00	3835.0
148.80	462.0
152.90	938.0
154.00	996.0
154.90	1897.0
156.00	2356.0
160.00	681.0
160.90	1321.0
164.70	648.0
166.00	1055.0
166.90	5155.0
168.00	4809.0
169.20	424.0
170.10	320.0
170.80	336.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

173.00	659.0
173.90	930.0
175.00	2358.0
175.80	397.0
177.00	1267.0
178.00	550.0
178.90	4059.0
180.00	3000.0
181.10	1649.0
184.80	1337.0
185.10	1543.0
186.00	17128.0
187.00	5149.0
188.00	829.0
188.80	1281.0
191.00	1057.0
191.90	1276.0
193.00	2285.0
194.00	499.0
196.00	3160.0
196.70	807.0
198.00	84368.0
198.90	6232.0
200.00	583.0
201.10	465.0
201.60	400.0
202.90	1189.0
204.10	3325.0
205.10	6575.0
206.00	26552.0
207.00	6066.0
207.90	1776.0
209.00	721.0
210.20	553.0
211.00	1714.0
211.80	305.0
217.00	9602.0
217.90	998.0
221.10	3467.0
221.80	1397.0
223.00	2382.0
224.00	18064.0
225.10	4782.0
226.00	430.0
226.90	7739.0
227.90	1210.0
228.90	1952.0
229.90	413.0
230.90	608.0
232.90	424.0
234.00	450.0
234.90	677.0
235.90	649.0
237.00	1047.0
237.90	321.0
238.70	332.0
240.00	386.0
240.90	738.0
242.00	1118.0
242.80	659.0
243.10	736.0
244.00	13744.0
244.90	1475.0
245.90	2891.0
246.80	795.0
248.80	500.0
252.80	671.0
254.10	935.0
255.00	65600.0
256.00	8390.0
256.90	887.0
258.00	4101.0
258.90	821.0
265.00	1463.0
270.00	339.0
273.00	2609.0
274.00	4924.0
275.00	23496.0
276.00	3054.0
276.90	2594.0
278.00	933.0
284.10	334.0
285.10	725.0
292.90	670.0
296.00	8599.0
296.90	931.0
302.90	1385.0
304.00	461.0
313.90	566.0
314.90	1449.0
316.00	575.0
321.10	626.0
323.00	2428.0
323.90	636.0
327.00	377.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

334.00	1961.0
335.00	367.0
341.90	540.0
346.00	685.0
351.90	964.0
352.90	356.0
354.10	756.0
364.90	3491.0
366.00	983.0
372.10	972.0
401.80	542.0
403.00	880.0
405.10	319.0
421.00	477.0
422.10	451.0
423.10	3281.0
424.10	1501.0
441.00	13135.0
442.00	73056.0
443.10	13004.0
443.90	1140.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

Scan 2470 (17.615 min): BM009657.D
DFTPP02

m/z	Abundance
39.90	645.0
44.10	737.0
72.90	965.0
76.90	336.0
146.90	340.0
206.90	1478.0
282.00	343.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02