

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041823\  
 Data File : BM039461.D  
 Acq On : 18 Apr 2023 17:15  
 Operator : CG/JU  
 Sample : 02299-03  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AE7

Quant Time: Apr 19 00:14:16 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Apr 18 23:56:45 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.834  | 152  | 202078   | 20.000 | ng/u1 | 0.00     |
| 20) Naphthalene-d8            | 10.640 | 136  | 931440   | 20.000 | ng/u1 | 0.00     |
| 38) Acenaphthene-d10          | 14.492 | 164  | 627828   | 20.000 | ng/u1 | 0.00     |
| 64) Phenanthrene-d10          | 17.239 | 188  | 1353844  | 20.000 | ng/u1 | 0.00     |
| 79) Chrysene-d12              | 21.433 | 240  | 1093571  | 20.000 | ng/u1 | 0.00     |
| 88) Perylene-d12              | 23.809 | 264  | 968139   | 20.000 | ng/u1 | 0.00     |
|                               |        |      |          |        |       |          |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.217  | 96   | 21927    | 4.165  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.640  | 84   | 742      | 0.050  | ng/u1 | 0.00     |
| 7) Phenol-d5                  | 7.028  | 99   | 105863   | 5.724  | ng/u1 | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.169  | 67   | 342930   | 28.052 | ng/u1 | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.369  | 132  | 322753   | 22.246 | ng/u1 | 0.00     |
| 15) 4-Methylphenol-d8         | 8.569  | 113  | 201688   | 13.538 | ng/u1 | 0.00     |
| 21) Nitrobenzene-d5           | 9.004  | 128  | 211543   | 28.230 | ng/u1 | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.728  | 143  | 227151   | 26.995 | ng/u1 | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.281 | 165  | 343931   | 23.754 | ng/u1 | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.822 | 131  | 13227    | 0.612  | ng/u1 | 0.03     |
| 46) Dimethylphthalate-d6      | 13.904 | 166  | 1737882  | 34.323 | ng/u1 | 0.00     |
| 49) Acenaphthylene-d8         | 14.181 | 160  | 1748023  | 30.730 | ng/u1 | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.751 | 143  | 7740     | 1.010  | ng/u1 | 0.02     |
| 60) Fluorene-d10              | 15.486 | 176  | 1451302  | 34.985 | ng/u1 | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.616 | 200  | 277679   | 30.864 | ng/u1 | 0.00     |
| 73) Anthracene-d10            | 17.339 | 188  | 2452745  | 37.671 | ng/u1 | 0.00     |
| 81) Pyrene-d10                | 19.639 | 212  | 2790499  | 38.401 | ng/u1 | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.656 | 264  | 1979557  | 37.873 | ng/u1 | 0.00     |
|                               |        |      |          |        |       |          |
| Target Compounds              |        |      |          |        |       | Qvalue   |
| 2) 1,4-Dioxane                | 3.252  | 88   | 145246   | 25.211 | ng/uL | 96       |
| -----                         |        |      |          |        |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041823\  
Data File : BM039461.D  
Acq On : 18 Apr 2023 17:15  
Operator : CG/JU  
Sample : 02299-03  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0AE7

Quant Time: Apr 19 00:14:16 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Apr 18 23:56:45 2023  
Response via : Initial Calibration

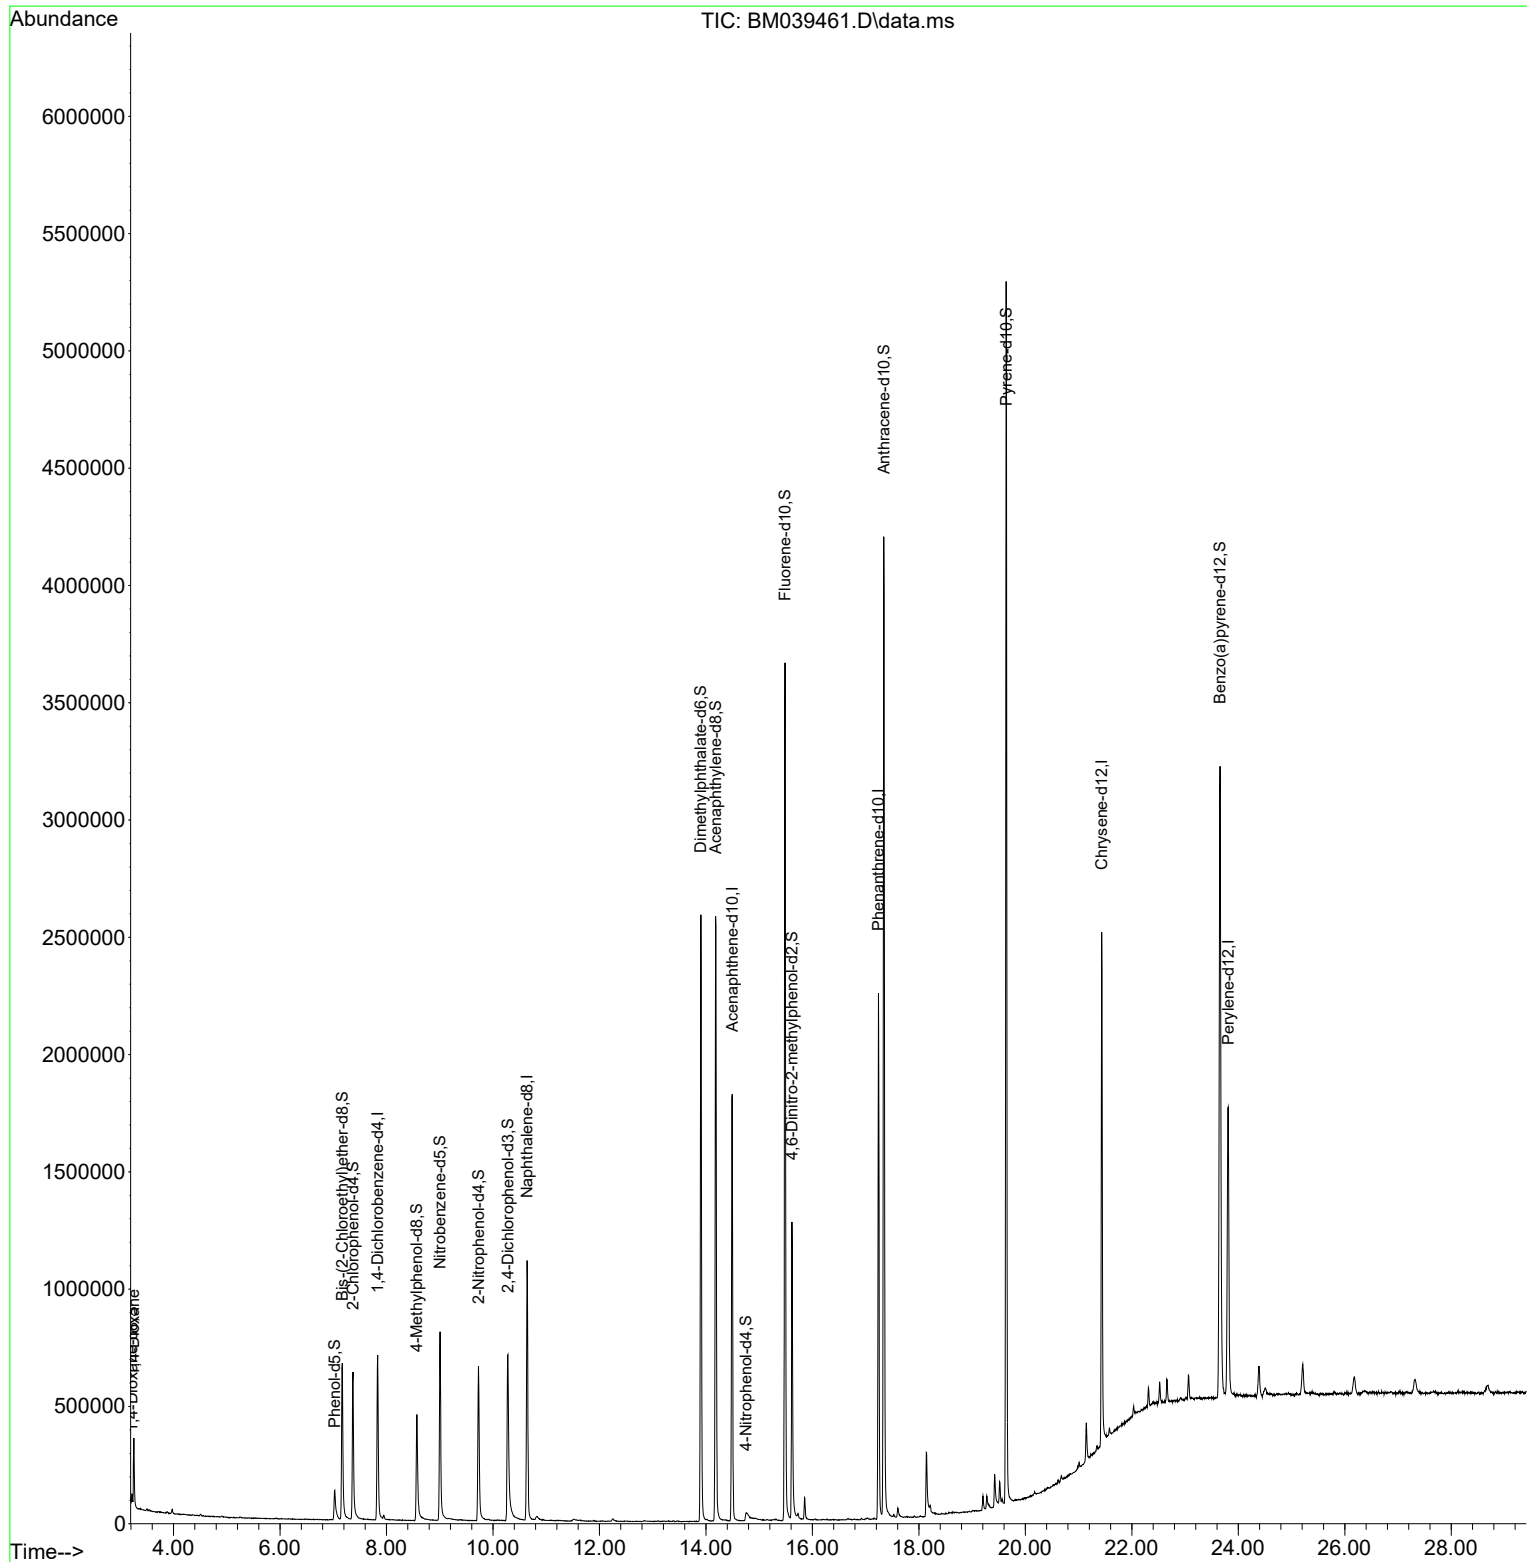

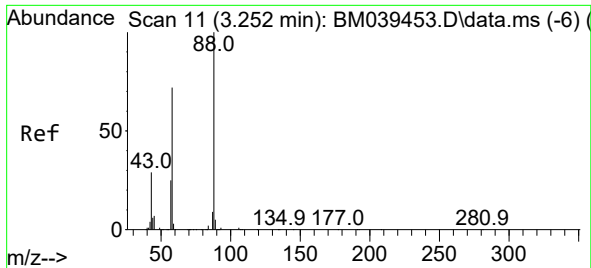

1,4-Dioxane

Concen: 25.211 ng/uL

RT: 3.252 min Scan# 11

Delta R.T. -0.000 min

Lab File: BM039461.D

Acq: 18 Apr 2023 17:15

Instrument :

BNA\_M

ClientSampleId :

C0AE7

Tgt Ion: 88 Resp: 145246

Ion Ratio Lower Upper

88 100

43 29.3 24.6 36.8

58 74.1 56.7 85.1

