

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039460.D
 Acq On : 18 Apr 2023 16:39
 Operator : CG/JU
 Sample : 02299-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	8	rVB	34436	30705	0.45%	0.053%
2	3.252	8	11	27	rVB	397790	543920	7.96%	0.946%
3	3.975	131	134	139	rVB	16292	22073	0.32%	0.038%
4	4.505	221	224	233	rVB	15087	24532	0.36%	0.043%
5	7.028	646	653	670	rBV	128588	298098	4.36%	0.519%
6	7.169	670	677	696	rBV	719790	1257257	18.41%	2.187%
7	7.369	704	711	732	rBV	656706	1203527	17.62%	2.094%
8	7.834	783	790	804	rBV	636424	1113682	16.31%	1.937%
9	7.946	805	809	819	rVB	51474	92011	1.35%	0.160%
10	8.569	906	915	933	rBV	452253	942062	13.79%	1.639%
11	9.004	981	989	1001	rBV	861373	1533342	22.45%	2.667%
12	9.398	1052	1056	1061	rVB	11193	17861	0.26%	0.031%
13	9.728	1105	1112	1137	rBV	700782	1319921	19.33%	2.296%
14	10.275	1199	1205	1238	rBV	736159	1752130	25.66%	3.048%
15	10.640	1259	1267	1279	rBV	992175	1759550	25.76%	3.061%
16	10.834	1293	1300	1303	rBV4	7706	19072	0.28%	0.033%
17	11.892	1475	1480	1486	rBV2	13262	22025	0.32%	0.038%
18	12.251	1535	1541	1547	rBV3	12147	27571	0.40%	0.048%
19	13.222	1700	1706	1709	rBV5	5551	8546	0.13%	0.015%
20	13.904	1815	1822	1838	rBV	2406188	3544381	51.90%	6.165%
21	14.010	1838	1840	1851	rVB9	7439	16812	0.25%	0.029%
22	14.186	1860	1870	1900	rBV	2651674	4131685	60.50%	7.187%
23	14.386	1900	1904	1910	rVB6	5579	9325	0.14%	0.016%
24	14.492	1915	1922	1940	rVV	1688782	2594772	37.99%	4.514%
25	14.769	1961	1969	1970	rBV4	23084	46130	0.68%	0.080%
26	15.239	2046	2049	2053	rBV	6969	8209	0.12%	0.014%
27	15.333	2062	2065	2070	rVB5	7237	9378	0.14%	0.016%
28	15.486	2082	2091	2108	rBV	3489068	5145528	75.34%	8.951%
29	15.616	2108	2113	2128	rVV	1043391	1694012	24.80%	2.947%
30	15.727	2129	2132	2139	rVB3	19022	34775	0.51%	0.060%
31	15.857	2149	2154	2165	rVB	51723	83603	1.22%	0.145%
32	16.063	2184	2189	2193	rVB7	6210	11624	0.17%	0.020%
33	16.204	2209	2213	2217	rBV6	4991	8193	0.12%	0.014%
34	17.033	2351	2354	2360	rVB5	5657	8963	0.13%	0.016%
35	17.163	2373	2376	2380	rVB5	5315	6900	0.10%	0.012%
36	17.239	2383	2389	2400	rBV	2091961	3103952	45.45%	5.399%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039460.D
 Acq On : 18 Apr 2023 16:39
 Operator : CG/JU
 Sample : 02299-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.339	2400	2406	2426	rVB2	3790539	5755621	84.28%	10.012%
38	17.527	2435	2438	2445	rVB2	18084	27409	0.40%	0.048%
39	18.139	2538	2542	2551	rBV	130608	270740	3.96%	0.471%
40	18.210	2552	2554	2559	rVB	28078	41666	0.61%	0.072%
41	18.427	2588	2591	2594	rBV5	5001	7668	0.11%	0.013%
42	19.204	2719	2723	2730	rBV4	54761	91998	1.35%	0.160%
43	19.280	2731	2736	2743	rBV	44955	94113	1.38%	0.164%
44	19.427	2756	2761	2772	rBV2	84514	206147	3.02%	0.359%
45	19.563	2782	2784	2788	rVB4	18931	20089	0.29%	0.035%
46	19.639	2791	2797	2815	rBV	4809814	6829563	100.00%	11.880%
47	21.145	3050	3053	3057	rBV5	65613	100561	1.47%	0.175%
48	21.433	3098	3102	3116	rBV	2169711	3156788	46.22%	5.491%
49	23.656	3473	3480	3493	rBV2	2779365	5637224	82.54%	9.806%
50	23.809	3499	3506	3516	rVB2	1337084	2802191	41.03%	4.874%




Sum of corrected areas: 57487905

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039460.D
Acq On : 18 Apr 2023 16:39
Operator : CG/JU
Sample : 02299-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

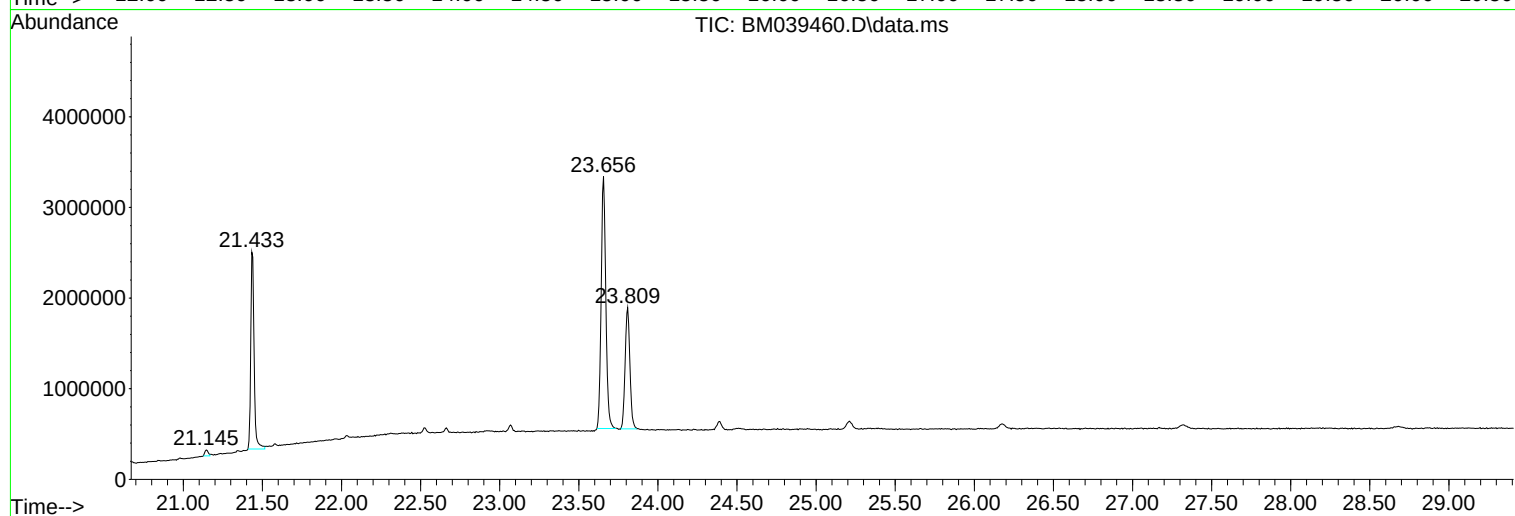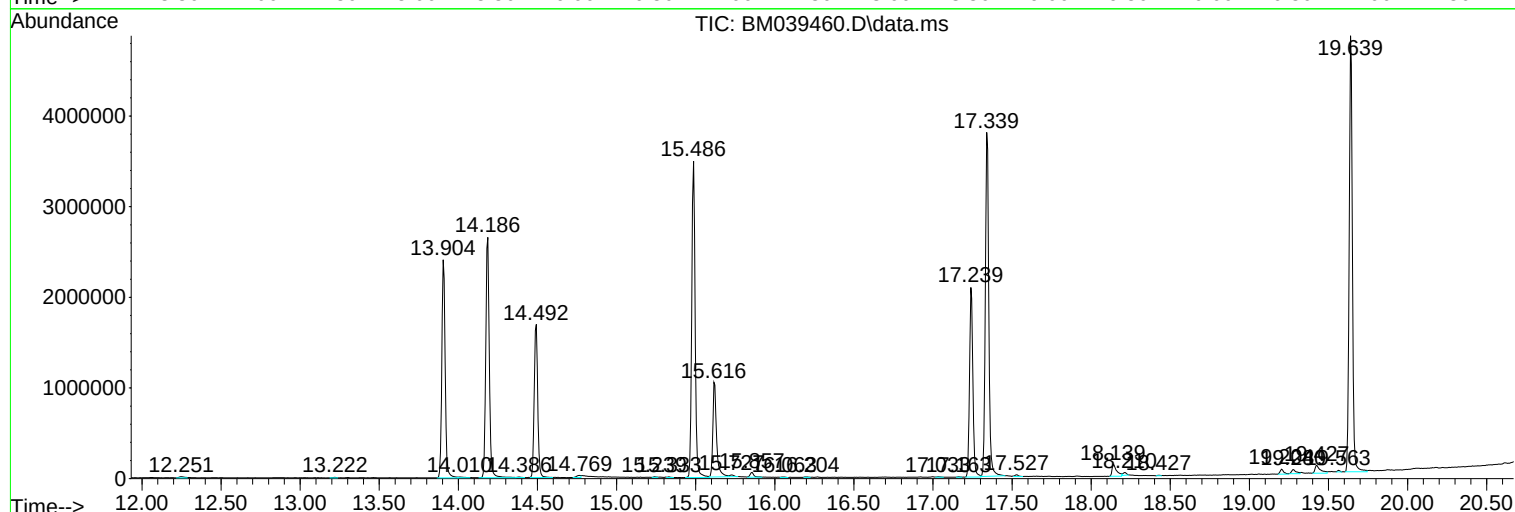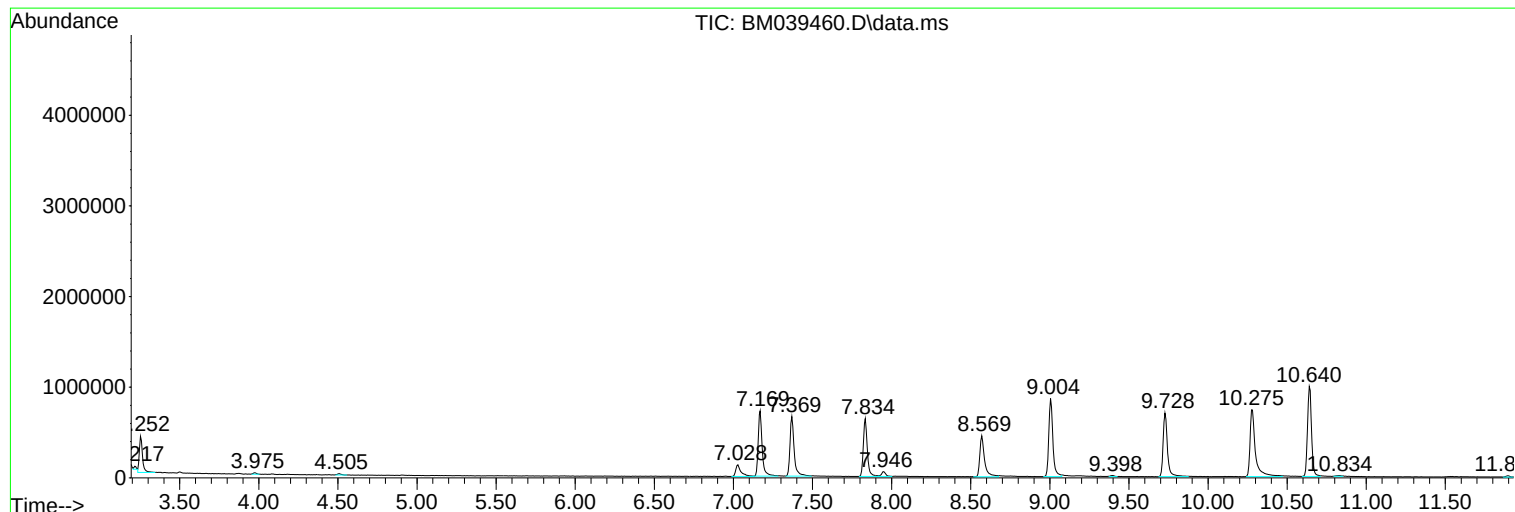

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039460.D
Acq On : 18 Apr 2023 16:39
Operator : CG/JU
Sample : 02299-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039460.D
Acq On : 18 Apr 2023 16:39
Operator : CG/JU
Sample : 02299-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------