

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039462.D
 Acq On : 18 Apr 2023 17:51
 Operator : CG/JU
 Sample : 02299-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	9	rBV	38624	47729	0.65%	0.078%
2	3.257	9	12	19	rVB	37139	55455	0.76%	0.091%
3	3.975	130	134	140	rVB	16470	23528	0.32%	0.039%
4	5.922	461	465	469	rBV5	13434	19527	0.27%	0.032%
5	7.022	646	652	670	rBV	148510	336162	4.58%	0.551%
6	7.169	670	677	697	rVV	766546	1348593	18.39%	2.210%
7	7.369	705	711	736	rBV	709707	1291911	17.61%	2.117%
8	7.834	782	790	800	rBV	679996	1168898	15.94%	1.915%
9	7.951	804	810	816	rVB2	61990	111496	1.52%	0.183%
10	8.569	908	915	944	rBV	506738	1066386	14.54%	1.747%
11	9.004	979	989	1010	rBV	907609	1693393	23.09%	2.775%
12	9.392	1051	1055	1063	rVB2	13264	21029	0.29%	0.034%
13	9.728	1104	1112	1128	rBV	764958	1408245	19.20%	2.307%
14	10.275	1199	1205	1230	rBV	808805	1850636	25.23%	3.032%
15	10.639	1259	1267	1285	rBV	1052962	1861347	25.38%	3.050%
16	11.898	1475	1481	1487	rBV	20249	33412	0.46%	0.055%
17	12.251	1534	1541	1549	rBV	12789	32499	0.44%	0.053%
18	13.386	1729	1734	1741	rVV3	17558	25844	0.35%	0.042%
19	13.468	1743	1748	1752	rVB7	3909	7926	0.11%	0.013%
20	13.904	1815	1822	1839	rBV	2586602	3801150	51.82%	6.228%
21	14.186	1862	1870	1891	rBV	2760473	4342216	59.20%	7.115%
22	14.492	1914	1922	1937	rBV	1792143	2722433	37.12%	4.461%
23	14.721	1955	1961	1962	rBV2	7867	8854	0.12%	0.015%
24	14.757	1962	1967	1970	rBV4	27494	55341	0.75%	0.091%
25	15.315	2060	2062	2068	rVB4	7602	10581	0.14%	0.017%
26	15.486	2084	2091	2108	rBV	3786533	5528267	75.37%	9.058%
27	15.615	2108	2113	2128	rVV	1168218	1897036	25.86%	3.108%
28	15.727	2128	2132	2146	rVB4	24144	59316	0.81%	0.097%
29	15.857	2149	2154	2159	rVV	28100	38814	0.53%	0.064%
30	16.268	2221	2224	2230	rVB7	4772	7499	0.10%	0.012%
31	17.239	2383	2389	2400	rBV	2160813	3260200	44.45%	5.342%
32	17.339	2400	2406	2426	rVB	4090063	6180170	84.26%	10.127%
33	17.527	2435	2438	2444	rVB2	11326	17312	0.24%	0.028%
34	17.651	2457	2459	2469	rVB2	6416	11174	0.15%	0.018%
35	17.915	2501	2504	2509	rVB7	5822	7912	0.11%	0.013%
36	18.145	2538	2543	2551	rBV2	79687	173288	2.36%	0.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039462.D
Acq On : 18 Apr 2023 17:51
Operator : CG/JU
Sample : 02299-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	18.215	2551	2555	2562	rVB	29828	52638	0.72%	0.086%
38	19.203	2719	2723	2730	rBV3	51864	75193	1.03%	0.123%
39	19.274	2731	2735	2743	rBV	47402	91162	1.24%	0.149%
40	19.421	2756	2760	2773	rBV3	63734	162761	2.22%	0.267%
41	19.639	2791	2797	2810	rBV	5224266	7334825	100.00%	12.019%
42	21.433	3097	3102	3117	rBV	2225330	3388698	46.20%	5.553%
43	23.656	3473	3480	3497	rVB2	3125187	6406804	87.35%	10.498%
44	23.809	3499	3506	3517	rVB2	1423140	2991679	40.79%	4.902%




Sum of corrected areas: 61029339

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039462.D
Acq On : 18 Apr 2023 17:51
Operator : CG/JU
Sample : 02299-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

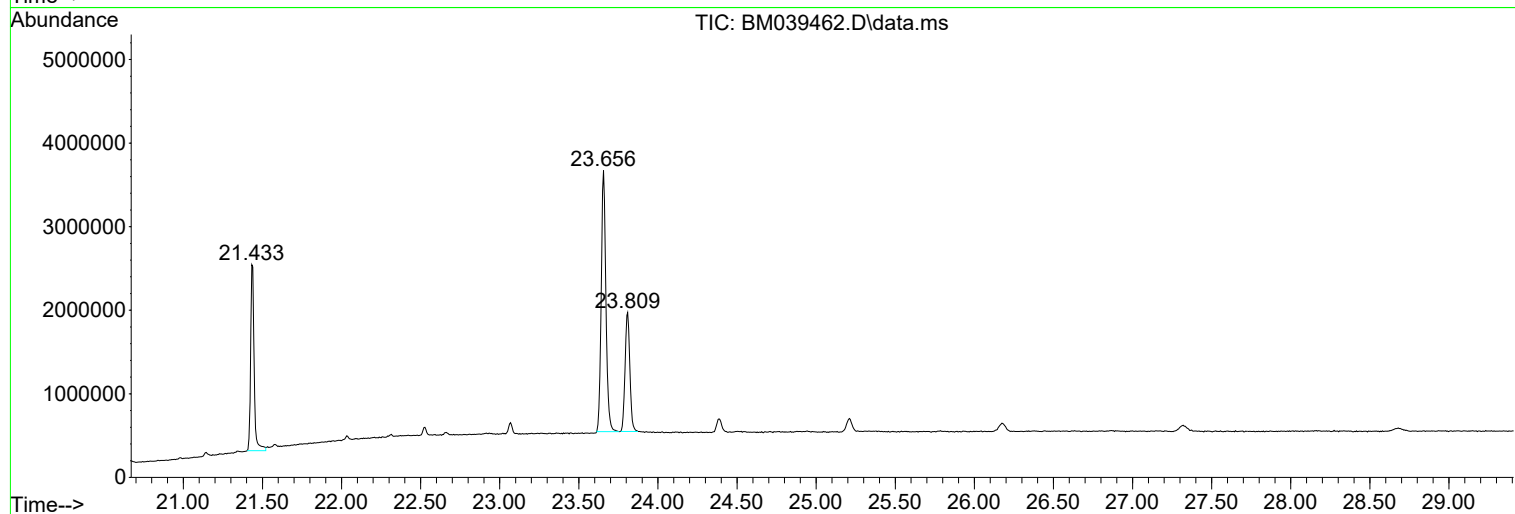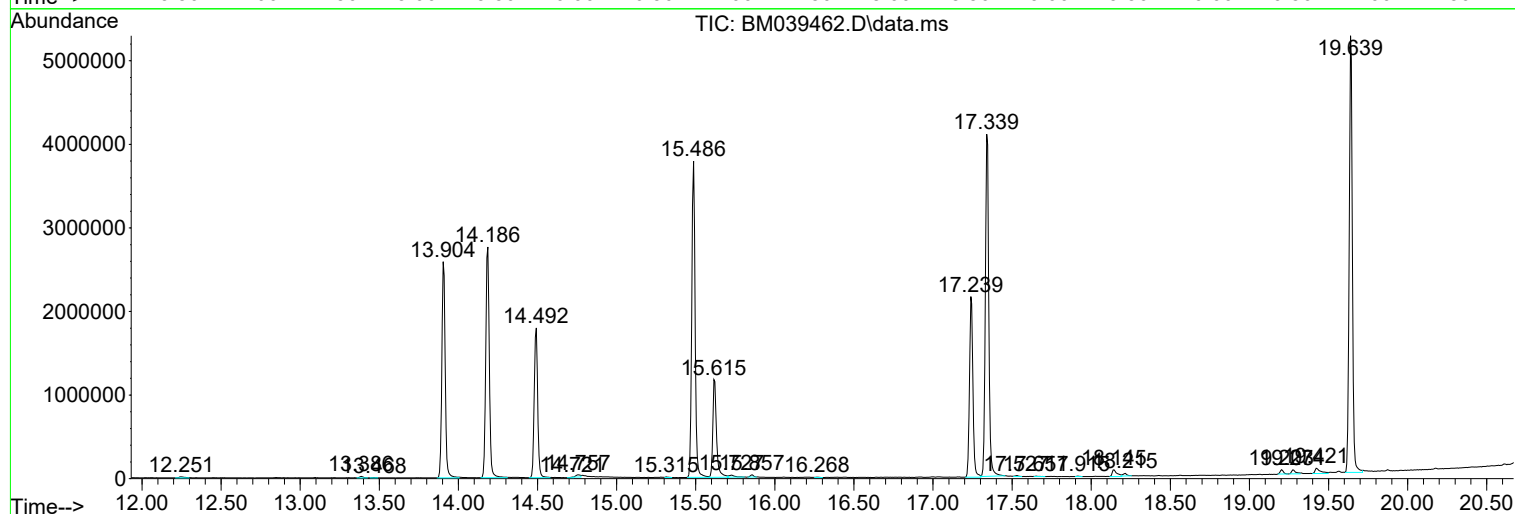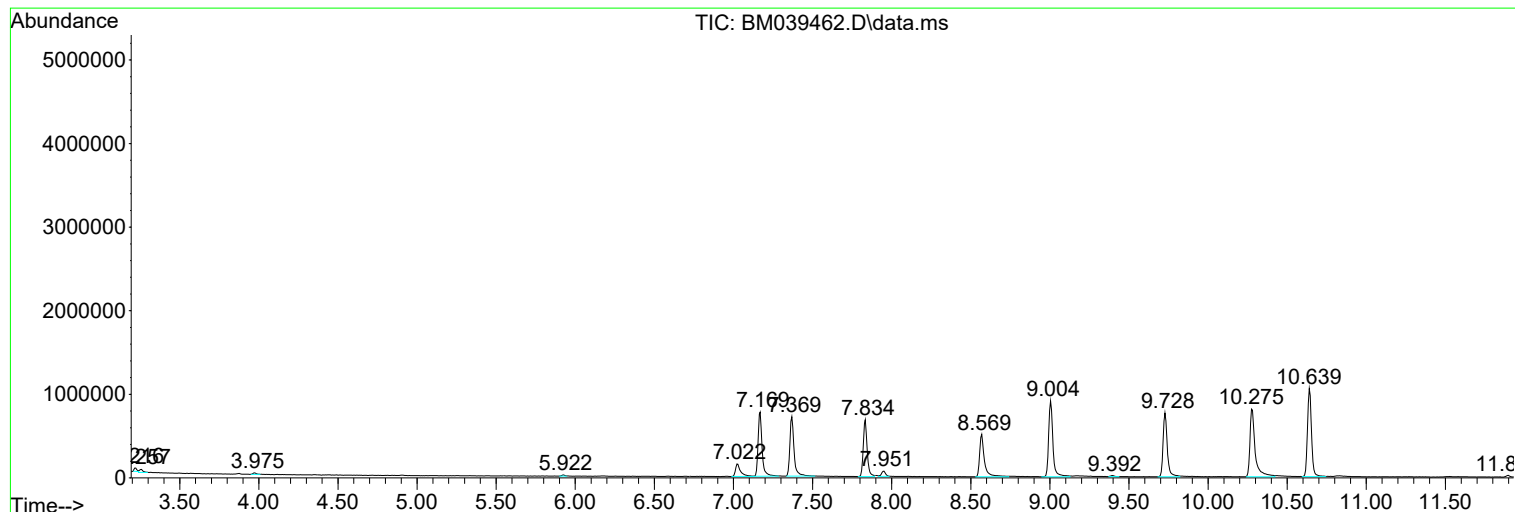

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039462.D
Acq On : 18 Apr 2023 17:51
Operator : CG/JU
Sample : 02299-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039462.D
Acq On : 18 Apr 2023 17:51
Operator : CG/JU
Sample : 02299-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc