

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039467.D
 Acq On : 18 Apr 2023 21:27
 Operator : CG/JU
 Sample : PB152173BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	21	rVB	81632	116570	1.73%	0.182%
2	3.657	78	80	91	rBV	55277	103661	1.54%	0.162%
3	3.969	130	133	142	rVB	19940	31825	0.47%	0.050%
4	7.016	645	651	670	rBV	817136	1580132	23.40%	2.468%
5	7.163	670	676	697	rVB	852762	1441604	21.35%	2.251%
6	7.363	704	710	730	rBV	991596	1718067	25.45%	2.683%
7	7.828	783	789	810	rBV	814483	1420602	21.04%	2.218%
8	8.563	908	914	932	rBV	1089540	2055436	30.44%	3.210%
9	9.004	981	989	1004	rBV	940492	1712303	25.36%	2.674%
10	9.728	1105	1112	1132	rBV	783542	1478043	21.89%	2.308%
11	10.275	1198	1205	1232	rBV	874629	2033338	30.12%	3.175%
12	10.639	1260	1267	1281	rBV	1257806	2176118	32.23%	3.398%
13	12.263	1536	1543	1551	rBV5	8398	26899	0.40%	0.042%
14	13.904	1815	1822	1837	rBV	2576140	3764722	55.76%	5.879%
15	14.180	1862	1869	1888	rBV	2342543	3657564	54.17%	5.712%
16	14.486	1915	1921	1938	rBV	2035282	3063621	45.38%	4.784%
17	14.727	1957	1962	1989	rBV	431751	1251995	18.54%	1.955%
18	15.480	2084	2090	2107	rBV	3445659	5287124	78.31%	8.256%
19	15.615	2107	2113	2128	rVV	1156999	1850764	27.41%	2.890%
20	15.721	2129	2131	2139	rVB	23942	35948	0.53%	0.056%
21	15.992	2172	2177	2184	rVB	20183	29015	0.43%	0.045%
22	16.268	2220	2224	2227	rBV6	4639	7246	0.11%	0.011%
23	17.027	2351	2353	2358	rBV5	4784	7056	0.10%	0.011%
24	17.239	2383	2389	2400	rBV	2574740	3635929	53.85%	5.678%
25	17.339	2400	2406	2429	rVB	3864131	5777086	85.57%	9.021%
26	17.921	2501	2505	2511	rVB5	7402	11587	0.17%	0.018%
27	18.162	2540	2546	2553	rBV10	9599	30787	0.46%	0.048%
28	19.203	2719	2723	2730	rBV2	45578	80122	1.19%	0.125%
29	19.274	2731	2735	2743	rVV	36219	61505	0.91%	0.096%
30	19.639	2791	2797	2813	rBV	4967944	6751572	100.00%	10.543%
31	21.433	3097	3102	3111	rBV	2690895	3694515	54.72%	5.769%
32	23.650	3472	3479	3496	rVB2	2722752	5753331	85.21%	8.984%
33	23.803	3498	3505	3519	rVB2	1621997	3391376	50.23%	5.296%




Sum of corrected areas: 64037463

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039467.D
Acq On : 18 Apr 2023 21:27
Operator : CG/JU
Sample : PB152173BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

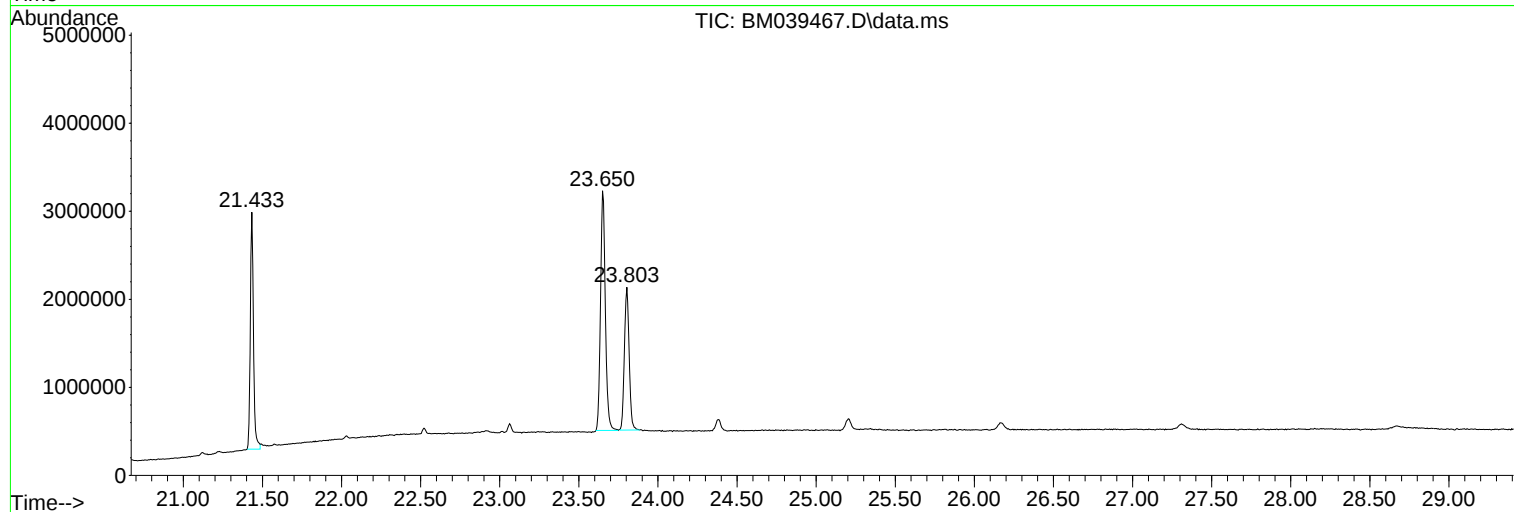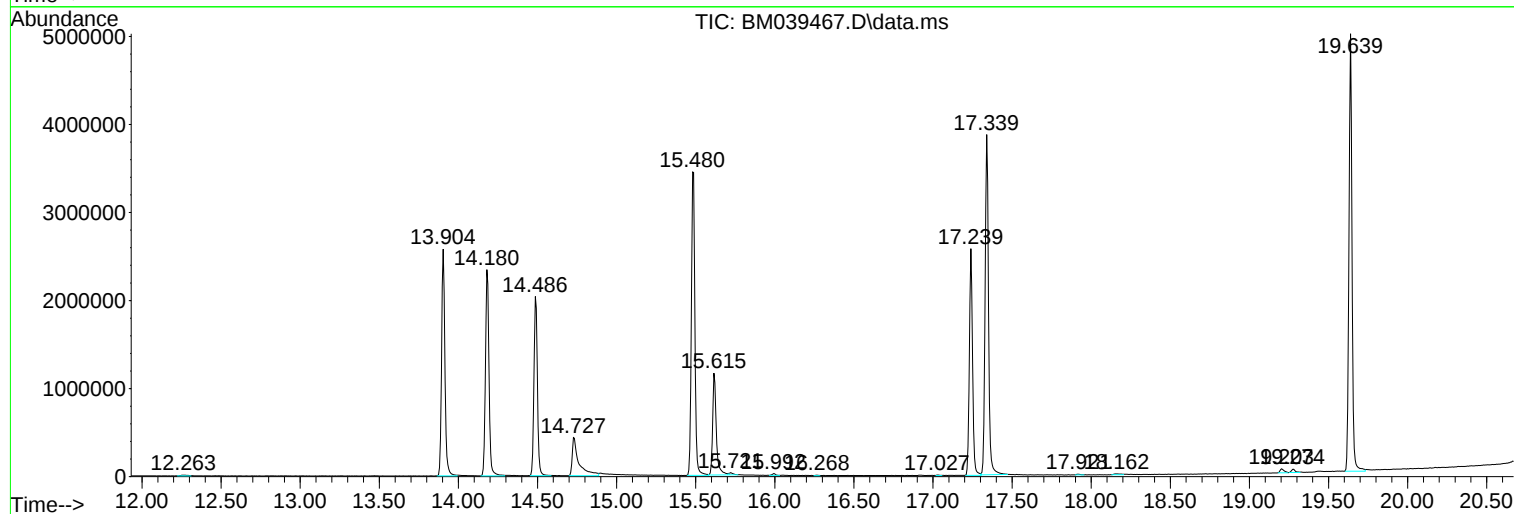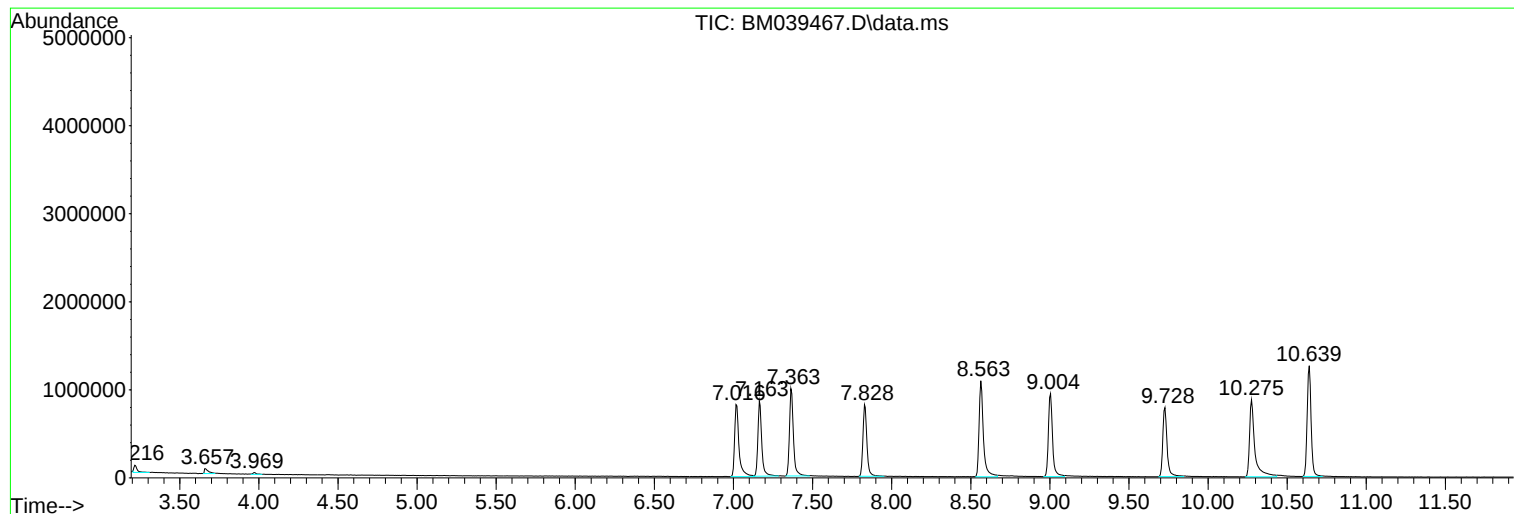

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039467.D
Acq On : 18 Apr 2023 21:27
Operator : CG/JU
Sample : PB152173BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039467.D
Acq On : 18 Apr 2023 21:27
Operator : CG/JU
Sample : PB152173BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------