

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039468.D
 Acq On : 18 Apr 2023 22:04
 Operator : CG/JU
 Sample : PB152152BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	14	rVB	74508	99241	1.55%	0.168%
2	3.975	130	134	138	rVB	16605	21410	0.34%	0.036%
3	7.016	645	651	670	rBV2	760552	1479276	23.15%	2.509%
4	7.163	670	676	699	rVB	781571	1360206	21.29%	2.307%
5	7.363	704	710	730	rVV	917904	1600574	25.05%	2.715%
6	7.828	782	789	806	rBV	695910	1227356	19.21%	2.082%
7	8.563	908	914	944	rBV	995755	1960312	30.68%	3.325%
8	9.004	982	989	1004	rBV	886492	1607057	25.16%	2.726%
9	9.728	1104	1112	1135	rBV	738407	1409967	22.07%	2.392%
10	10.275	1198	1205	1230	rBV	788845	1871810	29.30%	3.175%
11	10.639	1260	1267	1286	rBV	1110491	1904529	29.81%	3.231%
12	12.263	1537	1543	1545	rBV5	7671	14538	0.23%	0.025%
13	13.904	1815	1822	1837	rBV	2500933	3630536	56.83%	6.158%
14	14.180	1862	1869	1887	rBV	2557317	3904540	61.12%	6.623%
15	14.486	1914	1921	1938	rBV	1814070	2759492	43.19%	4.681%
16	14.733	1956	1963	1989	rBV	380855	1156297	18.10%	1.961%
17	15.486	2083	2091	2107	rBV	3287938	5059698	79.20%	8.582%
18	15.615	2107	2113	2128	rBV	1085316	1733115	27.13%	2.940%
19	15.992	2173	2177	2184	rVB2	16277	24951	0.39%	0.042%
20	16.274	2217	2225	2229	rBV8	5087	9059	0.14%	0.015%
21	16.915	2331	2334	2337	rBV4	5829	6778	0.11%	0.011%
22	17.033	2350	2354	2358	rBV4	4231	7054	0.11%	0.012%
23	17.239	2383	2389	2400	rBV	2278803	3245941	50.81%	5.506%
24	17.339	2400	2406	2426	rVB	3692725	5519178	86.39%	9.362%
25	17.915	2499	2504	2509	rBV7	5609	10053	0.16%	0.017%
26	18.151	2540	2544	2545	rBV3	9216	10184	0.16%	0.017%
27	19.203	2719	2723	2729	rBV	43626	60894	0.95%	0.103%
28	19.274	2731	2735	2743	rBV	34083	57607	0.90%	0.098%
29	19.639	2791	2797	2816	rBV	4536648	6388607	100.00%	10.837%
30	21.433	3097	3102	3116	rBV	2106724	3138012	49.12%	5.323%
31	23.650	3472	3479	3497	rVB2	2337603	4975527	77.88%	8.440%
32	23.803	3498	3505	3518	rVB2	1259557	2700692	42.27%	4.581%




Sum of corrected areas: 58954491

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039468.D
Acq On : 18 Apr 2023 22:04
Operator : CG/JU
Sample : PB152152BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

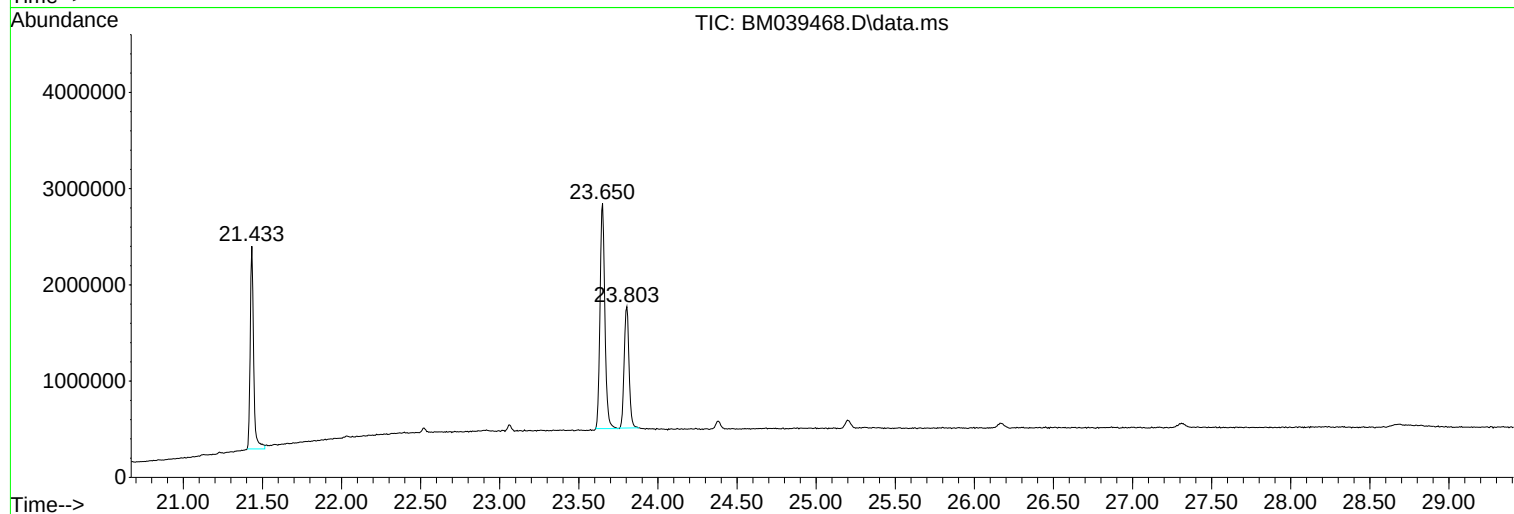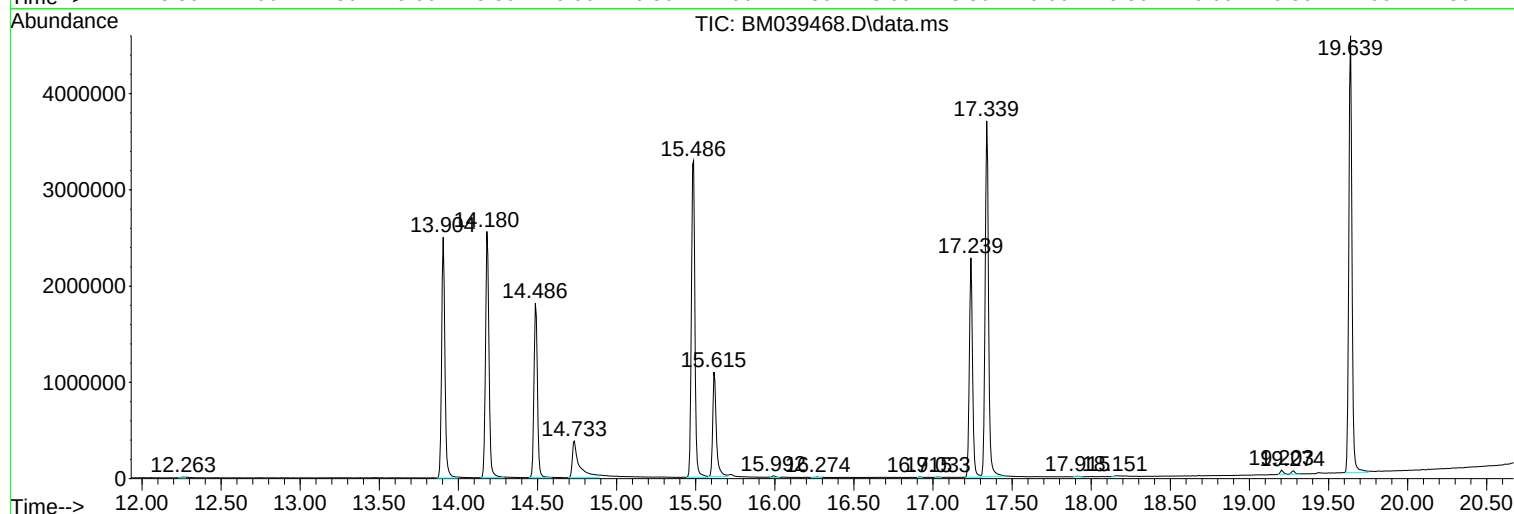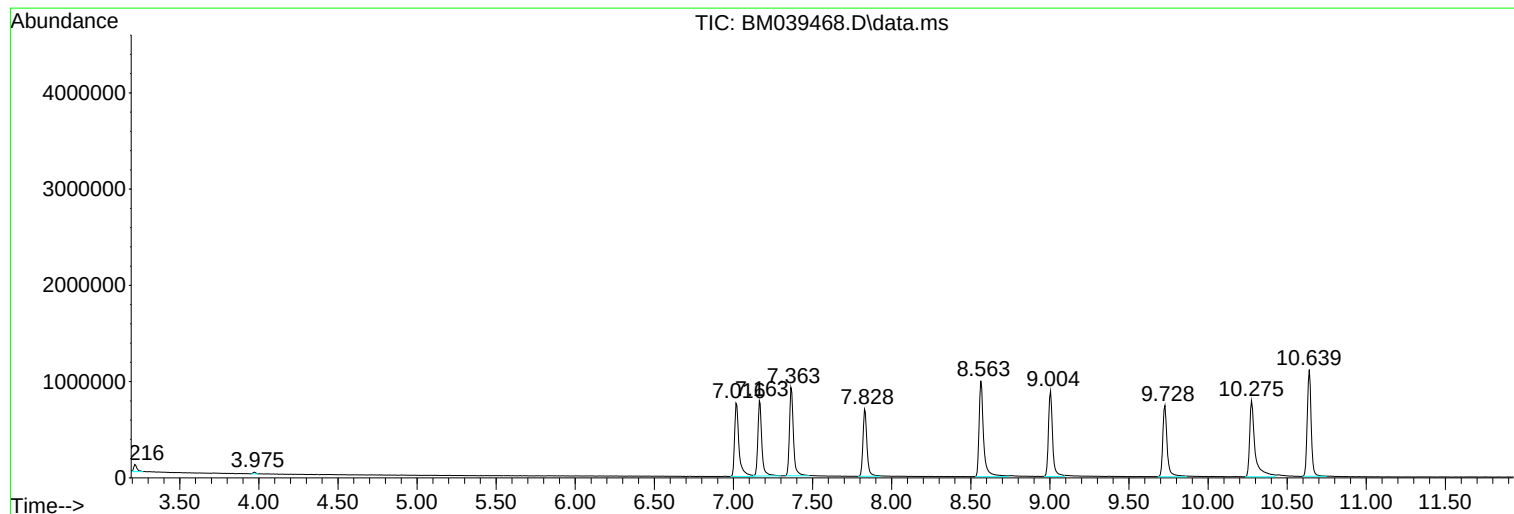

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039468.D
Acq On : 18 Apr 2023 22:04
Operator : CG/JU
Sample : PB152152BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039468.D
Acq On : 18 Apr 2023 22:04
Operator : CG/JU
Sample : PB152152BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------