

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039470.D
 Acq On : 18 Apr 2023 23:16
 Operator : CG/JU
 Sample : 02335-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	14	rVB	74394	91515	1.22%	0.141%
2	3.646	75	78	96	rBV	236764	414790	5.54%	0.641%
3	3.969	130	133	140	rVB	22403	30278	0.40%	0.047%
4	5.093	319	324	333	rVB2	13929	27215	0.36%	0.042%
5	5.569	403	405	414	rVB8	4531	9235	0.12%	0.014%
6	7.022	646	652	670	rBV	213565	461851	6.17%	0.714%
7	7.163	670	676	698	rVB	939175	1606531	21.45%	2.484%
8	7.363	703	710	731	rBV	865080	1554330	20.75%	2.403%
9	7.828	783	789	810	rBV	735732	1301348	17.37%	2.012%
10	8.563	908	914	929	rBV	641662	1282859	17.13%	1.983%
11	9.004	981	989	1009	rBV	1075880	1973789	26.35%	3.051%
12	9.363	1045	1050	1052	rBV4	11717	19159	0.26%	0.030%
13	9.728	1104	1112	1137	rBV	844152	1587521	21.19%	2.454%
14	10.275	1197	1205	1227	rBV	933669	2108969	28.16%	3.260%
15	10.640	1259	1267	1288	rBV	1160923	2000944	26.71%	3.093%
16	10.828	1293	1299	1311	rVB4	11856	41613	0.56%	0.064%
17	12.251	1535	1541	1551	rBV3	13526	36686	0.49%	0.057%
18	12.498	1576	1583	1588	rVB2	5352	10178	0.14%	0.016%
19	13.304	1714	1720	1725	rBV7	5215	9518	0.13%	0.015%
20	13.381	1728	1733	1738	rVB6	4541	8654	0.12%	0.013%
21	13.904	1815	1822	1835	rBV	2916691	4171181	55.69%	6.448%
22	14.181	1862	1869	1888	rBV	3262083	4939231	65.94%	7.636%
23	14.486	1914	1921	1938	rBV	1903061	2802153	37.41%	4.332%
24	14.751	1959	1966	1982	rBV3	46567	210112	2.81%	0.325%
25	15.239	2045	2049	2054	rBV	9737	14803	0.20%	0.023%
26	15.333	2059	2065	2070	rVB8	4337	8174	0.11%	0.013%
27	15.486	2083	2091	2107	rBV	3936085	6133565	81.89%	9.482%
28	15.616	2107	2113	2128	rVV	1331167	2046230	27.32%	3.163%
29	15.722	2128	2131	2139	rVB2	23521	43622	0.58%	0.067%
30	15.851	2148	2153	2164	rVB	121205	181084	2.42%	0.280%
31	16.416	2245	2249	2255	rBV2	13228	20107	0.27%	0.031%
32	16.722	2298	2301	2306	rVB7	6678	8132	0.11%	0.013%
33	16.833	2315	2320	2328	rBV	29943	44209	0.59%	0.068%
34	16.916	2330	2334	2340	rVB7	5680	9392	0.13%	0.015%
35	17.033	2348	2354	2358	rBV6	5540	10230	0.14%	0.016%
36	17.239	2383	2389	2400	rBV	2216000	3228567	43.10%	4.991%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039470.D
Acq On : 18 Apr 2023 23:16
Operator : CG/JU
Sample : 02335-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	17.339	2400	2406	2425	rVB	4584922	6669747	89.05%	10.311%
38	18.139	2537	2542	2553	rBV	103951	224120	2.99%	0.346%
39	18.416	2586	2589	2596	rVB5	12362	20436	0.27%	0.032%
40	19.204	2718	2723	2728	rBV2	55641	83951	1.12%	0.130%
41	19.274	2731	2735	2740	rBV	45704	71203	0.95%	0.110%
42	19.421	2756	2760	2773	rBV3	64021	154745	2.07%	0.239%
43	19.563	2781	2784	2787	rVB3	16943	16979	0.23%	0.026%
44	19.639	2791	2797	2817	rVV	5357879	7490176	100.00%	11.579%
45	21.145	3049	3053	3061	rBV3	94591	181835	2.43%	0.281%
46	21.433	3096	3102	3115	rBV	1952524	2962433	39.55%	4.580%
47	23.645	3471	3478	3493	rBV2	2797650	5803107	77.48%	8.971%
48	23.798	3498	3504	3519	rVB2	1203377	2558559	34.16%	3.955%




Sum of corrected areas: 64685066

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039470.D
Acq On : 18 Apr 2023 23:16
Operator : CG/JU
Sample : 02335-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

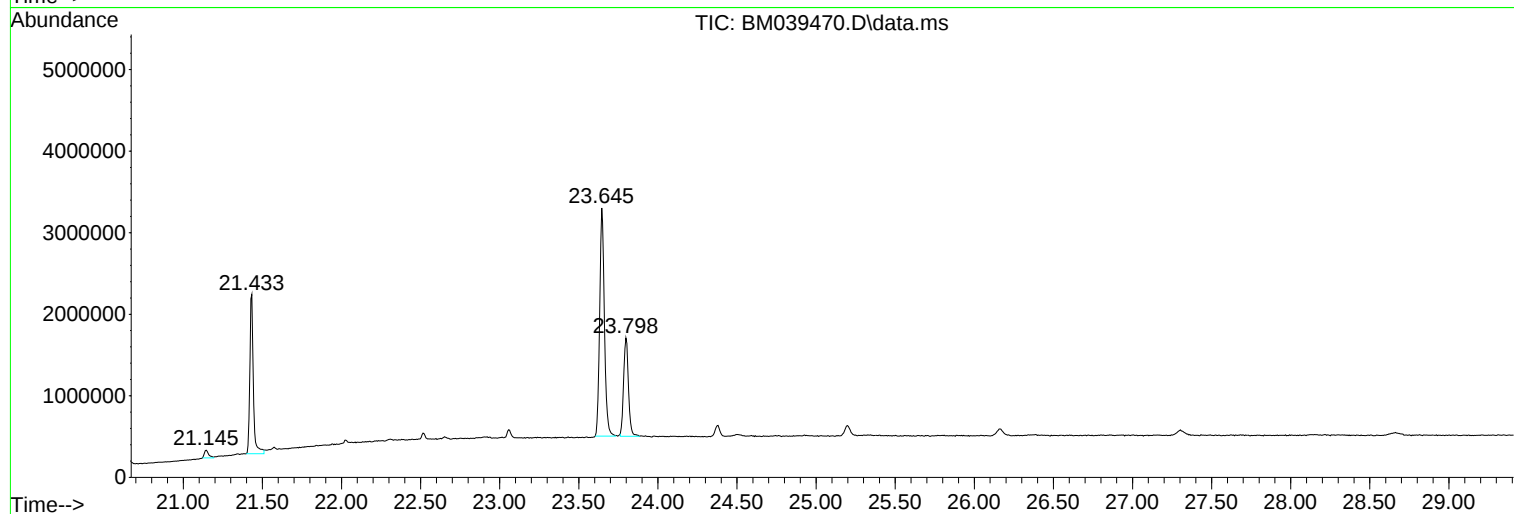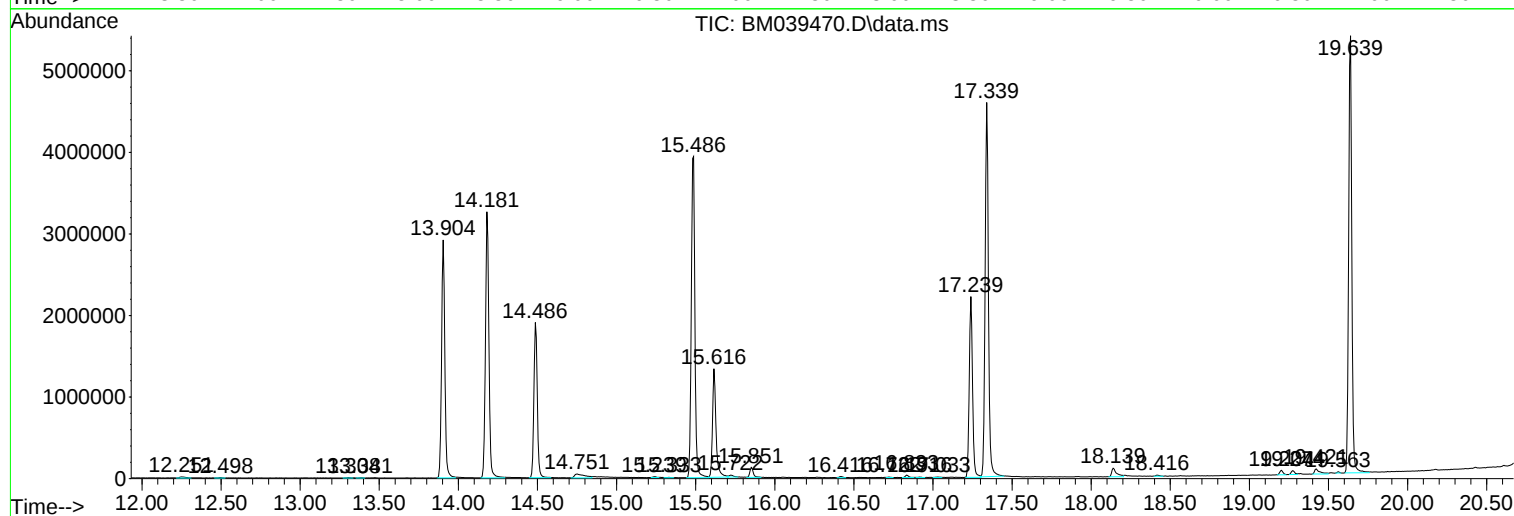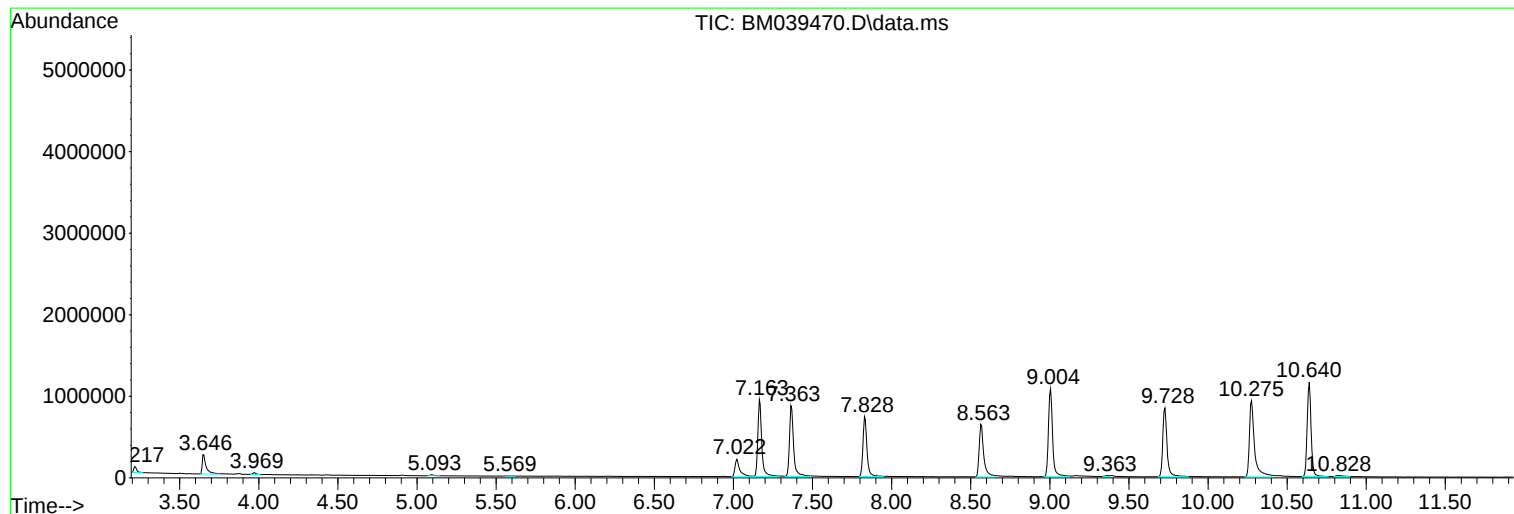

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039470.D
Acq On : 18 Apr 2023 23:16
Operator : CG/JU
Sample : 02335-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039470.D
Acq On : 18 Apr 2023 23:16
Operator : CG/JU
Sample : 02335-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------