

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039471.D
 Acq On : 18 Apr 2023 23:52
 Operator : CG/JU
 Sample : 02335-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	13	rVB	54936	68015	0.98%	0.111%
2	3.646	76	78	95	rBV	209657	359266	5.17%	0.584%
3	3.969	130	133	141	rVB2	22381	33195	0.48%	0.054%
4	7.022	646	652	668	rVV	136945	317807	4.57%	0.517%
5	7.163	670	676	698	rVV	780757	1347673	19.39%	2.191%
6	7.363	704	710	732	rBV	720816	1277287	18.38%	2.076%
7	7.828	783	789	809	rBV	747003	1330872	19.15%	2.163%
8	8.563	908	914	935	rBV	483989	1011079	14.55%	1.644%
9	9.004	982	989	1010	rBV	896732	1676614	24.13%	2.726%
10	9.163	1012	1016	1019	rVV5	4568	7426	0.11%	0.012%
11	9.392	1052	1055	1064	rVB4	8024	14382	0.21%	0.023%
12	9.728	1104	1112	1131	rBV	735294	1394961	20.07%	2.268%
13	10.275	1198	1205	1230	rBV	905875	1879594	27.05%	3.056%
14	10.639	1259	1267	1283	rBV	1213885	2054972	29.57%	3.341%
15	10.792	1285	1293	1319	rBV	701728	1577281	22.70%	2.564%
16	11.892	1473	1480	1486	rBV2	6634	11601	0.17%	0.019%
17	12.251	1534	1541	1555	rBV2	11595	32585	0.47%	0.053%
18	13.904	1815	1822	1837	rBV	2514058	3653665	52.58%	5.939%
19	14.180	1862	1869	1890	rBV	2808919	4280661	61.60%	6.959%
20	14.486	1914	1921	1934	rBV	1906558	2888252	41.56%	4.695%
21	14.574	1934	1936	1940	rVB5	6246	7043	0.10%	0.011%
22	14.751	1961	1966	1967	rBV2	26567	36213	0.52%	0.059%
23	15.239	2044	2049	2054	rBV3	6752	12536	0.18%	0.020%
24	15.310	2058	2061	2068	rVB2	7219	13519	0.19%	0.022%
25	15.480	2084	2090	2107	rBV	3553859	5378866	77.41%	8.744%
26	15.615	2107	2113	2128	rVV	1192113	1894384	27.26%	3.080%
27	15.727	2128	2132	2143	rVB6	22785	48917	0.70%	0.080%
28	15.851	2148	2153	2165	rVB	87561	141599	2.04%	0.230%
29	16.992	2344	2347	2351	rBV6	4102	7843	0.11%	0.013%
30	17.027	2351	2353	2360	rVB5	5413	9209	0.13%	0.015%
31	17.239	2382	2389	2400	rBV	2277958	3340792	48.08%	5.431%
32	17.339	2400	2406	2428	rVB	4216686	6157810	88.62%	10.010%
33	17.521	2435	2437	2442	rVB5	6277	9036	0.13%	0.015%
34	17.909	2501	2503	2509	rVB7	4853	7488	0.11%	0.012%
35	18.139	2537	2542	2551	rBV	125991	245080	3.53%	0.398%
36	18.204	2551	2553	2559	rVB	12996	23701	0.34%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039471.D
Acq On : 18 Apr 2023 23:52
Operator : CG/JU
Sample : 02335-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	18.562	2609	2614	2619	rBV	98773	124103	1.79%	0.202%
38	19.203	2718	2723	2730	rBV2	50859	83482	1.20%	0.136%
39	19.274	2730	2735	2741	rBV	49214	87086	1.25%	0.142%
40	19.421	2756	2760	2768	rBV2	77743	149265	2.15%	0.243%
41	19.639	2791	2797	2813	rBV	5047958	6948796	100.00%	11.296%
42	21.145	3049	3053	3059	rBV3	164053	276977	3.99%	0.450%
43	21.427	3096	3101	3117	rBV	2077393	3130326	45.05%	5.089%
44	23.644	3471	3478	3496	rVV	2697542	5422258	78.03%	8.815%
45	23.797	3497	3504	3518	rVB2	1266047	2741573	39.45%	4.457%




Sum of corrected areas: 61515090

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039471.D
Acq On : 18 Apr 2023 23:52
Operator : CG/JU
Sample : 02335-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

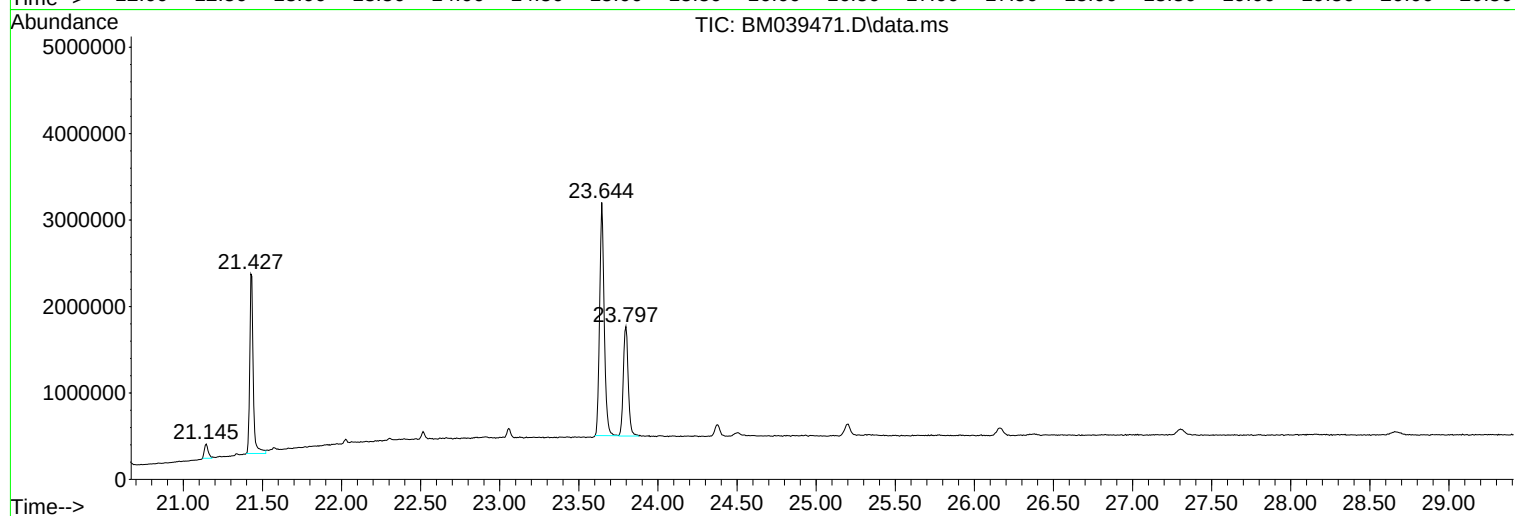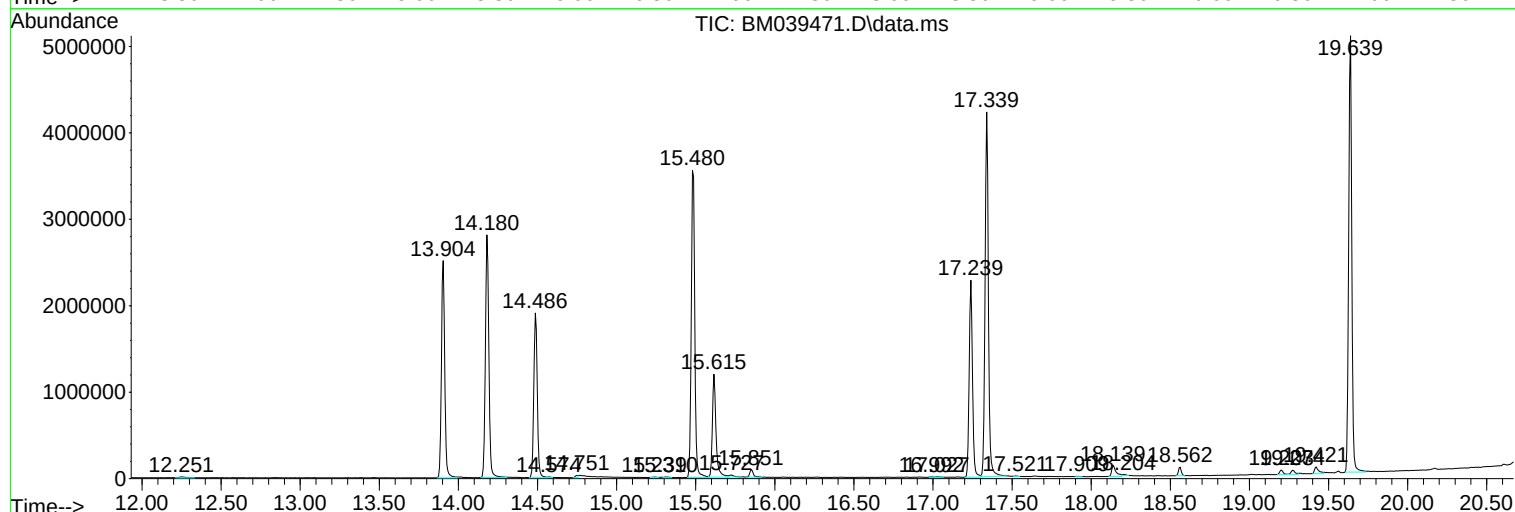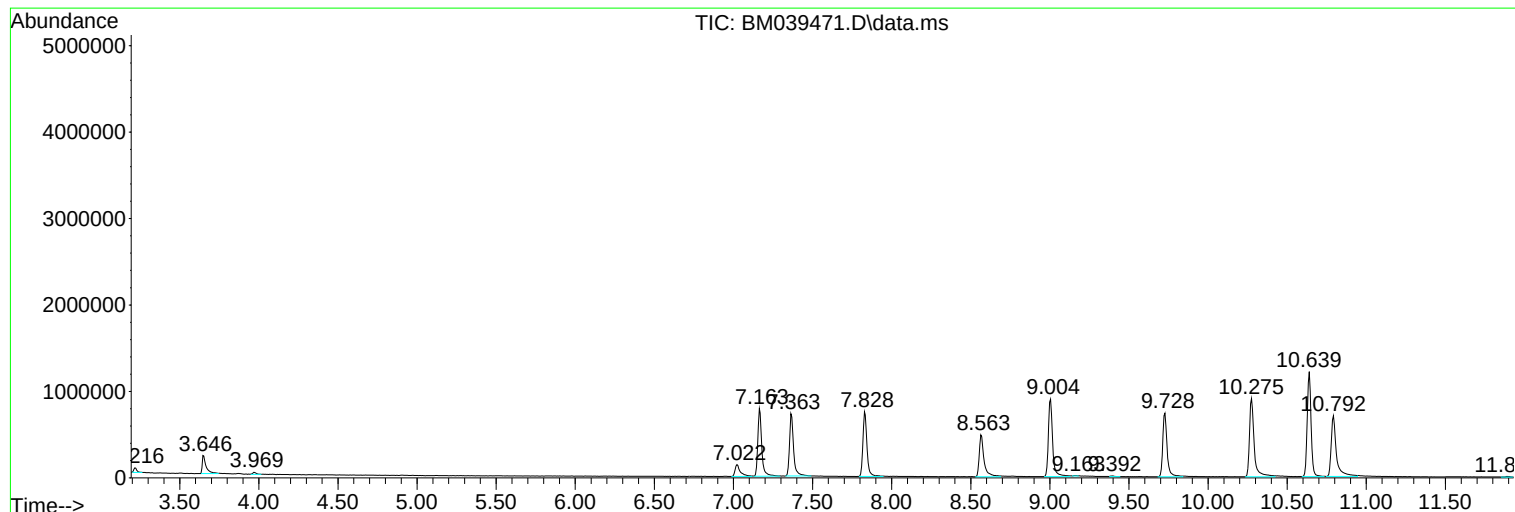

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039471.D
Acq On : 18 Apr 2023 23:52
Operator : CG/JU
Sample : 02335-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039471.D
Acq On : 18 Apr 2023 23:52
Operator : CG/JU
Sample : 02335-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc