

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039472.D
 Acq On : 19 Apr 2023 00:28
 Operator : CG/JU
 Sample : 02335-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	14	rVB	52896	65942	0.90%	0.105%
2	3.651	76	79	92	rBV	121906	220539	3.01%	0.350%
3	3.969	130	133	139	rVB2	17400	23355	0.32%	0.037%
4	5.093	319	324	332	rBV	42273	69826	0.95%	0.111%
5	7.022	647	652	670	rBV	149034	342622	4.67%	0.544%
6	7.163	670	676	698	rVV	858832	1534497	20.92%	2.436%
7	7.363	704	710	732	rBV	768374	1371474	18.70%	2.177%
8	7.828	782	789	811	rBV	689948	1235668	16.84%	1.962%
9	8.563	908	914	934	rBV	427725	917709	12.51%	1.457%
10	9.004	981	989	1012	rBV	1002178	1838847	25.07%	2.919%
11	9.727	1104	1112	1130	rBV	816213	1522606	20.76%	2.417%
12	10.275	1198	1205	1232	rBV	994512	2032544	27.71%	3.227%
13	10.639	1259	1267	1283	rBV	1115844	1908044	26.01%	3.029%
14	10.792	1286	1293	1315	rBV	677406	1490724	20.32%	2.367%
15	11.486	1404	1411	1412	rBV4	13655	22900	0.31%	0.036%
16	12.251	1534	1541	1544	rBV2	12285	24962	0.34%	0.040%
17	13.904	1814	1822	1838	rBV	2815228	4025306	54.87%	6.390%
18	14.180	1861	1869	1887	rBV	3026123	4653625	63.44%	7.388%
19	14.333	1889	1895	1899	rVB5	10135	16660	0.23%	0.026%
20	14.486	1914	1921	1939	rBV	1800783	2710187	36.94%	4.302%
21	14.757	1957	1967	1978	rBV5	34945	152530	2.08%	0.242%
22	15.486	2084	2091	2107	rBV	3838750	5862007	79.91%	9.306%
23	15.615	2107	2113	2127	rVV	1315439	2052808	27.98%	3.259%
24	15.727	2129	2132	2143	rVB5	28156	53440	0.73%	0.085%
25	15.851	2148	2153	2161	rBV	78591	118140	1.61%	0.188%
26	16.215	2209	2215	2219	rBV3	15778	29127	0.40%	0.046%
27	16.715	2296	2300	2305	rVB7	8446	15658	0.21%	0.025%
28	16.780	2307	2311	2316	rBV3	16263	25291	0.34%	0.040%
29	16.833	2316	2320	2324	rVV2	24841	33409	0.46%	0.053%
30	17.039	2350	2355	2360	rVB2	17929	25037	0.34%	0.040%
31	17.115	2365	2368	2372	rBV3	13404	16941	0.23%	0.027%
32	17.239	2383	2389	2400	rBV	2154357	3145283	42.88%	4.993%
33	17.339	2400	2406	2424	rVB	4386670	6426504	87.60%	10.202%
34	17.651	2455	2459	2465	rBV9	8083	14127	0.19%	0.022%
35	18.139	2538	2542	2553	rBV2	122764	255434	3.48%	0.406%
36	19.203	2718	2723	2730	rBV	53935	88697	1.21%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039472.D
Acq On : 19 Apr 2023 00:28
Operator : CG/JU
Sample : 02335-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.274	2731	2735	2739	rBV	48652	78819	1.07%	0.125%
38	19.421	2756	2760	2773	rBV2	86082	193957	2.64%	0.308%
39	19.639	2791	2797	2815	rBV	5342262	7335904	100.00%	11.646%
40	21.144	3049	3053	3059	rBV6	86930	162265	2.21%	0.258%
41	21.427	3096	3101	3118	rBV	1946968	2908261	39.64%	4.617%
42	23.644	3471	3478	3495	rBV2	2600877	5554835	75.72%	8.818%
43	23.797	3498	3504	3516	rVB2	1169213	2415361	32.93%	3.834%




Sum of corrected areas: 62991872

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039472.D
Acq On : 19 Apr 2023 00:28
Operator : CG/JU
Sample : 02335-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

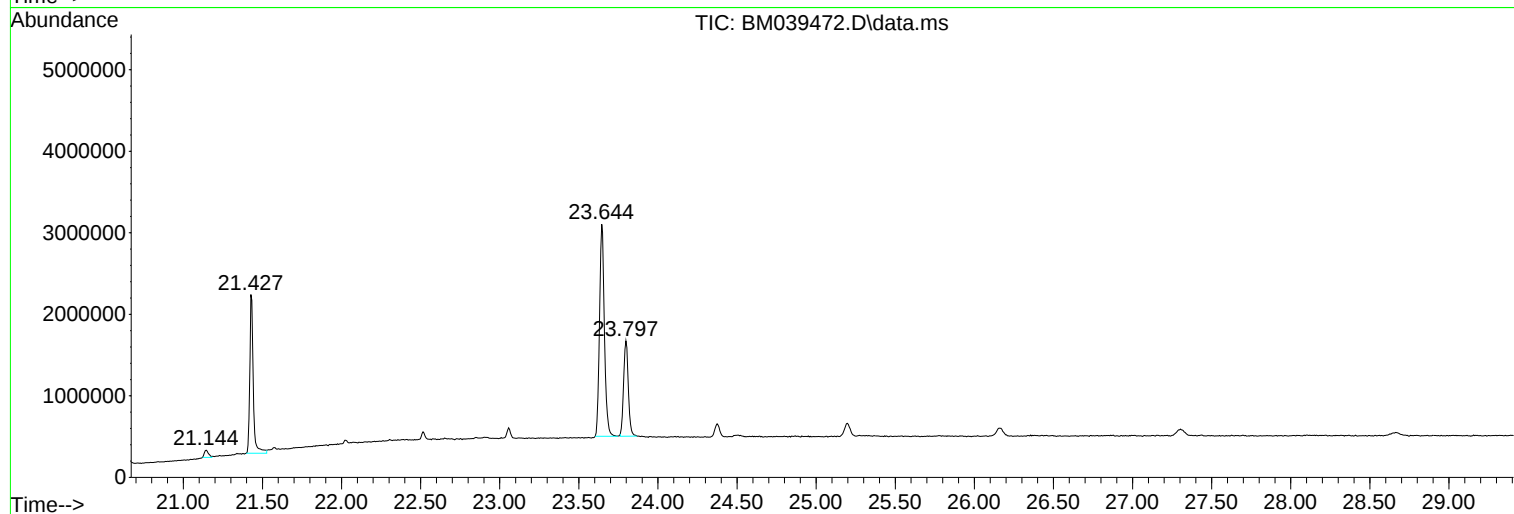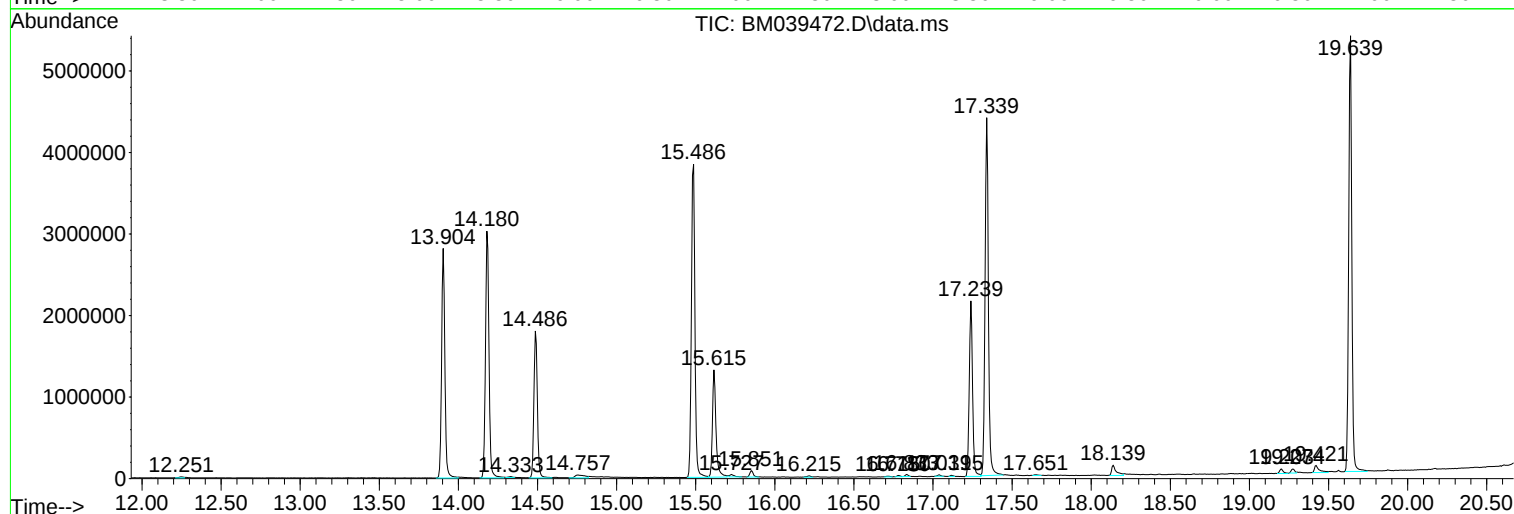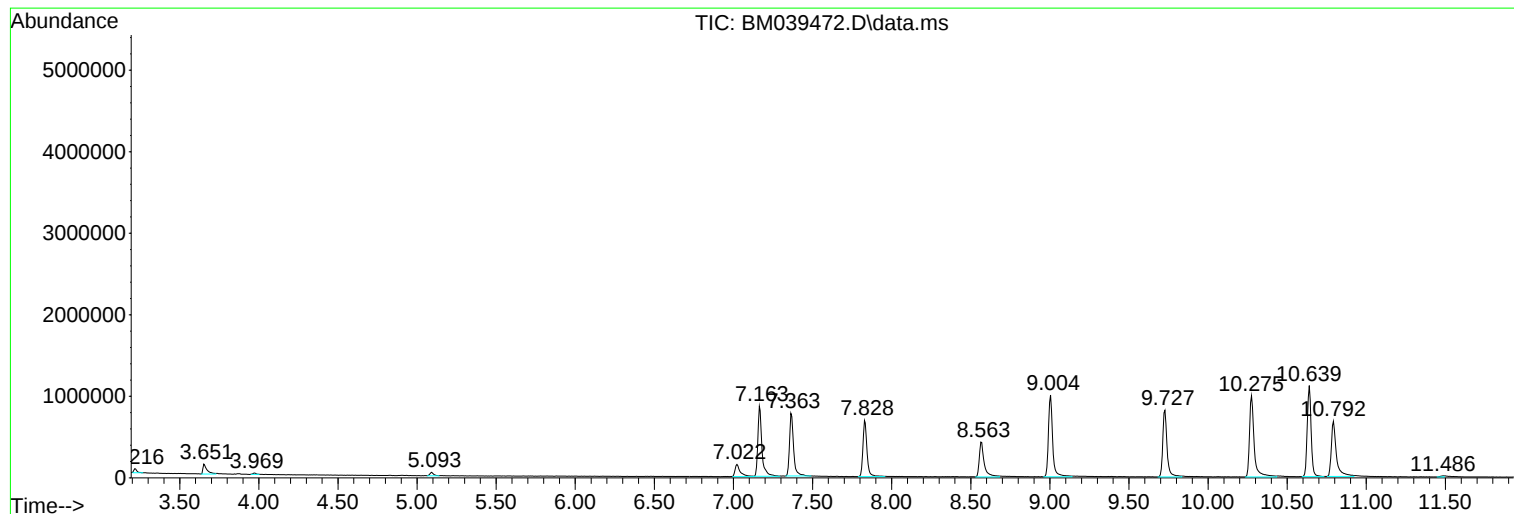

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039472.D
Acq On : 19 Apr 2023 00:28
Operator : CG/JU
Sample : 02335-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039472.D
Acq On : 19 Apr 2023 00:28
Operator : CG/JU
Sample : 02335-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------