

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039473.D
 Acq On : 19 Apr 2023 01:04
 Operator : CG/JU
 Sample : 02335-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	12	rVB	60384	67106	0.95%	0.106%
2	3.646	76	78	97	rBV	207979	364351	5.18%	0.575%
3	3.969	130	133	139	rVB	20893	28014	0.40%	0.044%
4	7.022	645	652	669	rBV	163327	371467	5.28%	0.586%
5	7.163	670	676	698	rVV	894856	1574037	22.39%	2.483%
6	7.363	704	710	731	rBV	811205	1450521	20.63%	2.288%
7	7.828	783	789	807	rBV	764764	1327702	18.89%	2.095%
8	8.563	908	914	938	rBV	566056	1160379	16.51%	1.831%
9	9.004	980	989	1011	rBV	1011280	1885458	26.82%	2.975%
10	9.728	1104	1112	1134	rBV	829415	1573524	22.38%	2.482%
11	10.275	1197	1205	1233	rBV	1022803	2105047	29.94%	3.321%
12	10.639	1258	1267	1283	rBV	1181073	2064902	29.37%	3.258%
13	10.792	1286	1293	1322	rBV	834981	1870872	26.61%	2.951%
14	12.251	1535	1541	1546	rBV3	11247	23387	0.33%	0.037%
15	12.816	1630	1637	1645	rBV9	3382	7913	0.11%	0.012%
16	13.304	1716	1720	1725	rVB7	4349	7429	0.11%	0.012%
17	13.904	1815	1822	1837	rBV	2636037	3911922	55.64%	6.171%
18	14.180	1862	1869	1886	rBV	3141852	4687818	66.68%	7.396%
19	14.327	1890	1894	1900	rVB9	11679	20547	0.29%	0.032%
20	14.486	1914	1921	1934	rBV	1940808	2864731	40.75%	4.519%
21	14.751	1961	1966	1967	rBV2	26990	38541	0.55%	0.061%
22	15.480	2084	2090	2107	rBV	3720237	5748045	81.76%	9.068%
23	15.616	2107	2113	2128	rVV	1202055	1899837	27.02%	2.997%
24	15.727	2128	2132	2143	rVB2	24364	54703	0.78%	0.086%
25	15.851	2148	2153	2162	rVV	66689	98287	1.40%	0.155%
26	16.716	2297	2300	2310	rVB10	7474	14773	0.21%	0.023%
27	16.833	2317	2320	2324	rBV6	6574	8802	0.13%	0.014%
28	17.239	2382	2389	2399	rBV	2288697	3285390	46.73%	5.183%
29	17.339	2399	2406	2426	rVB	4284744	6292572	89.51%	9.927%
30	18.139	2537	2542	2554	rBV	92763	206162	2.93%	0.325%
31	19.198	2718	2722	2728	rBV2	49496	82508	1.17%	0.130%
32	19.274	2731	2735	2740	rBV	41112	65764	0.94%	0.104%
33	19.421	2756	2760	2765	rBV	59471	102484	1.46%	0.162%
34	19.562	2781	2784	2787	rBV3	14582	16987	0.24%	0.027%
35	19.639	2790	2797	2815	rBV	4982406	7030217	100.00%	11.091%
36	21.427	3096	3101	3113	rBV	2004313	2946575	41.91%	4.649%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039473.D
Acq On : 19 Apr 2023 01:04
Operator : CG/JU
Sample : 02335-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	23.645	3471	3478	3493	rBV2	2724790	5484844	78.02%	8.653%
38	23.797	3497	3504	3517	rVB2	1275709	2643714	37.61%	4.171%




Sum of corrected areas: 63387332

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039473.D
Acq On : 19 Apr 2023 01:04
Operator : CG/JU
Sample : 02335-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

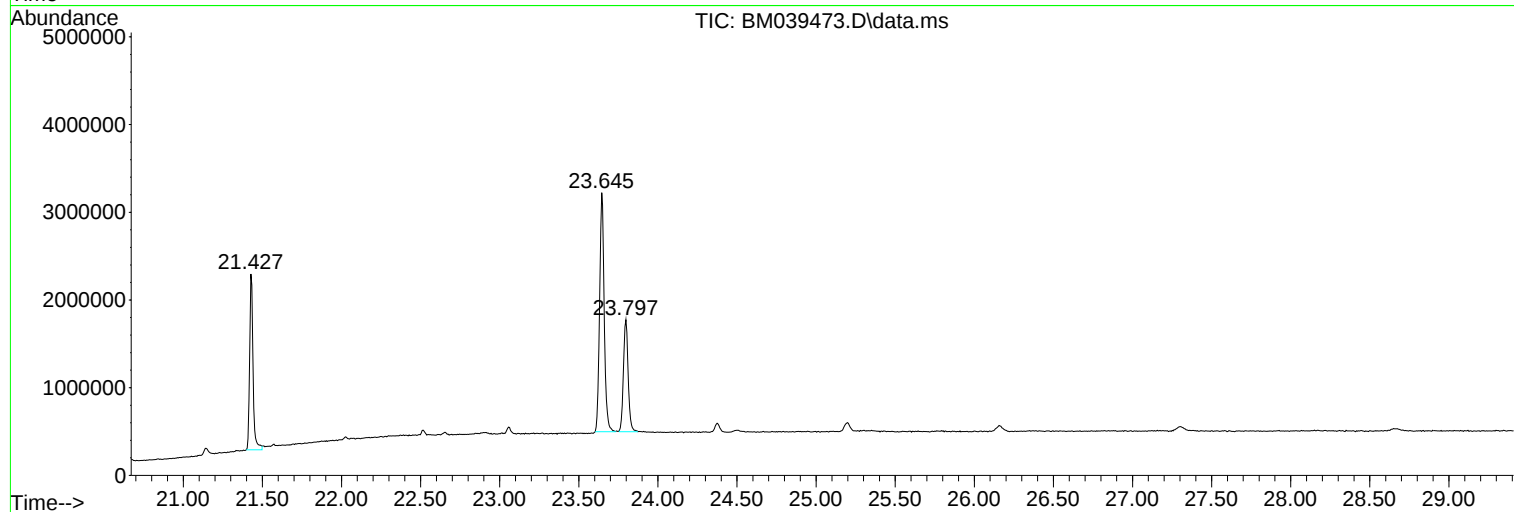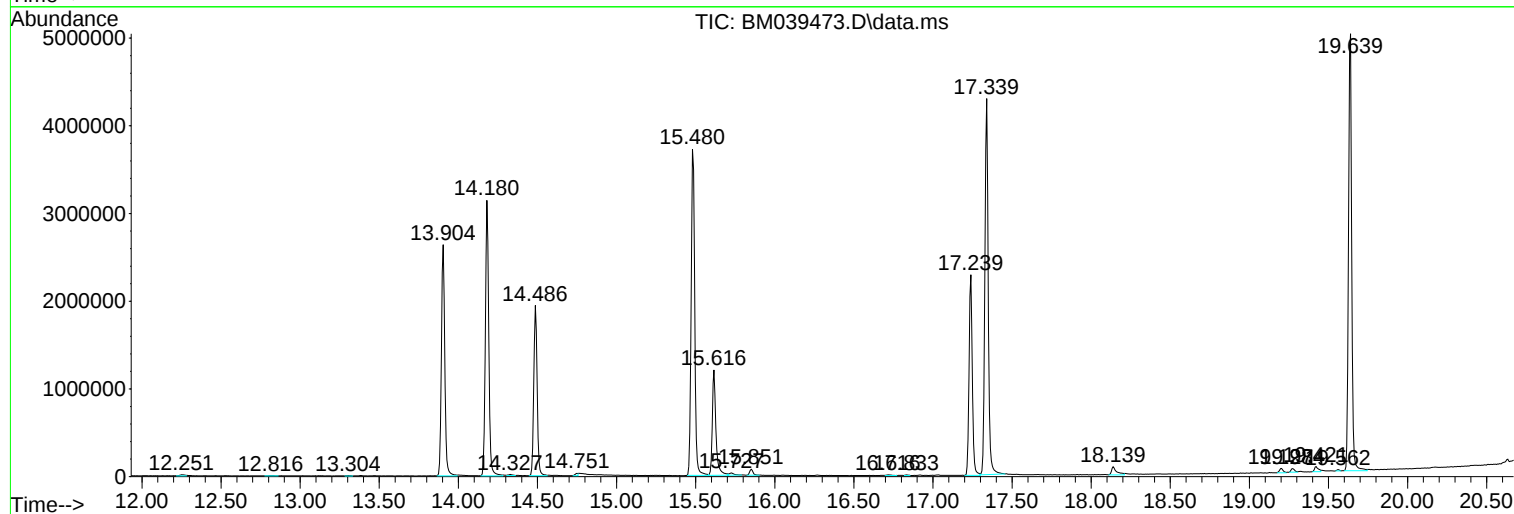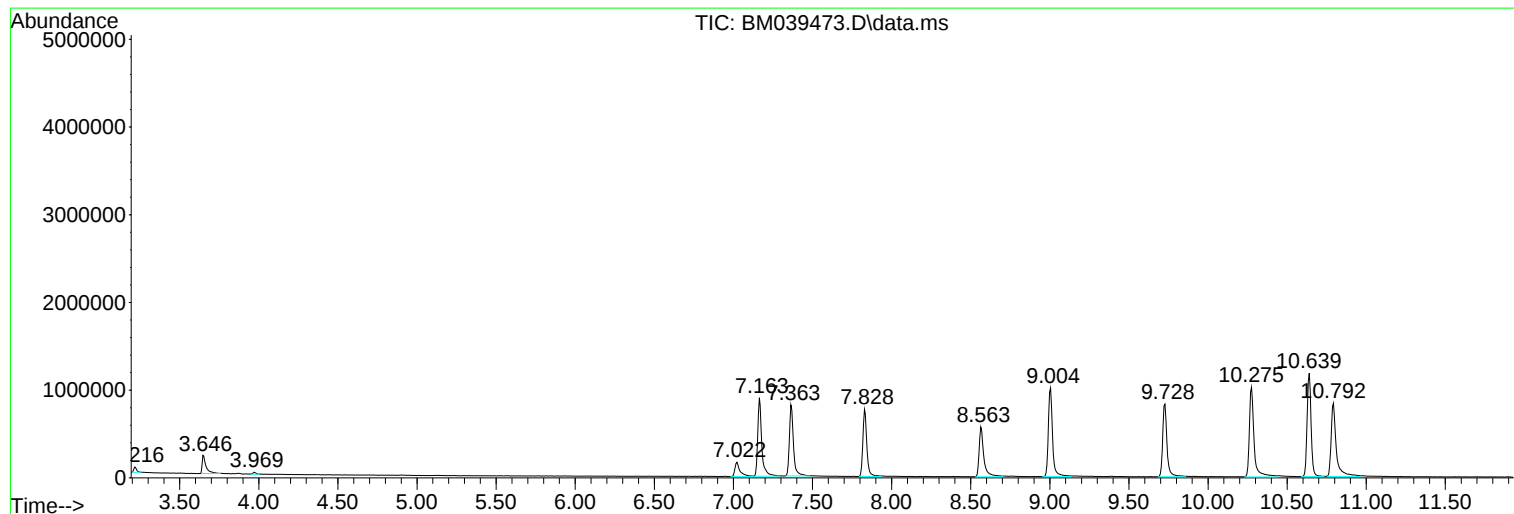

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039473.D
Acq On : 19 Apr 2023 01:04
Operator : CG/JU
Sample : 02335-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039473.D
Acq On : 19 Apr 2023 01:04
Operator : CG/JU
Sample : 02335-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc