

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039477.D
 Acq On : 19 Apr 2023 03:28
 Operator : CG/JU
 Sample : 02335-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	11	rVB	67052	78948	0.93%	0.107%
2	3.646	75	78	97	rBV	209896	378945	4.45%	0.512%
3	3.969	130	133	142	rVB	20202	27595	0.32%	0.037%
4	7.022	646	652	669	rBV	199301	444579	5.22%	0.601%
5	7.163	670	676	698	rVV	1040693	1750568	20.56%	2.366%
6	7.363	703	710	731	rVV	953753	1687827	19.82%	2.281%
7	7.828	782	789	808	rBV	798040	1410435	16.57%	1.906%
8	8.563	907	914	930	rBV	687344	1331172	15.64%	1.799%
9	9.004	981	989	1011	rBV	1206731	2188670	25.71%	2.958%
10	9.728	1104	1112	1137	rBV	958218	1815722	21.33%	2.454%
11	10.275	1198	1205	1232	rBV	1182451	2391957	28.10%	3.233%
12	10.639	1257	1267	1284	rBV	1249657	2177018	25.57%	2.943%
13	10.786	1285	1292	1322	rBV	935821	2069312	24.31%	2.797%
14	12.251	1534	1541	1553	rBV2	13059	35913	0.42%	0.049%
15	13.457	1741	1746	1751	rBV5	4204	9071	0.11%	0.012%
16	13.904	1814	1822	1839	rBV	3121963	4452977	52.30%	6.019%
17	14.180	1861	1869	1888	rBV	3583870	5366093	63.03%	7.253%
18	14.486	1914	1921	1934	rBV	2124404	3062564	35.97%	4.140%
19	14.751	1959	1966	1979	rBV3	40418	170616	2.00%	0.231%
20	15.480	2082	2090	2107	rBV	4328758	6546286	76.89%	8.849%
21	15.615	2107	2113	2128	rVV	1490595	2252907	26.46%	3.045%
22	15.721	2128	2131	2139	rVB4	23143	42326	0.50%	0.057%
23	15.851	2148	2153	2166	rVB	74439	116518	1.37%	0.157%
24	16.268	2221	2224	2231	rVB7	6639	9467	0.11%	0.013%
25	16.415	2245	2249	2256	rVB4	11070	17934	0.21%	0.024%
26	16.915	2331	2334	2339	rVB6	8155	10173	0.12%	0.014%
27	17.033	2351	2354	2361	rVB7	5579	10344	0.12%	0.014%
28	17.239	2382	2389	2400	rBV	2477855	3619948	42.52%	4.893%
29	17.339	2400	2406	2429	rVB	4924785	7287407	85.60%	9.850%
30	18.139	2538	2542	2552	rBV4	43561	95074	1.12%	0.129%
31	19.197	2718	2722	2730	rBV	60282	92533	1.09%	0.125%
32	19.274	2731	2735	2741	rBV	53852	76872	0.90%	0.104%
33	19.421	2756	2760	2768	rBV3	39658	85193	1.00%	0.115%
34	19.562	2781	2784	2788	rVB5	16564	20913	0.25%	0.028%
35	19.639	2790	2797	2816	rBV	5976678	8513754	100.00%	11.508%
36	21.139	3049	3052	3060	rBV6	56672	104295	1.23%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039477.D
Acq On : 19 Apr 2023 03:28
Operator : CG/JU
Sample : 02335-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	21.427	3096	3101	3113	rBV	2609222	3680323	43.23%	4.975%
38	23.644	3470	3478	3495	rBV	3563266	7303749	85.79%	9.872%
39	23.791	3497	3503	3515	rVB2	1563835	3244816	38.11%	4.386%




Sum of corrected areas: 73980814

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039477.D
Acq On : 19 Apr 2023 03:28
Operator : CG/JU
Sample : 02335-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

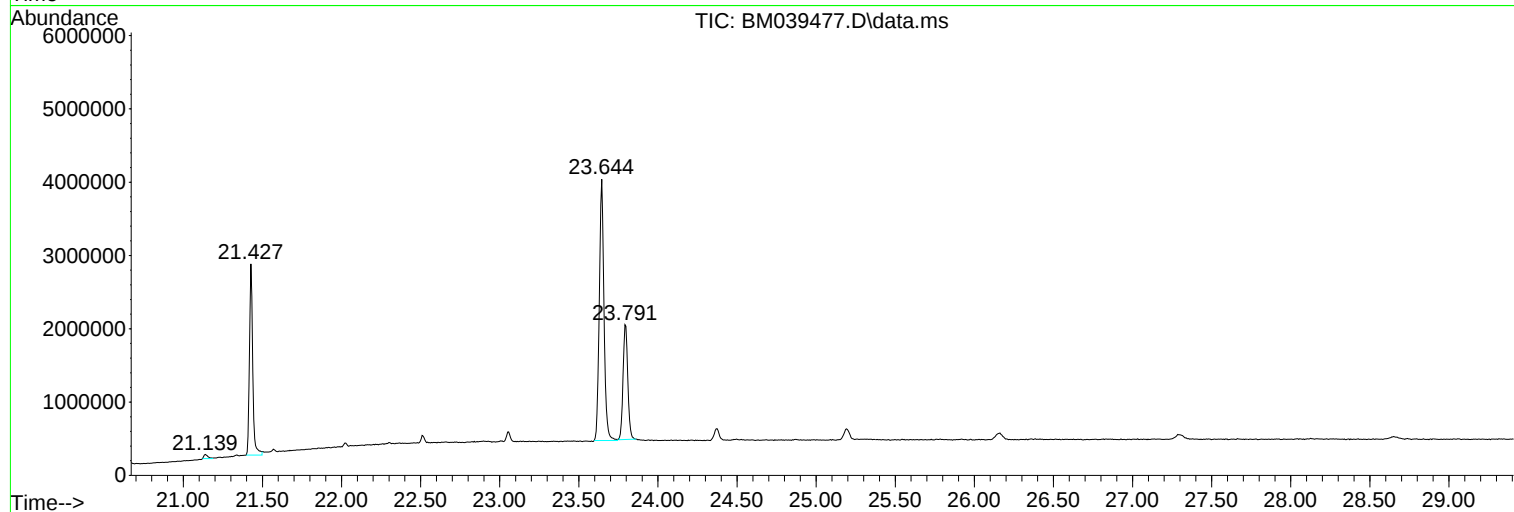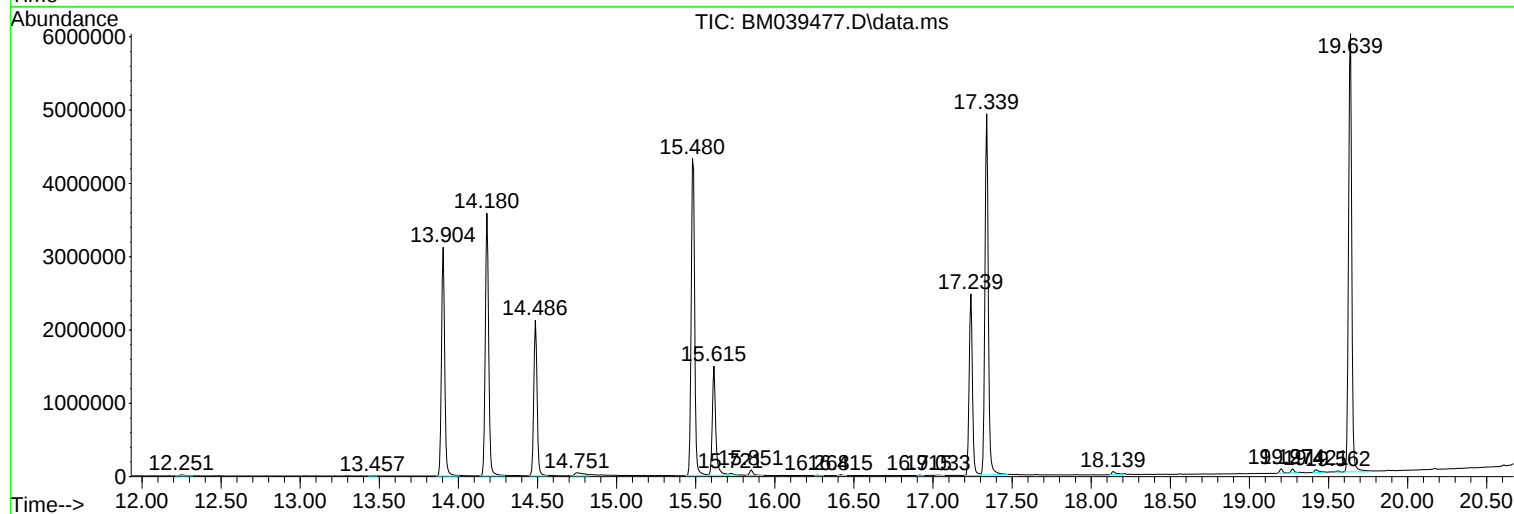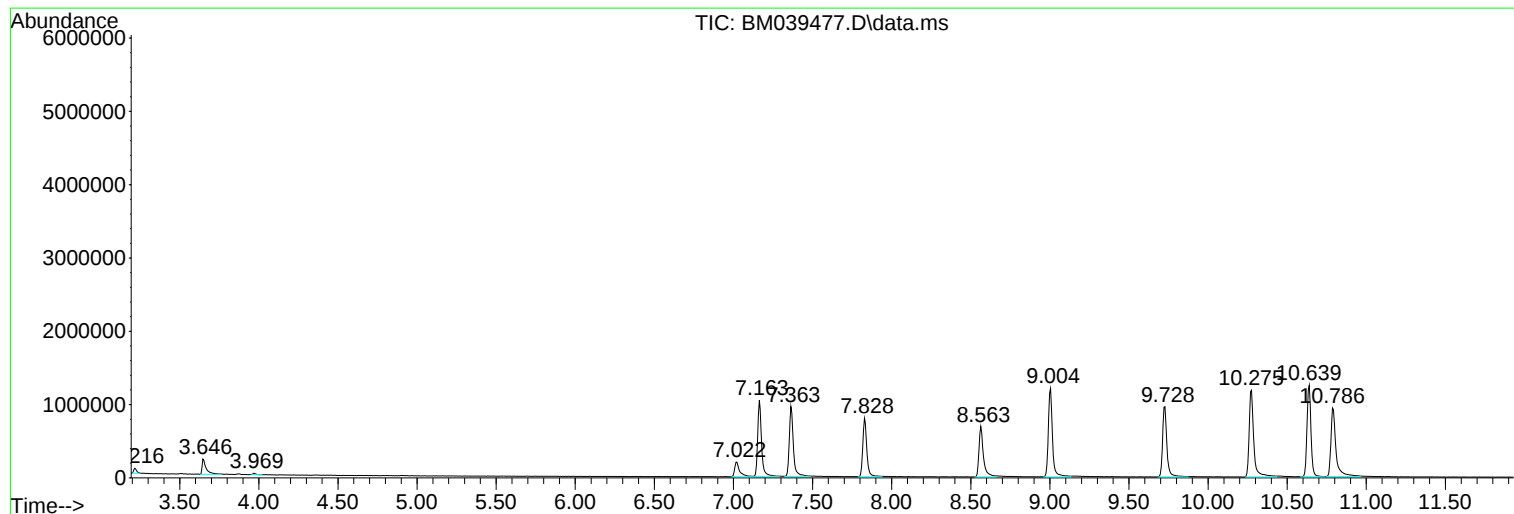

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039477.D
Acq On : 19 Apr 2023 03:28
Operator : CG/JU
Sample : 02335-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039477.D
Acq On : 19 Apr 2023 03:28
Operator : CG/JU
Sample : 02335-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------