

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039478.D
 Acq On : 19 Apr 2023 04:04
 Operator : CG/JU
 Sample : 02335-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	15	rVB	62192	74165	0.88%	0.103%
2	3.646	76	78	94	rBV	265052	452339	5.38%	0.628%
3	3.969	130	133	139	rVB2	19055	27154	0.32%	0.038%
4	7.016	646	651	670	rBV	196503	430544	5.12%	0.598%
5	7.163	670	676	691	rBV	1008391	1684737	20.02%	2.340%
6	7.363	703	710	734	rBV	936973	1633266	19.41%	2.268%
7	7.722	767	771	778	rVB7	7313	14731	0.18%	0.020%
8	7.828	782	789	810	rBV	769524	1504175	17.88%	2.089%
9	8.187	843	850	862	rBV2	20826	44059	0.52%	0.061%
10	8.563	908	914	933	rBV	675846	1324310	15.74%	1.839%
11	9.004	981	989	1009	rBV	1144879	2131860	25.34%	2.961%
12	9.722	1104	1111	1130	rBV	935273	1758804	20.90%	2.442%
13	10.269	1197	1204	1229	rBV	1172882	2351130	27.94%	3.265%
14	10.498	1239	1243	1249	rVB7	10042	17962	0.21%	0.025%
15	10.639	1259	1267	1284	rVB	1178339	2064890	24.54%	2.868%
16	10.786	1285	1292	1314	rBV	1012424	2152652	25.58%	2.989%
17	12.251	1535	1541	1553	rBV3	12870	34953	0.42%	0.049%
18	13.304	1716	1720	1727	rBV5	22949	38730	0.46%	0.054%
19	13.510	1750	1755	1759	rBV4	6430	9712	0.12%	0.013%
20	13.904	1815	1822	1836	rBV	3160237	4527201	53.80%	6.287%
21	14.180	1860	1869	1890	rBV	3541448	5391727	64.08%	7.488%
22	14.369	1899	1901	1908	rVB6	6720	11350	0.13%	0.016%
23	14.486	1914	1921	1934	rBV	1971800	2921473	34.72%	4.057%
24	14.751	1960	1966	1970	rBV3	45715	114124	1.36%	0.158%
25	15.480	2083	2090	2107	rBV	4385949	6589802	78.31%	9.151%
26	15.616	2107	2113	2128	rVV	1481616	2289964	27.21%	3.180%
27	15.721	2128	2131	2142	rVB	27216	60923	0.72%	0.085%
28	15.851	2148	2153	2169	rVB	79717	135235	1.61%	0.188%
29	16.415	2245	2249	2255	rVB3	14879	19436	0.23%	0.027%
30	16.915	2331	2334	2339	rVB7	6037	10043	0.12%	0.014%
31	17.239	2382	2389	2399	rBV	2389487	3429361	40.75%	4.762%
32	17.339	2399	2406	2425	rVB	4812363	7208107	85.66%	10.010%
33	18.139	2538	2542	2547	rBV2	39267	70141	0.83%	0.097%
34	19.198	2718	2722	2728	rBV2	59508	87065	1.03%	0.121%
35	19.274	2731	2735	2739	rBV	50864	71071	0.84%	0.099%
36	19.421	2756	2760	2768	rBV5	30962	68556	0.81%	0.095%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039478.D
Acq On : 19 Apr 2023 04:04
Operator : CG/JU
Sample : 02335-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.556	2781	2783	2788	rVB3	14641	17661	0.21%	0.025%
38	19.639	2790	2797	2813	rBV	5908665	8414679	100.00%	11.685%
39	21.427	3096	3101	3115	rBV	2332477	3309581	39.33%	4.596%
40	23.644	3471	3478	3493	rVB2	3252922	6739127	80.09%	9.359%
41	23.791	3497	3503	3513	rVB2	1332383	2772827	32.95%	3.851%




Sum of corrected areas: 72009627

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039478.D
Acq On : 19 Apr 2023 04:04
Operator : CG/JU
Sample : 02335-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

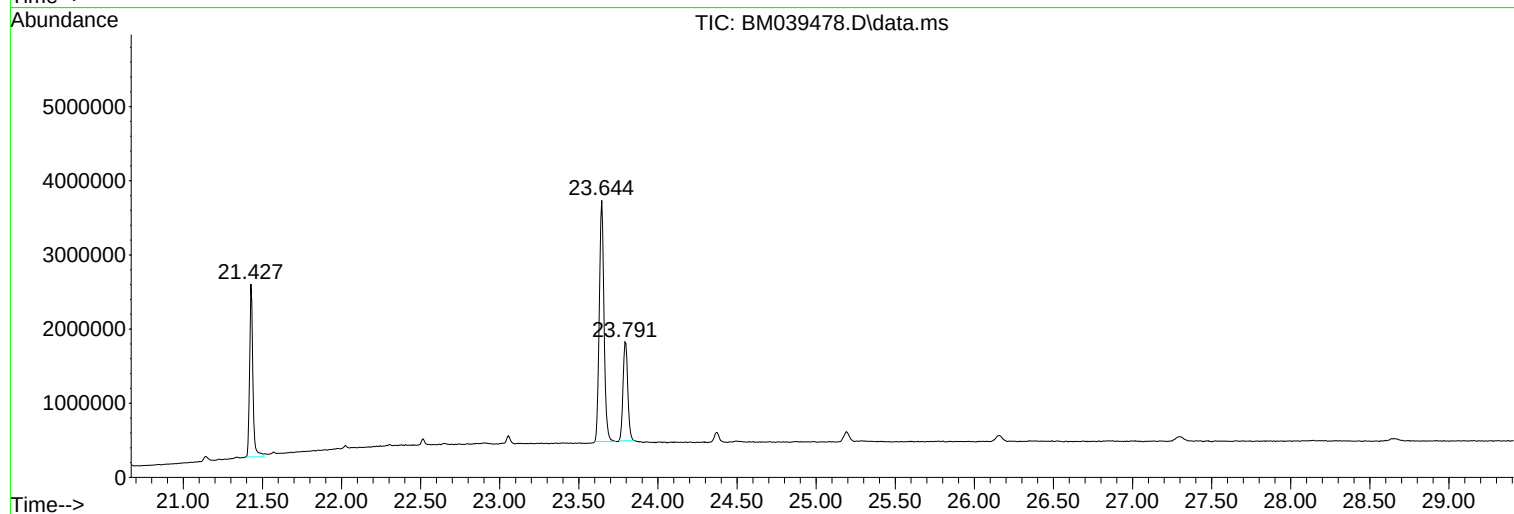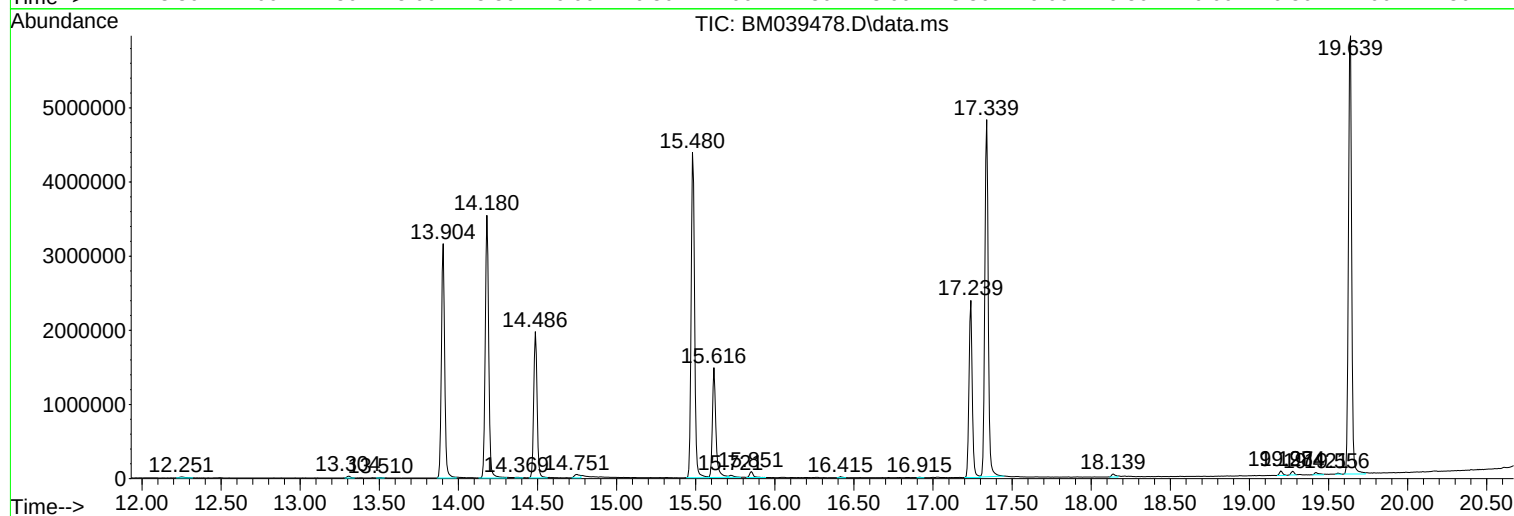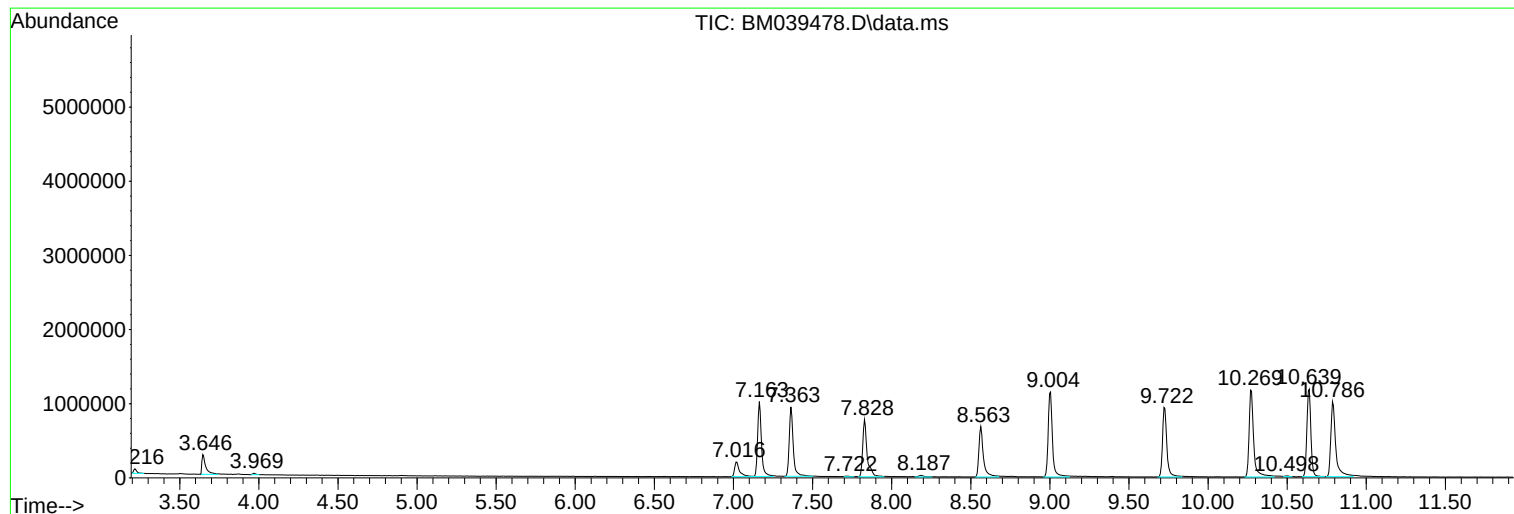

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039478.D
Acq On : 19 Apr 2023 04:04
Operator : CG/JU
Sample : 02335-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039478.D
Acq On : 19 Apr 2023 04:04
Operator : CG/JU
Sample : 02335-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc